

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060722\
Data File : VW023408.D
Acq On : 07 Jun 2022 09:38
Operator : SY/VA
Sample : VW0607SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1




Instrument :
MSVOA_W
ClientSampleId :
VBLK524

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/08/2022
Supervised By :Mahesh Dadoda 06/08/2022

Supervised By :Mahesh
Dadoda
06/08/2022

Quant Time: Jun 08 01:21:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060622SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 08 01:20:30 2022
Response via : Initial Calibration

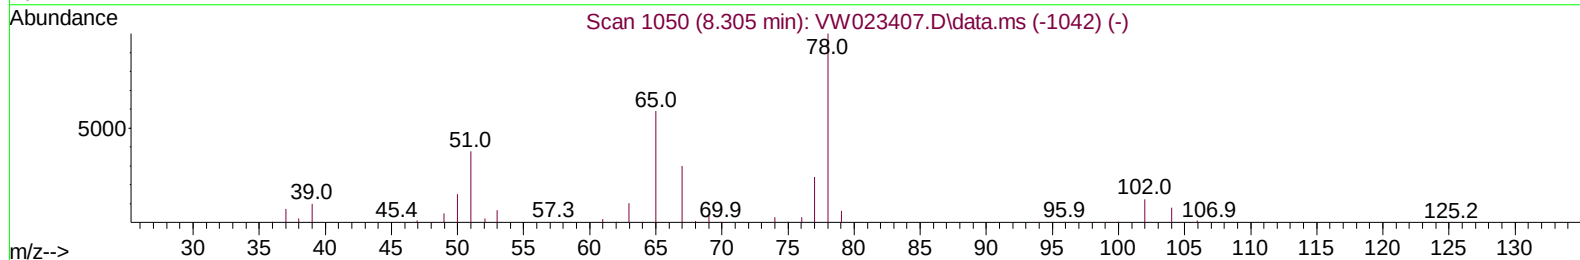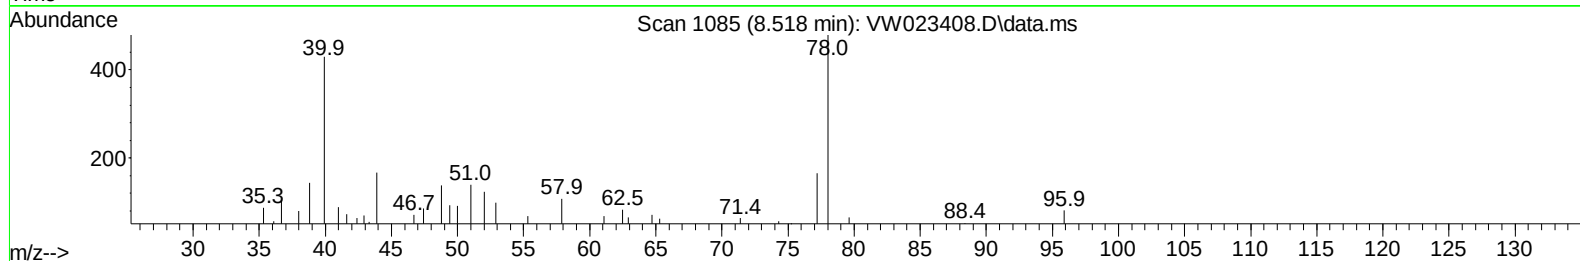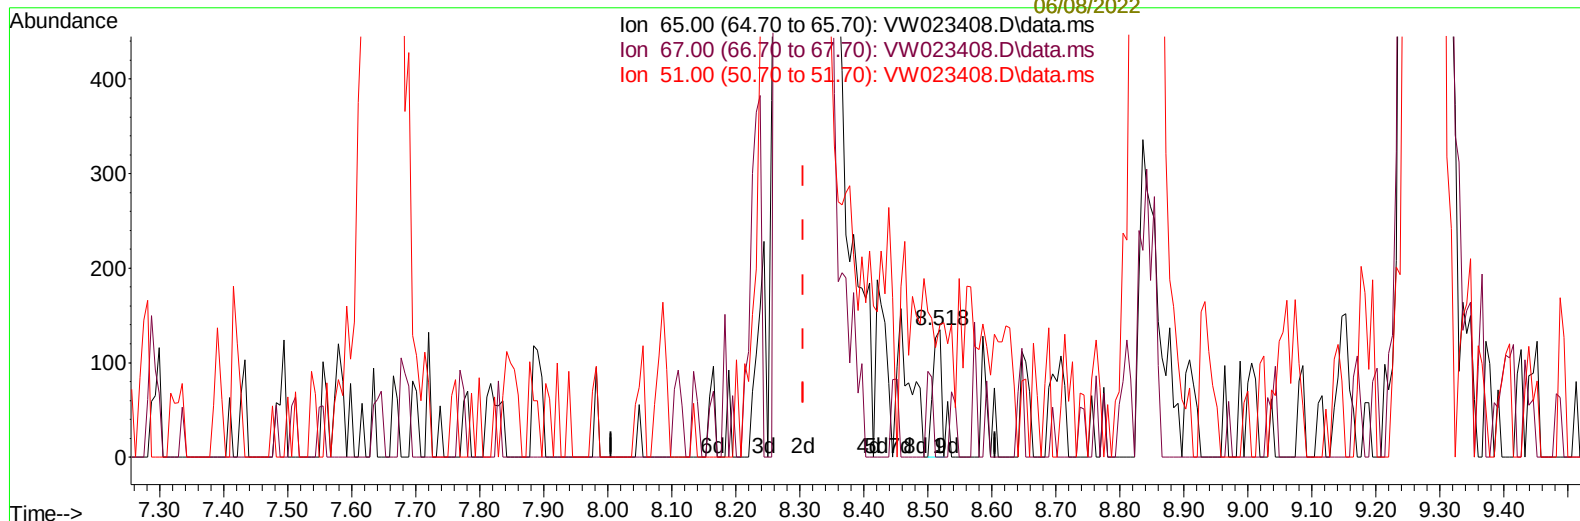

TIC: VW023408.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.518min (+ 0.213) 0.02 ug/L

response 118

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.10	54.24
51.00	92.30	116.95
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060722\
 Data File : VW023408.D
 Acq On : 07 Jun 2022 09:38
 Operator : SY/VA
 Sample : VW0607SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK524

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/08/2022
 Supervised By :Mahesh Dadoda 06/08/2022

Supervised By :Mahesh
 Dadoda
 06/08/2022

Quant Time: Jun 08 01:21:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 08 01:20:30 2022
 Response via : Initial Calibration

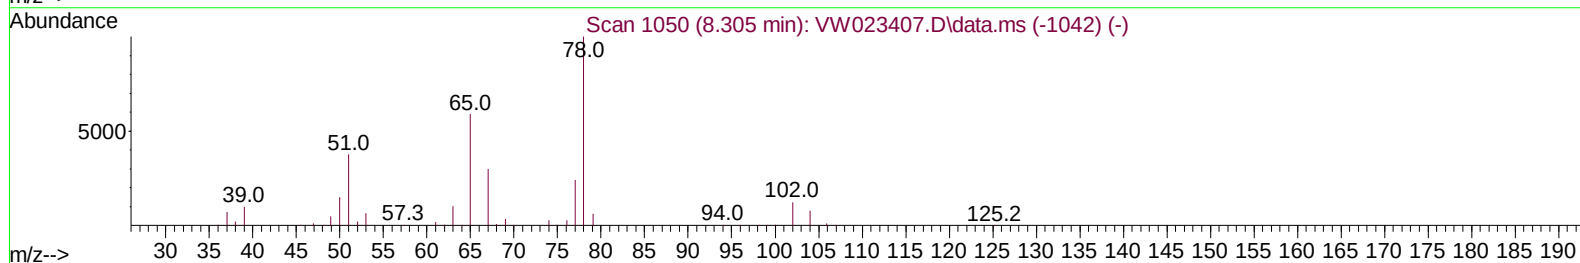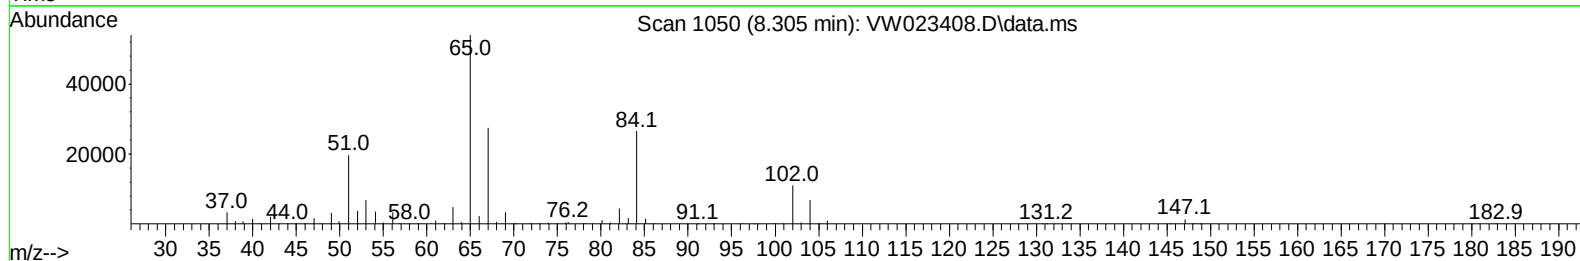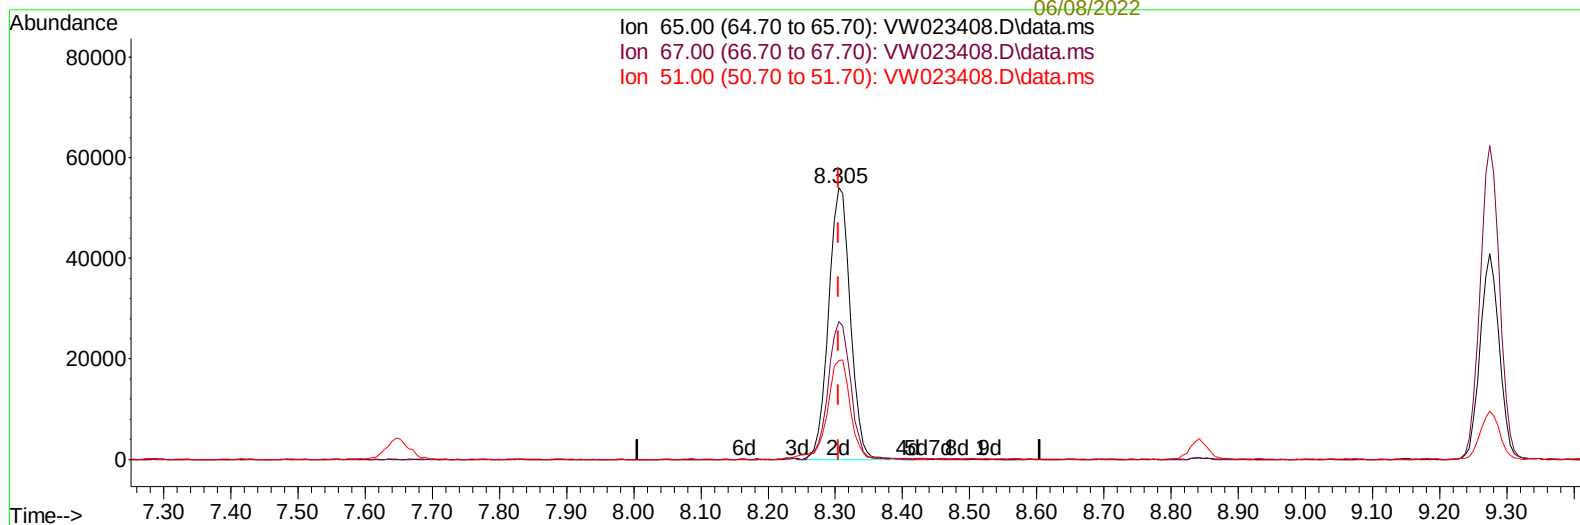

TIC: VW023408.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (-0.000) 23.53 ug/L m

response 121754

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.10	0.05#
51.00	92.30	0.11#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060722\
 Data File : VW023408.D
 Acq On : 07 Jun 2022 09:38
 Operator : SY/VA
 Sample : VW0607SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK524

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/08/2022
 Supervised By :Mahesh Dadoda 06/08/2022

Supervised By :Mahesh
 Dadoda
 06/08/2022

Quant Time: Jun 08 01:21:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 08 01:20:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	365359	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	339627	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	152225	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	131646	23.278	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	93.120%	
7) Chloroethane-d5	2.891	69	95633	24.004	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	96.000%	
11) 1,1-Dichloroethene-d2	4.019	63	151762	17.869	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	71.480%	
21) 2-Butanone-d5	7.080	46	48785	44.728	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	89.460%	
24) Chloroform-d	7.647	84	224761	22.814	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	91.240%	
26) 1,2-Dichloroethane-d4	8.305	65	121754m	23.526	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	94.120%	
32) Benzene-d6	8.275	84	443453	23.522	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	94.080%	
36) 1,2-Dichloropropane-d6	9.274	67	125941	23.834	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	95.320%	
41) Toluene-d8	10.323	98	419248	23.350	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	93.400%	
43) trans-1,3-Dichloroprop...	10.579	79	50914	21.596	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	86.400%	
47) 2-Hexanone-d5	10.927	63	34845	44.053	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	88.100%	
56) 1,1,2,2-Tetrachloroeth...	12.694	84	99104	21.920	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	87.680%	
66) 1,2-Dichlorobenzene-d4	13.853	152	134569	24.424	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	97.680%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060722\
Data File : VW023408.D
Acq On : 07 Jun 2022 09:38
Operator : SY/VA
Sample : VW0607SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK524

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/08/2022
Supervised By :Mahesh Dadoda 06/08/2022

Supervised By :Mahesh
Dadoda
06/08/2022

Quant Time: Jun 08 01:21:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060622SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 08 01:20:30 2022
Response via : Initial Calibration

