




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060722\
 Data File : VW023409.D
 Acq On : 07 Jun 2022 13:03
 Operator : SY/VA
 Sample : N3226-01
 Misc : 4.61g/10mL/MSVOA_W/SoIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4L2

Manual IntegrationsAPPROVED

Quant Time: Jun 08 01:21:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 08 01:20:30 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/08/2022
 Supervised By :Mahesh Dadoda 06/08/2022

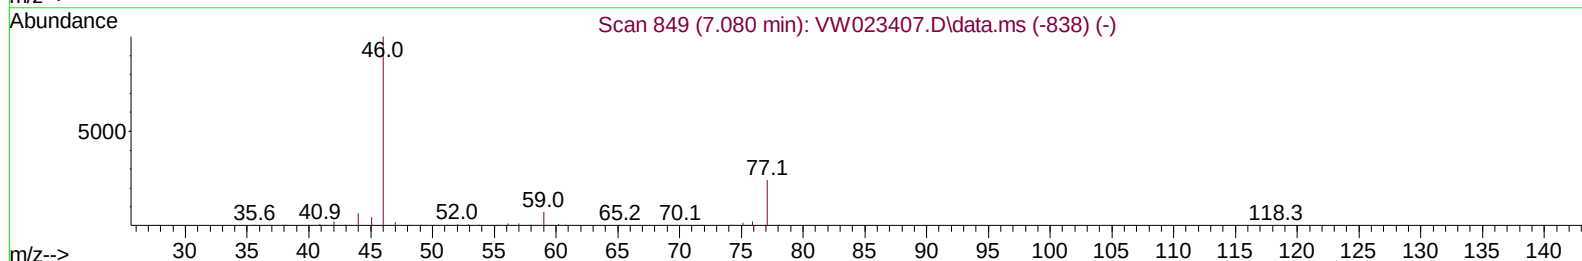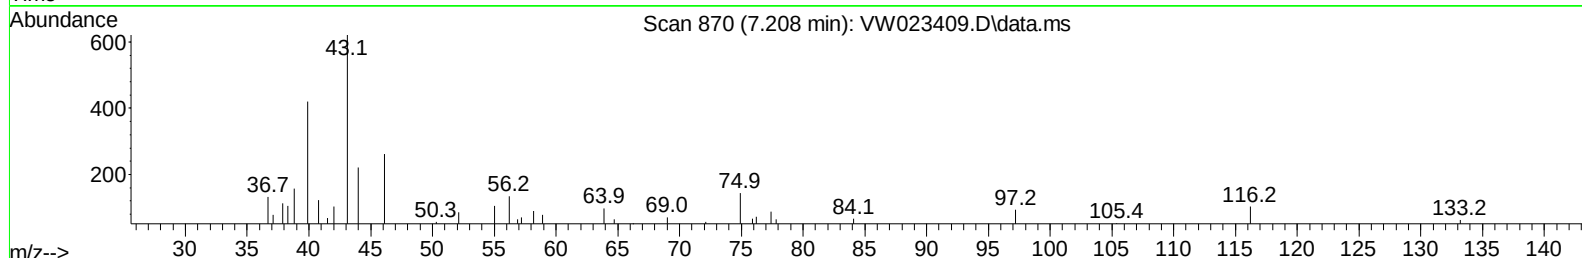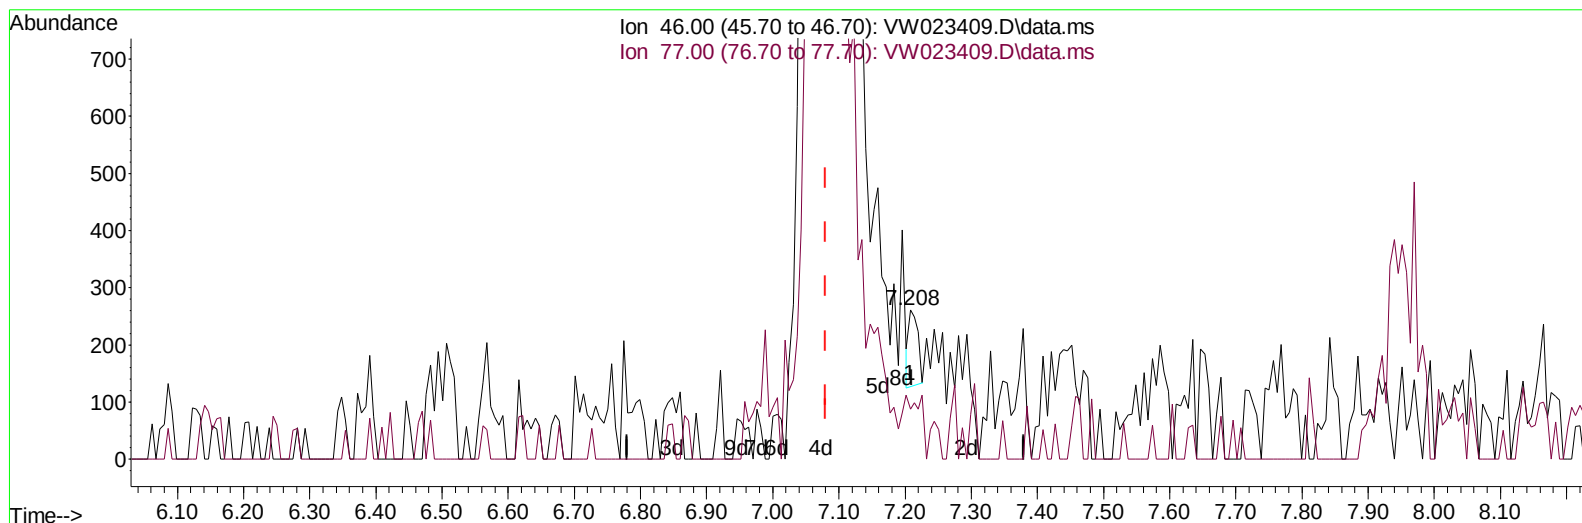

TIC: VW023409.D\data.ms

(21) 2-Butanone-d5 (S)

7.208min (+ 0.128) 0.10 ug/L

response 128

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.90	32.03
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060722\
 Data File : VW023409.D
 Acq On : 07 Jun 2022 13:03
 Operator : SY/VA
 Sample : N3226-01
 Misc : 4.61g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4L2

Manual IntegrationsAPPROVED

Quant Time: Jun 08 01:21:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 08 01:20:30 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/08/2022
 Supervised By :Mahesh Dadoda 06/08/2022

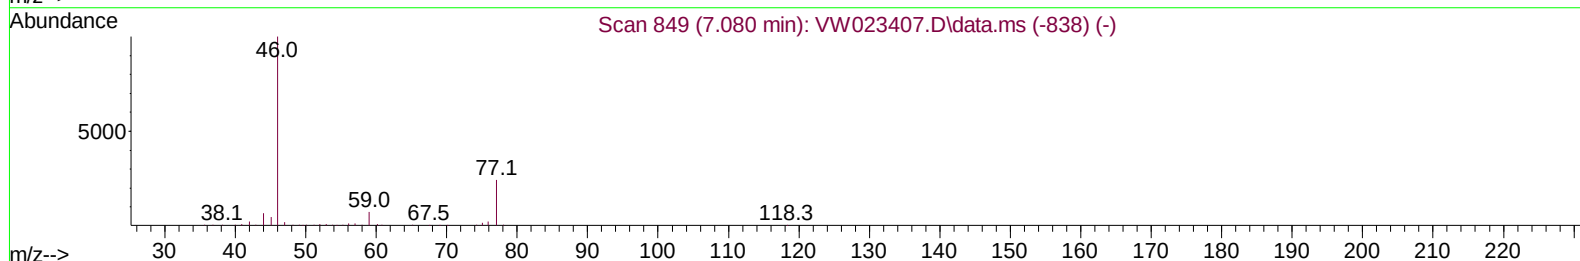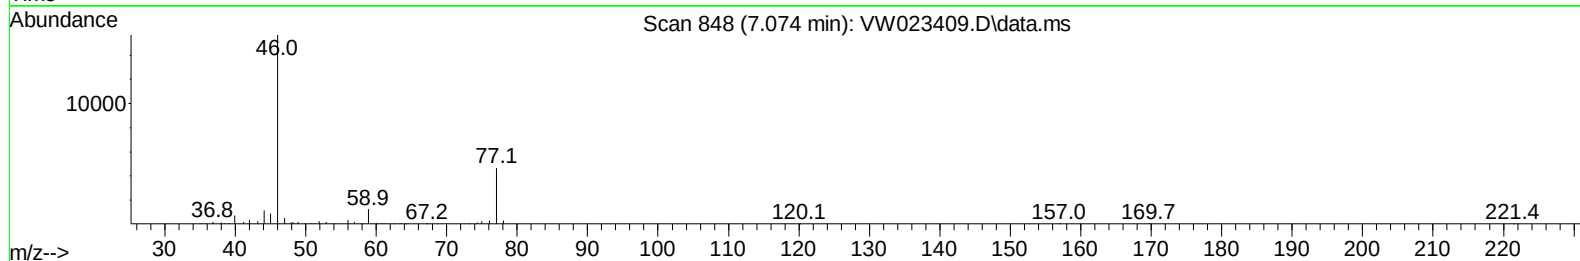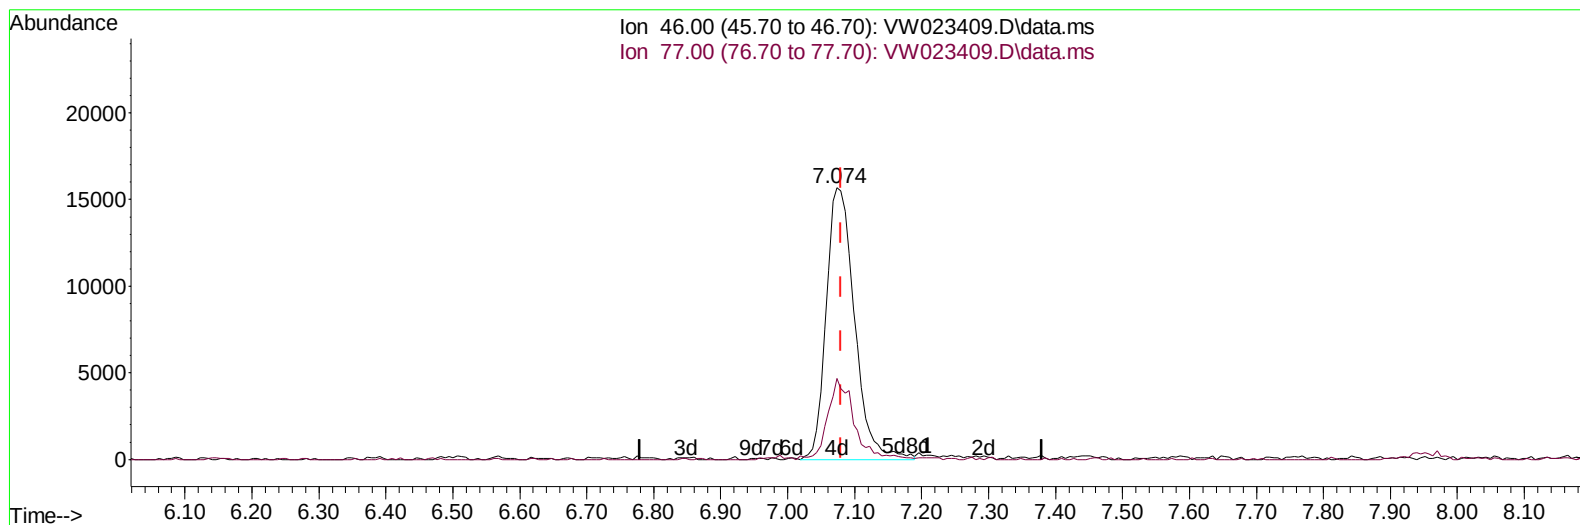

TIC: VW023409.D\data.ms

(21) 2-Butanone-d5 (S)

7.074min (-0.006) 36.95 ug/L m

response 46009

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.90	0.09#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060722\
 Data File : VW023409.D
 Acq On : 07 Jun 2022 13:03
 Operator : SY/VA
 Sample : N3226-01
 Misc : 4.61g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4L2

Manual IntegrationsAPPROVED

Quant Time: Jun 08 01:21:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 08 01:20:30 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/08/2022
 Supervised By :Mahesh Dadoda 06/08/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	417142	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	340733	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	101010	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	141234	21.873	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	87.480%	
7) Chloroethane-d5	2.885	69	95049	20.896	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	83.600%	
11) 1,1-Dichloroethene-d2	4.013	63	159953	16.496	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110	Recovery	=	66.000%	
21) 2-Butanone-d5	7.074	46	46009m	36.946	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	73.900%	
24) Chloroform-d	7.647	84	259941	23.110	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	92.440%	
26) 1,2-Dichloroethane-d4	8.305	65	139022	23.528	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	94.120%	
32) Benzene-d6	8.268	84	495837	26.215	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	104.840%	
36) 1,2-Dichloropropane-d6	9.274	67	142768	26.930	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	107.720%	
41) Toluene-d8	10.323	98	436332	24.222	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	96.880%	
43) trans-1,3-Dichloroprop...	10.579	79	53619	22.670	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	90.680%	
47) 2-Hexanone-d5	10.920	63	35157	44.304	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	88.600%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	102484	22.594	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	90.360%	
66) 1,2-Dichlorobenzene-d4	13.853	152	84477	23.106	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	92.440%	
Target Compounds						
						Qvalue
13) Acetone	4.129	43	5414	5.796	ug/L	74
29) Cyclohexane	7.958	56	21012	2.886	ug/L	93
42) Toluene	10.384	91	54953	2.437	ug/L	99
52) Ethylbenzene	11.731	91	11468	0.462	ug/L	91
53) m,p-Xylene	11.835	106	17172	1.786	ug/L	90
54) o-Xylene	12.164	106	6525	0.708	ug/L	84
63) 1,2,4-Trimethylbenzene	13.249	105	10049	0.849	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060722\
Data File : VW023409.D
Acq On : 07 Jun 2022 13:03
Operator : SY/VA
Sample : N3226-01
Misc : 4.61g/10mL/MSVOA_W/soil
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW4L2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/08/2022
Supervised By :Mahesh Dadoda 06/08/2022

Quant Time: Jun 08 01:21:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060622SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 08 01:20:30 2022
Response via : Initial Calibration

