




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060722\
 Data File : VW023418.D
 Acq On : 07 Jun 2022 17:40
 Operator : SY/VA
 Sample : N3226-05
 Misc : 6.05g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4L6

Manual IntegrationsAPPROVED

Quant Time: Jun 08 01:23:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 08 01:20:30 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/08/2022
 Supervised By :Mahesh Dadoda 06/08/2022

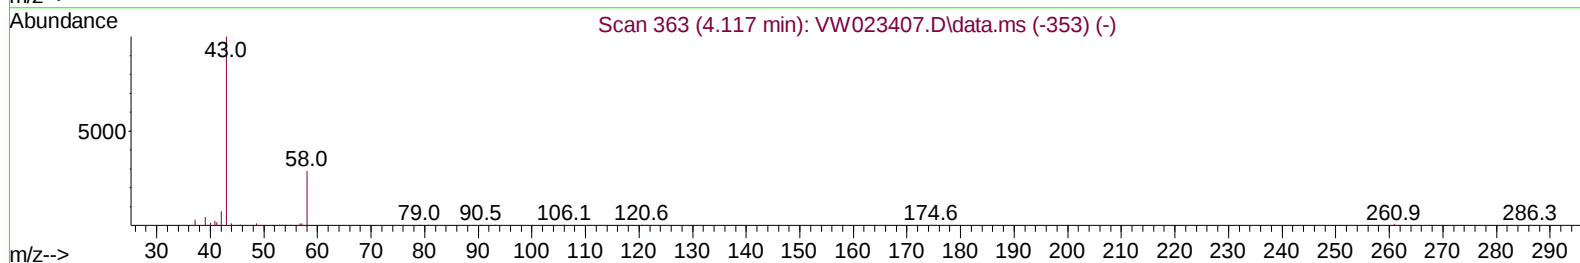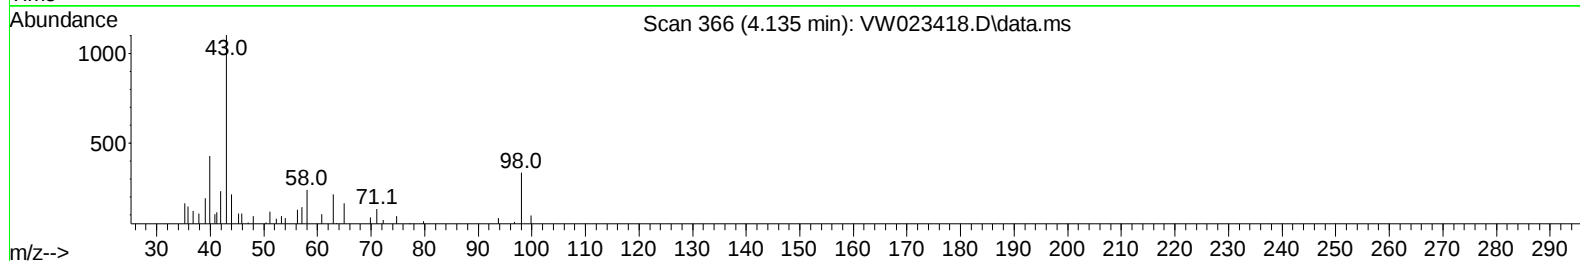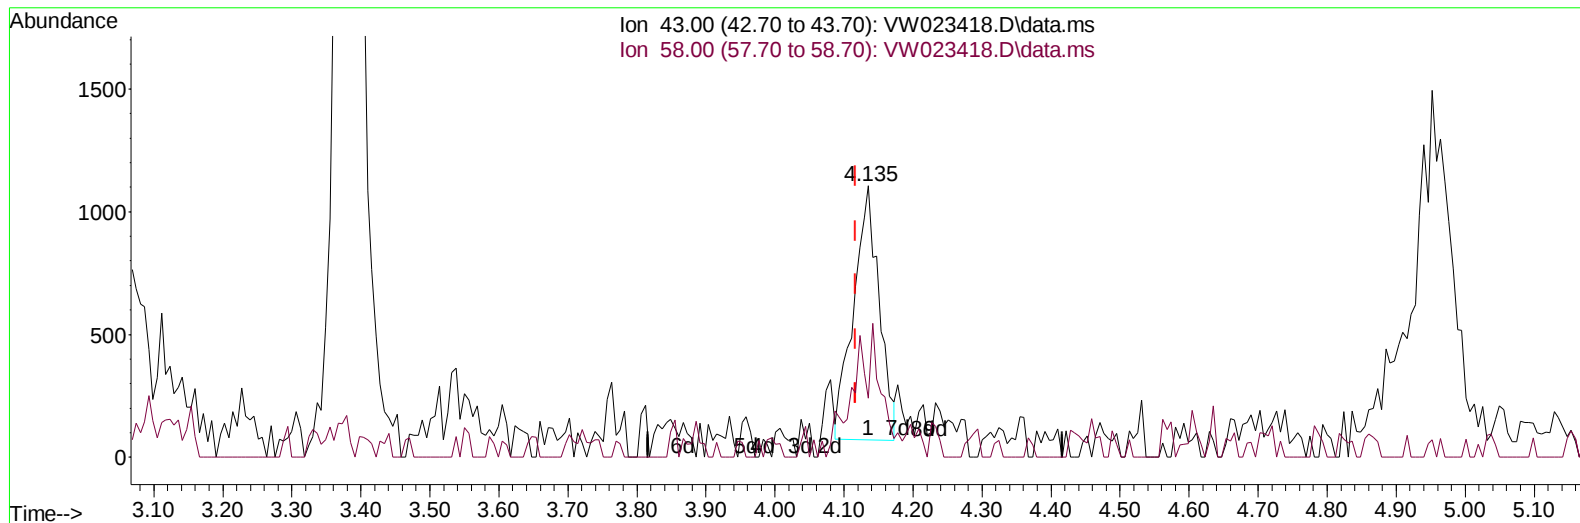

TIC: VW023418.D\data.ms

(13) Acetone (T)

4.135min (+ 0.018) 3.46 ug/L

response 2675

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	23.93
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060722\
 Data File : VW023418.D
 Acq On : 07 Jun 2022 17:40
 Operator : SY/VA
 Sample : N3226-05
 Misc : 6.05g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4L6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/08/2022
 Supervised By :Mahesh Dadoda 06/08/2022

Quant Time: Jun 08 01:23:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 08 01:20:30 2022
 Response via : Initial Calibration

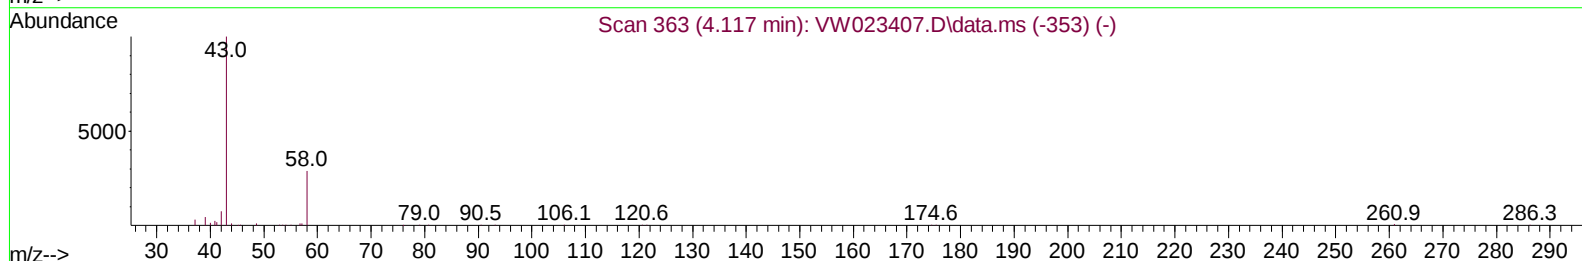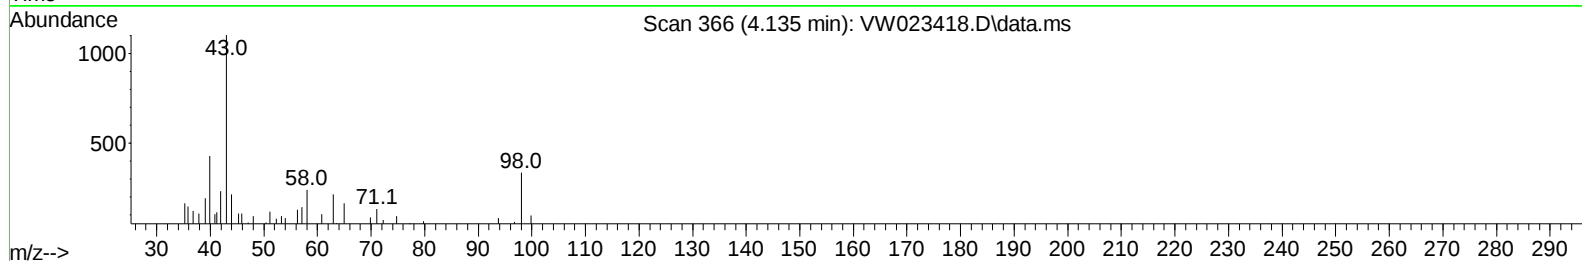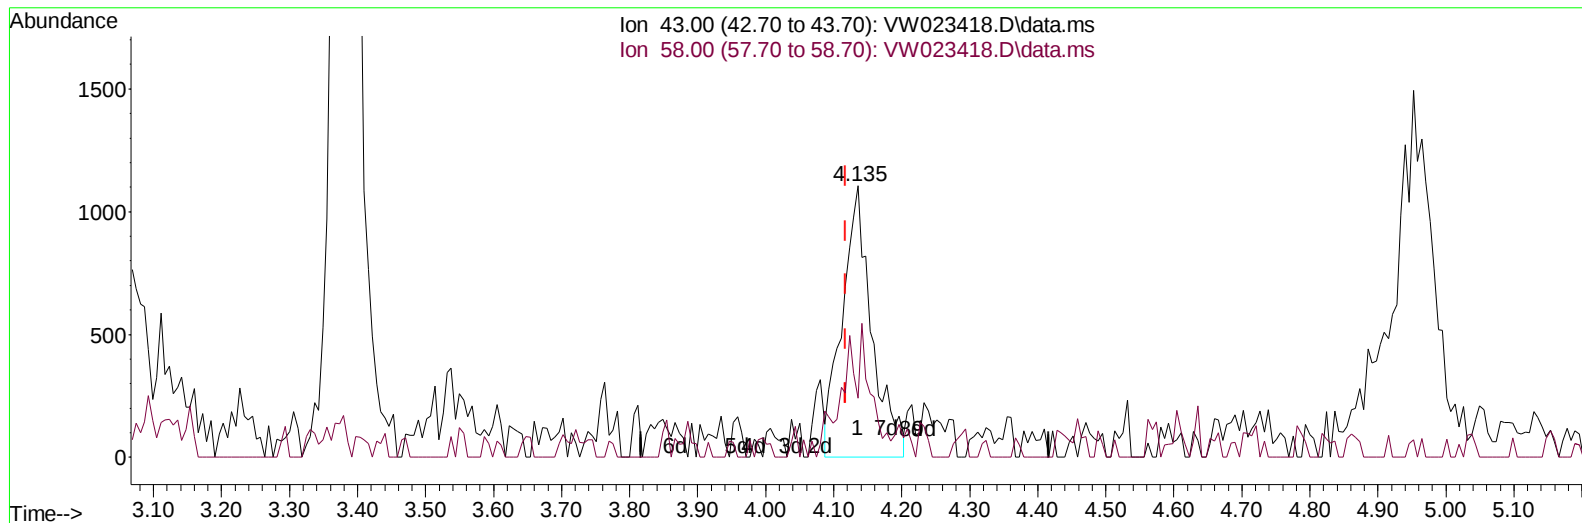

TIC: VW023418.D\data.ms

(13) Acetone (T)

4.135min (+ 0.018) 4.35 ug/L m

response 3360

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	19.05
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060722\
 Data File : VW023418.D
 Acq On : 07 Jun 2022 17:40
 Operator : SY/VA
 Sample : N3226-05
 Misc : 6.05g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4L6

Manual IntegrationsAPPROVED

Quant Time: Jun 08 01:23:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 08 01:20:30 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/08/2022
 Supervised By :Mahesh Dadoda 06/08/2022

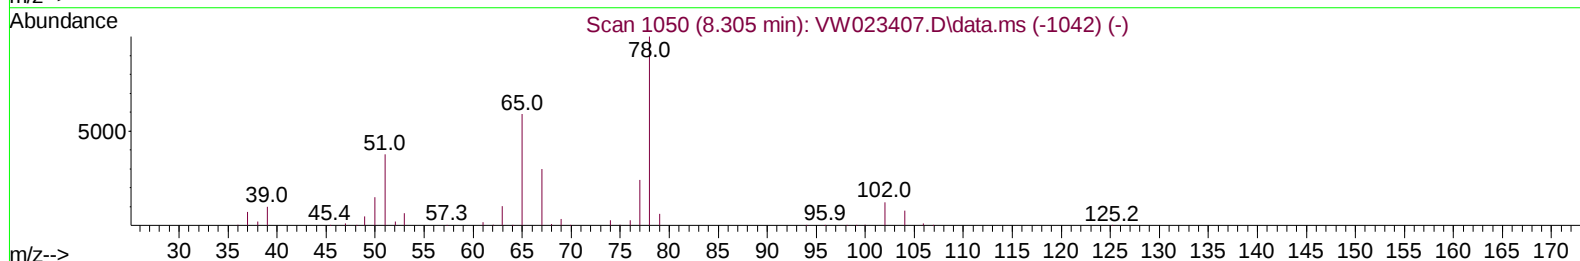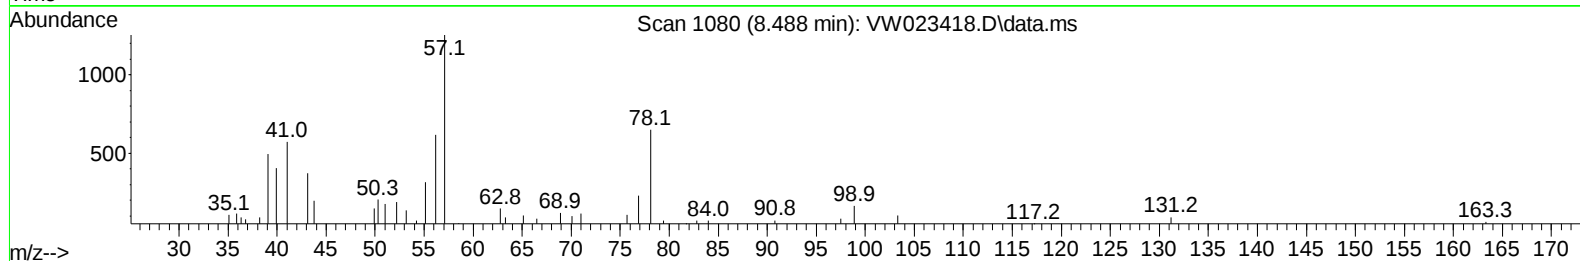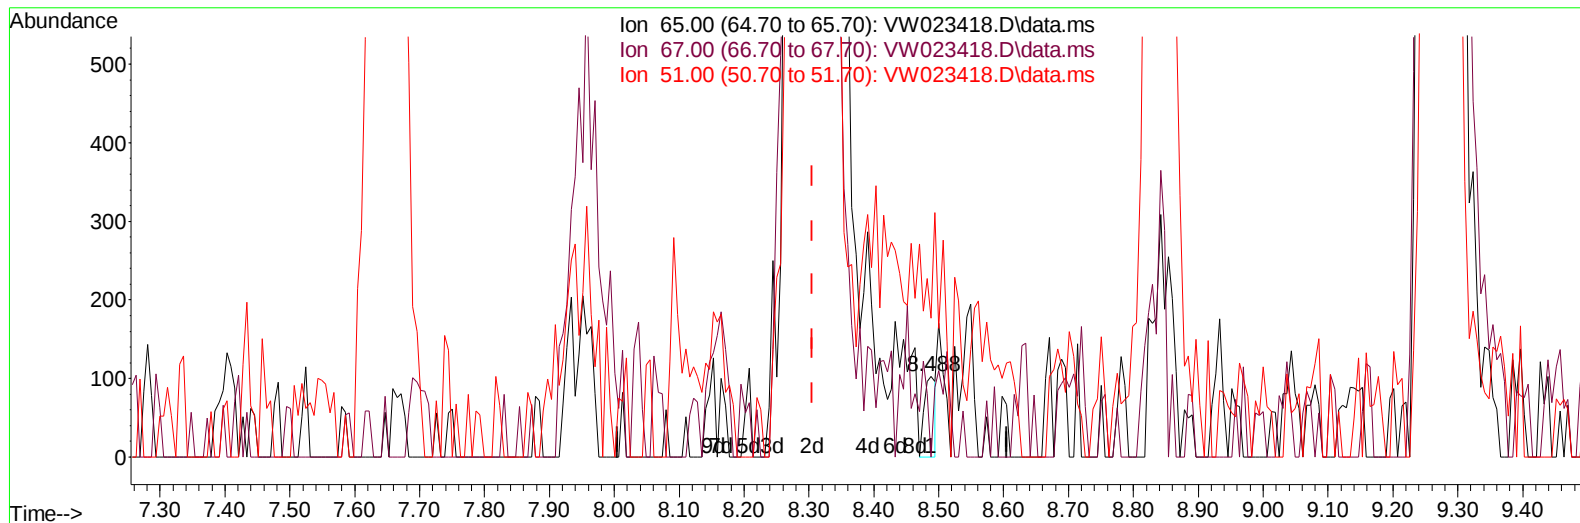

TIC: VW023418.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.488min (+ 0.183) 0.03 ug/L

response 129

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.10	57.36
51.00	92.30	79.84
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060722\
Data File : VW023418.D
Acq On : 07 Jun 2022 17:40
Operator : SY/VA
Sample : N3226-05
Misc : 6.05g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW4L6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/08/2022
Supervised By :Mahesh Dadoda 06/08/2022

Quant Time: Jun 08 01:23:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060622SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 08 01:20:30 2022
Response via : Initial Calibration

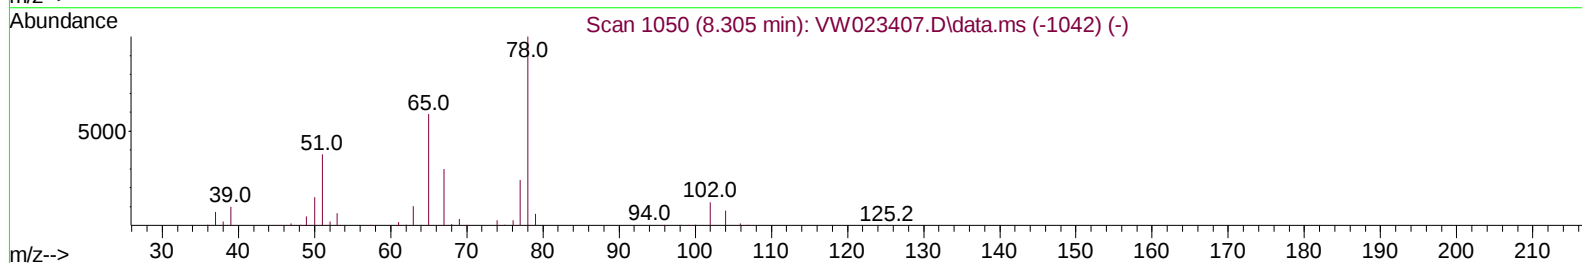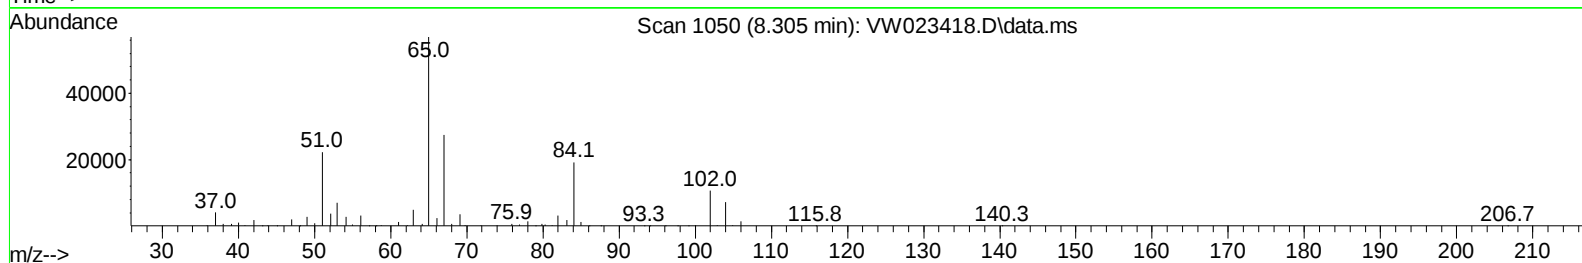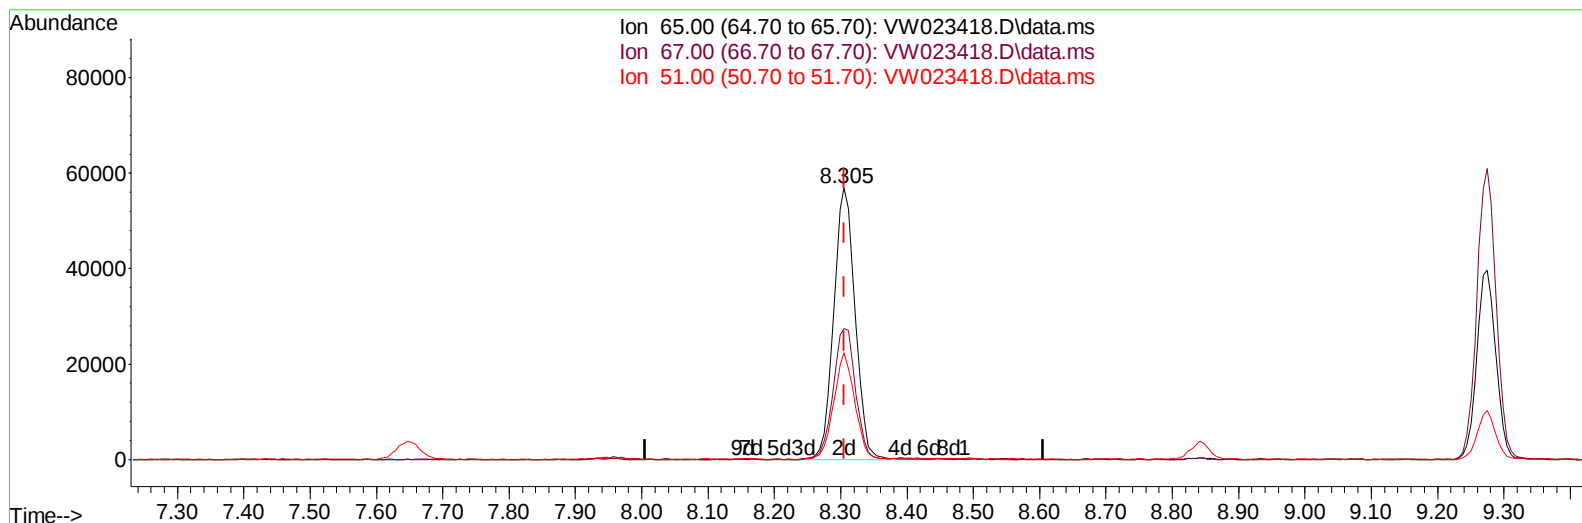

TIC: VW023418.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (+ 0.000) 25.99 ug/L m

response 126974

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.10	0.06#
51.00	92.30	0.08#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060722\
 Data File : VW023418.D
 Acq On : 07 Jun 2022 17:40
 Operator : SY/VA
 Sample : N3226-05
 Misc : 6.05g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4L6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/08/2022
 Supervised By :Mahesh Dadoda 06/08/2022

Quant Time: Jun 08 01:23:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 08 01:20:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	344930	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	316640	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	127155	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	129316	24.220	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	96.880%	
7) Chloroethane-d5	2.879	69	85568	22.750	ug/L	-0.01
Spiked Amount 25.000	Range 30	- 150	Recovery	=	91.000%	
11) 1,1-Dichloroethene-d2	4.019	63	126702	15.802	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	63.200%	
21) 2-Butanone-d5	7.074	46	56033	54.416	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	108.840%	
24) Chloroform-d	7.647	84	214060	23.015	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	92.040%	
26) 1,2-Dichloroethane-d4	8.305	65	126974m	25.988	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	103.960%	
32) Benzene-d6	8.275	84	406777	23.143	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	92.560%	
36) 1,2-Dichloropropane-d6	9.275	67	124139	25.198	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	100.800%	
41) Toluene-d8	10.323	98	376090	22.467	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	89.880%	
43) trans-1,3-Dichloroprop...	10.579	79	50456	22.956	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	91.840%	
47) 2-Hexanone-d5	10.927	63	42157	57.167	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	114.340%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	114079	27.063	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	108.240%	
66) 1,2-Dichlorobenzene-d4	13.853	152	110041	23.910	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	95.640%	
Target Compounds						
13) Acetone	4.135	43	3360m	4.350	ug/L	
29) Cyclohexane	7.952	56	6188	0.915	ug/L #	83
42) Toluene	10.390	91	20464	0.977	ug/L	93
53) m,p-Xylene	11.835	106	8772	0.982	ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060722\
Data File : VW023418.D
Acq On : 07 Jun 2022 17:40
Operator : SY/VA
Sample : N3226-05
Misc : 6.05g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW4L6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/08/2022
Supervised By :Mahesh Dadoda 06/08/2022

Quant Time: Jun 08 01:23:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060622SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 08 01:20:30 2022
Response via : Initial Calibration

