

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060722\
 Data File : VW023415.D
 Acq On : 07 Jun 2022 16:21
 Operator : SY/VA
 Sample : N3226-07
 Misc : 6.58g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4M4

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 06/08/2022
 Supervised By : Mahesh Dadoda 06/08/2022

Quant Time: Jun 08 01:22:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 08 01:20:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	219311	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	91627	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	11027	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	131271	38.669	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	154.680%#	
7) Chloroethane-d5	2.879	69	88174	36.871	ug/L	-0.01
Spiked Amount	25.000	Range 30 - 150	Recovery	=	147.480%	
11) 1,1-Dichloroethene-d2	4.019	63	107863	21.158	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery	=	84.640%	
21) 2-Butanone-d5	7.080	46	61691	94.227	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	188.460%#	
24) Chloroform-d	7.647	84	175748	29.719	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	=	118.880%	
26) 1,2-Dichloroethane-d4	8.305	65	98279	31.636	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	=	126.560%	
32) Benzene-d6	8.275	84	305742	60.111	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	=	240.440%#	
36) 1,2-Dichloropropane-d6	9.274	67	92189	64.667	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	=	258.680%#	
41) Toluene-d8	10.323	98	161510	33.342	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	=	133.360%#	
43) trans-1,3-Dichloroprop...	10.579	79	19425	30.541	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	=	122.160%	
47) 2-Hexanone-d5	10.921	63	29430	137.914	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	275.820%#	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	69303	56.816	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	=	227.280%#	
66) 1,2-Dichlorobenzene-d4	13.853	152	12821	32.123	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	=	128.480%#	
Target Compounds						
13) Acetone	4.129	43	4366	8.891	ug/L	88
29) Cyclohexane	7.958	56	6540	3.340	ug/L #	80
42) Toluene	10.390	91	15400	2.540	ug/L	91
52) Ethylbenzene	11.725	91	5638	0.844	ug/L	85
53) m,p-Xylene	11.835	106	8299	3.210	ug/L	96
54) o-Xylene	12.164	106	3747	1.513	ug/L	99
62) 1,3,5-Trimethylbenzene	12.945	105	1401m	1.073	ug/L	
63) 1,2,4-Trimethylbenzene	13.249	105	4612	3.568	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060722\
 Data File : VW023415.D
 Acq On : 07 Jun 2022 16:21
 Operator : SY/VA
 Sample : N3226-07
 Misc : 6.58g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampleId :
 EW4M4

Quant Time: Jun 08 01:22:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 08 01:20:30 2022
 Response via : Initial Calibration


Manual Integrations
APPROVED
 Reviewed By :Semsettin Yesilyurt 06/08/2022
 Supervised By :Mahesh Dadoda 06/08/2022

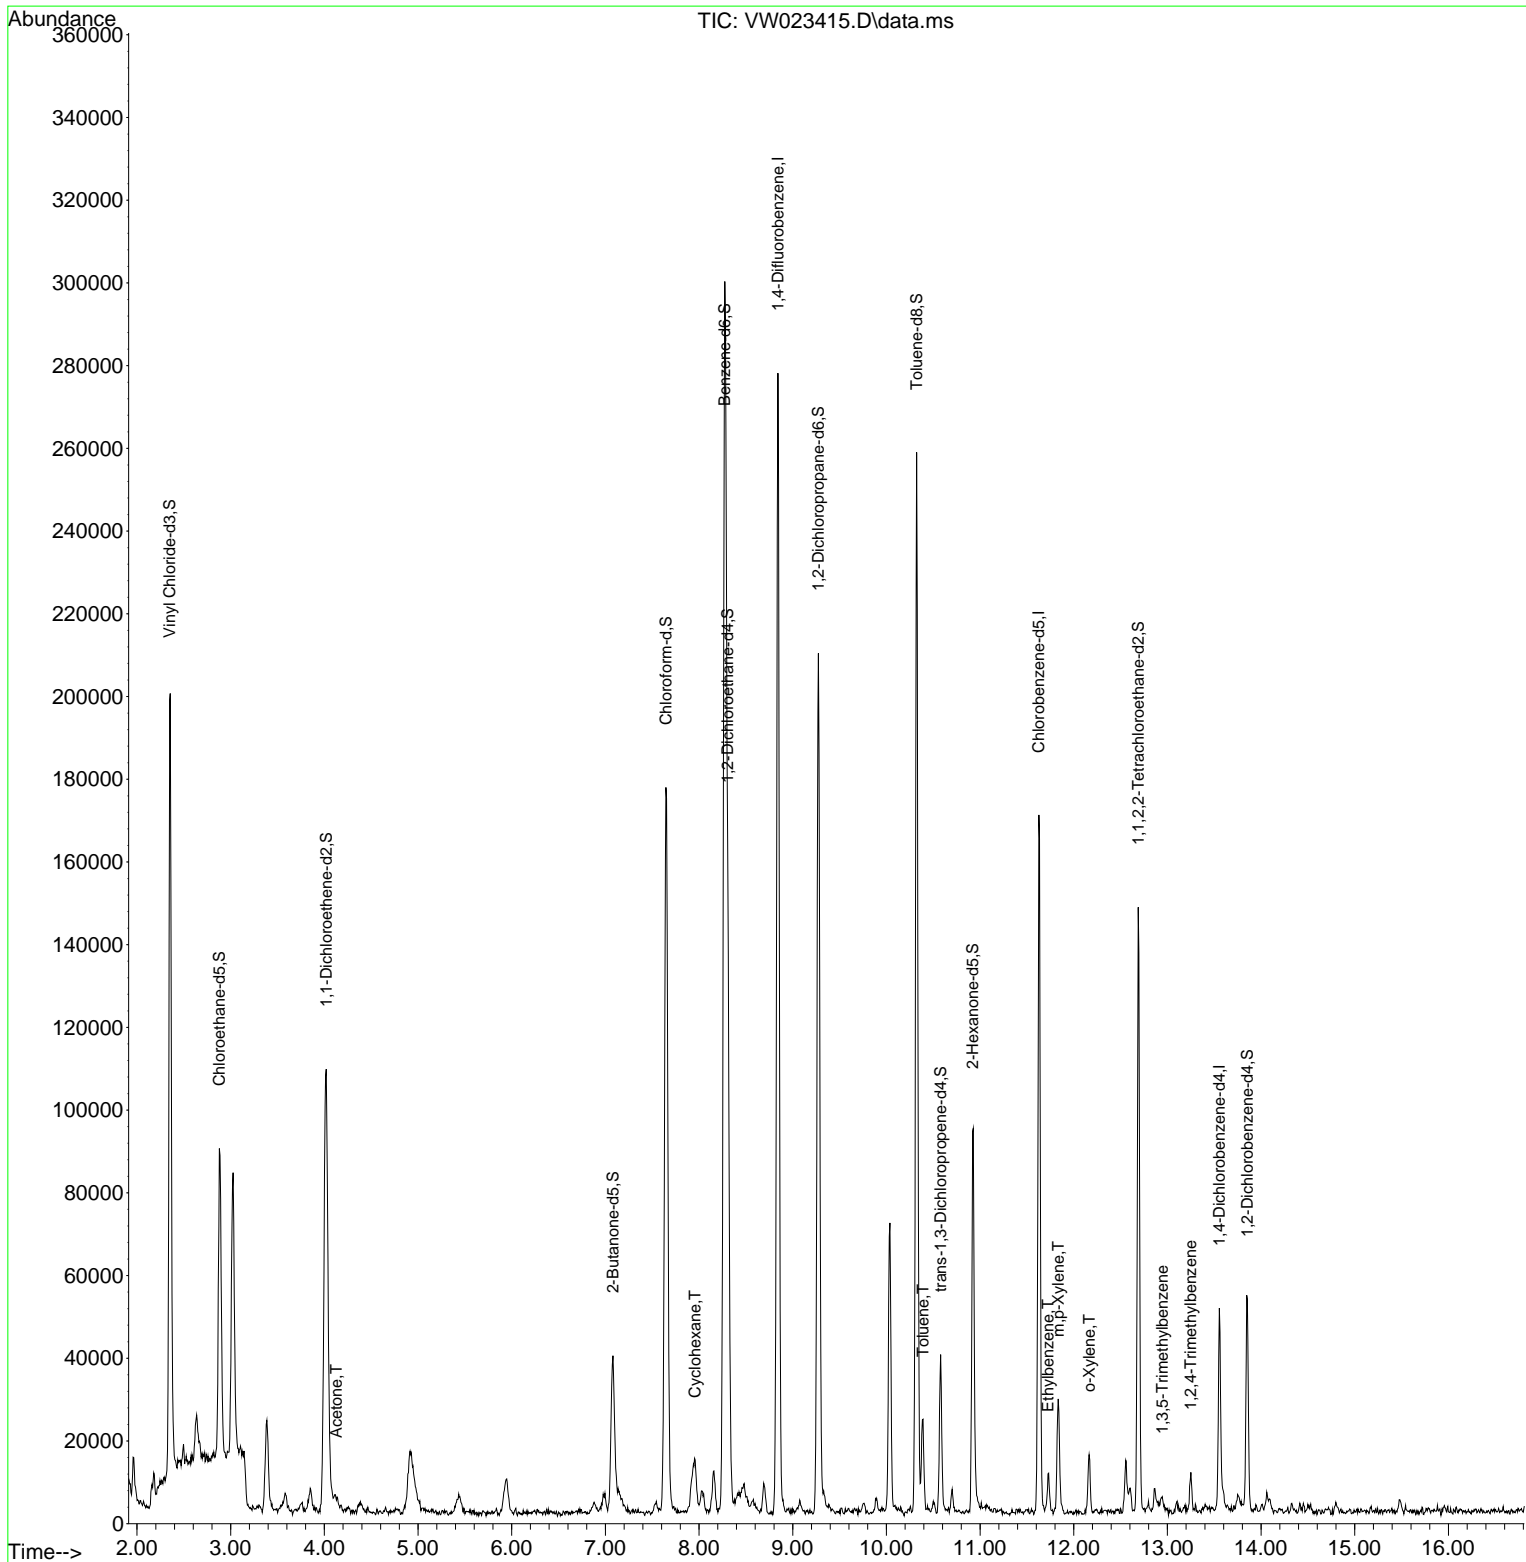

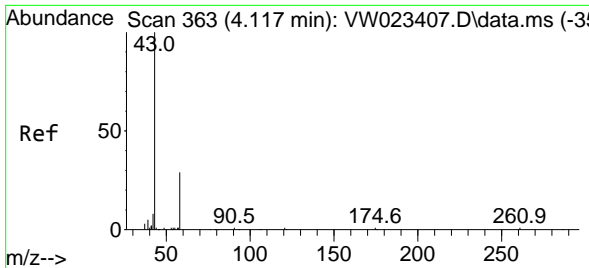




#13
 Acetone
 Concen: 8.891 ug/L
 RT: 4.129 min Scan# 30
 Delta R.T. 0.012 min
 Lab File: VW023415.D
 Acq: 07 Jun 2022 16:21

Instrument : MSVOA_W
 Client Sample Id : EW4M4

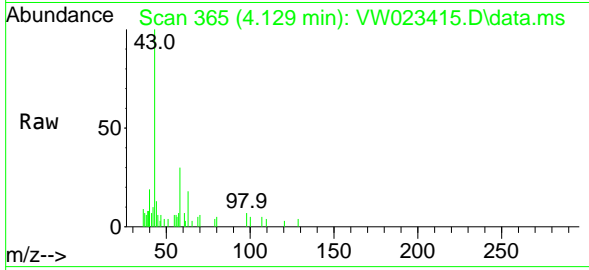


Tgt Ion: 43 Resp: 4360
 Ion Ratio Lower Upper
 43 100
 58 25.6 0.0 64.0



Manual Integrations
APPROVED
 Reviewed By : Semsettin Yesilyurt 06/08/2022
 Supervised By : Mahesh Dadoda 06/08/2022

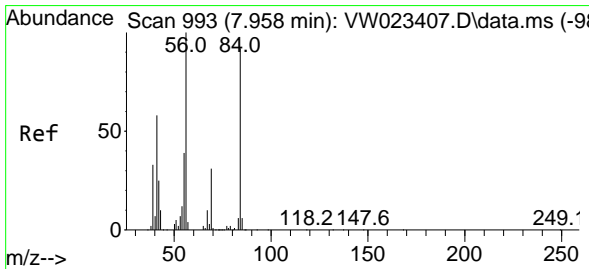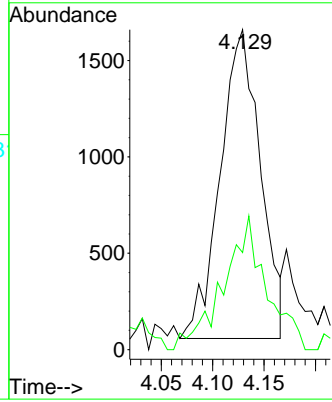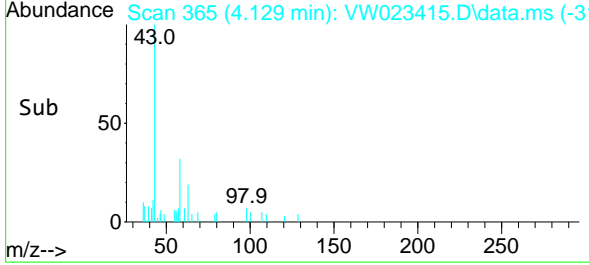


#29
 Cyclohexane
 Concen: 3.340 ug/L
 RT: 7.958 min Scan# 993
 Delta R.T. -0.000 min
 Lab File: VW023415.D
 Acq: 07 Jun 2022 16:21

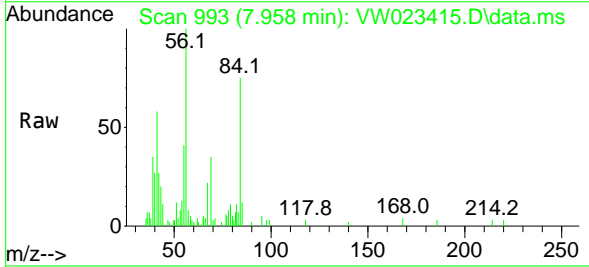


Tgt Ion: 56 Resp: 6540
 Ion Ratio Lower Upper
 56 100
 69 27.3 25.6 38.4
 84 74.3 78.2 117.4#

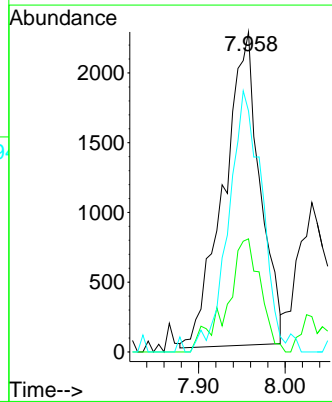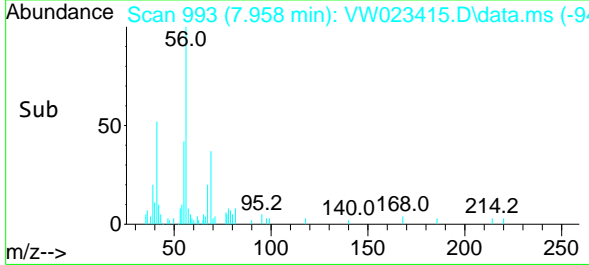

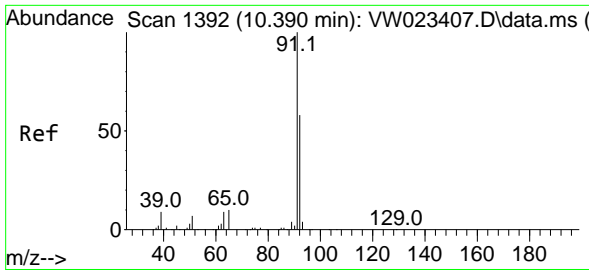

#42
 Toluene
 Concen: 2.540 ug/L
 RT: 10.390 min Scan# 11
 Delta R.T. -0.000 min
 Lab File: VW023415.D
 Acq: 07 Jun 2022 16:21




Instrument : MSVOA_W
 ClientSampleId : EW4M4

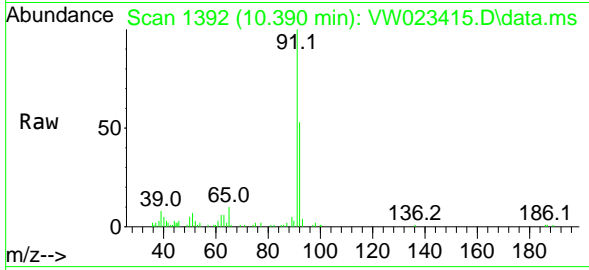


Tgt Ion: 91 Resp: 15400
 Ion Ratio Lower Upper
 91 100
 92 52.9 41.6 77.2

Manual Integrations
 APPROVED



Reviewed By :Semsettin Yesilyurt 06/08/2022
 Supervised By :Mahesh Dadoda 06/08/2022

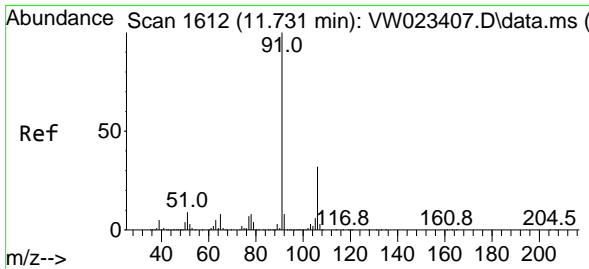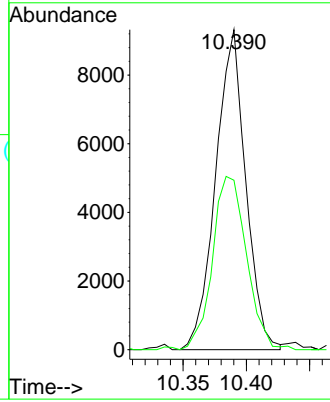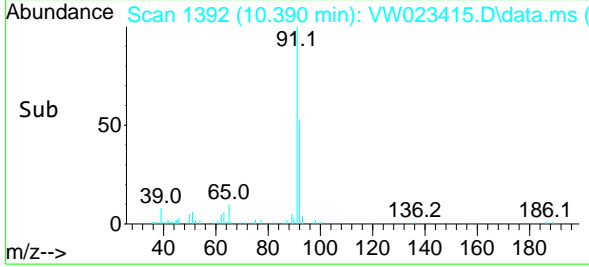


#52
 Ethylbenzene
 Concen: 0.844 ug/L
 RT: 11.725 min Scan# 1611
 Delta R.T. -0.006 min
 Lab File: VW023415.D
 Acq: 07 Jun 2022 16:21

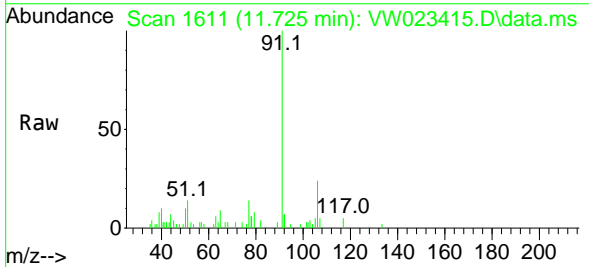


Tgt Ion: 91 Resp: 5638
 Ion Ratio Lower Upper
 91 100
 106 23.7 22.3 41.3

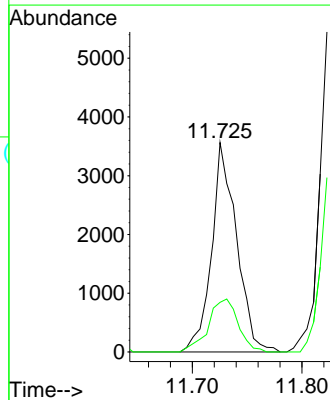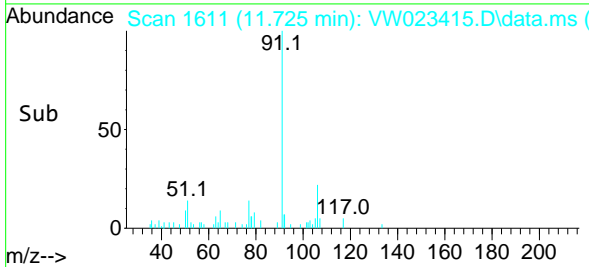

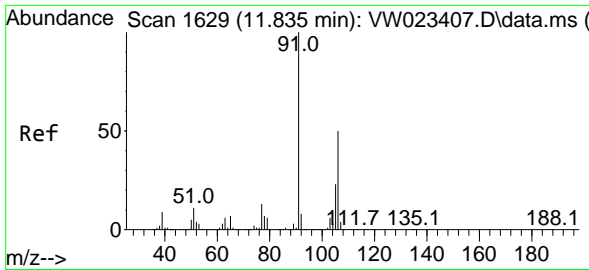

#53
 m,p-Xylene
 Concen: 3.210 ug/L
 RT: 11.835 min Scan# 1629
 Delta R.T. -0.000 min
 Lab File: VW023415.D
 Acq: 07 Jun 2022 16:21




Instrument : MSVOA_W
 ClientSampleId : EW4M4

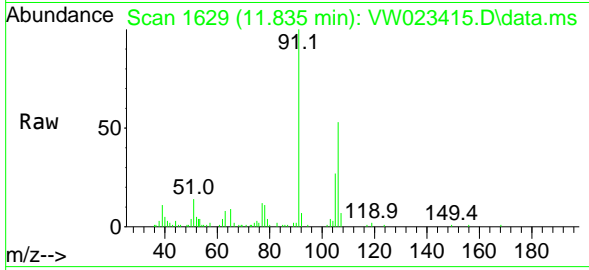


Tgt Ion:106 Resp: 8299
 Ion Ratio Lower Upper
 106 100
 91 188.8 136.8 254.0

Manual Integrations
 APPROVED



Reviewed By :Semsettin Yesilyurt 06/08/2022
 Supervised By :Mahesh Dadoda 06/08/2022

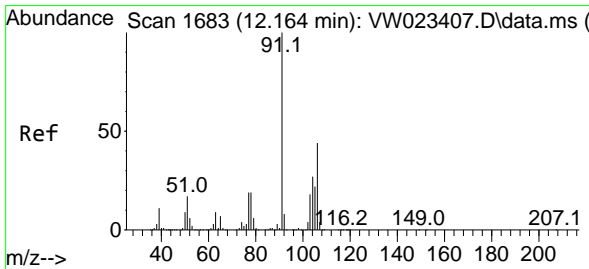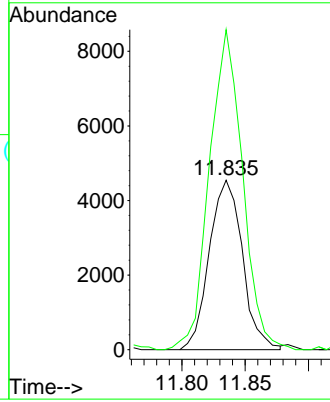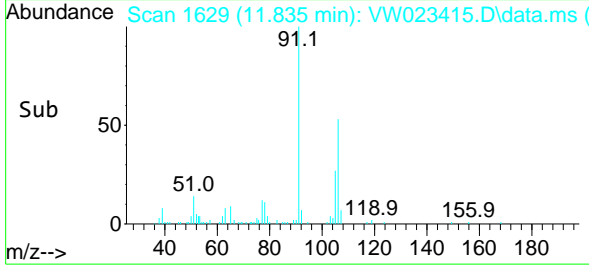


#54
 o-Xylene
 Concen: 1.513 ug/L
 RT: 12.164 min Scan# 1683
 Delta R.T. -0.000 min
 Lab File: VW023415.D
 Acq: 07 Jun 2022 16:21

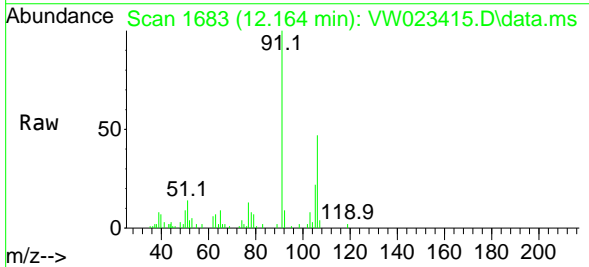


Tgt Ion:106 Resp: 3747
 Ion Ratio Lower Upper
 106 100
 91 211.4 147.2 273.4

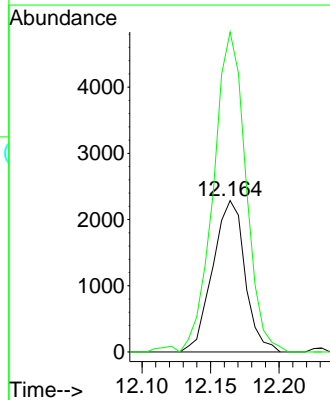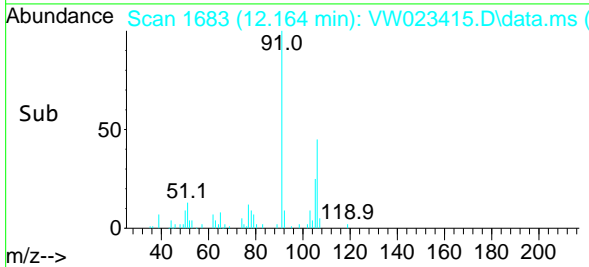

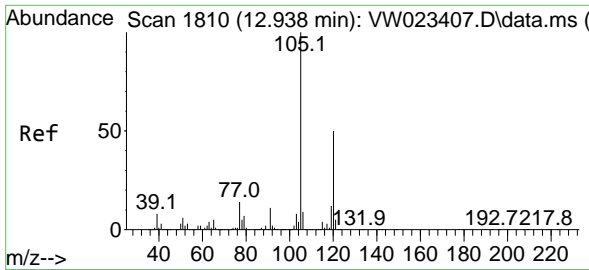

#62
 1,3,5-Trimethylbenzene
 Concen: 1.073 ug/L m
 RT: 12.945 min Scan# 1811
 Delta R.T. 0.006 min
 Lab File: VW023415.D
 Acq: 07 Jun 2022 16:21




Instrument :
 MSVOA_W
 ClientSampleId :
 EW4M4

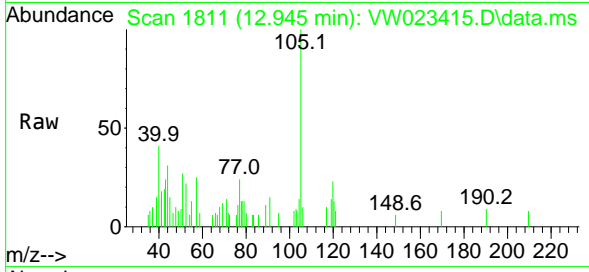

Tgt Ion:105 Resp: 140
 Ion Ratio Lower Upper
 105 100
 120 152.0 38.9 58.3

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 06/08/2022
 Supervised By :Mahesh Dadoda 06/08/2022

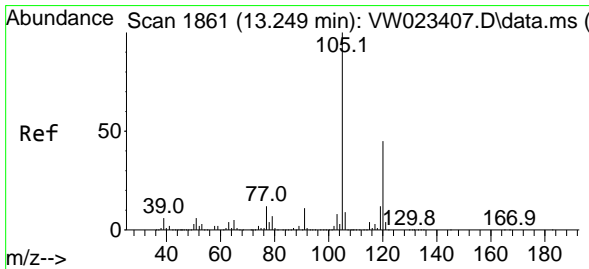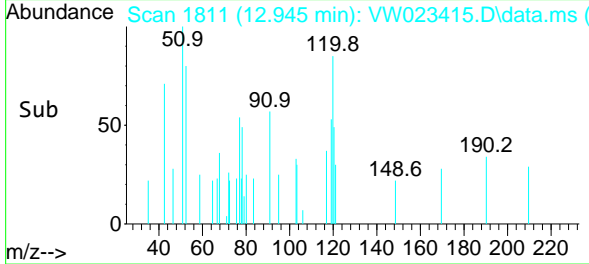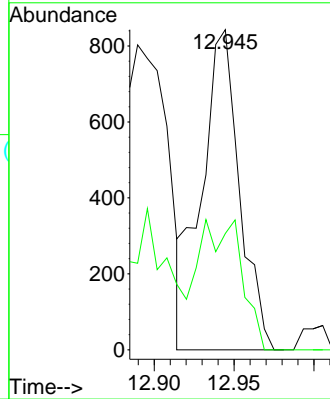

#63
 1,2,4-Trimethylbenzene
 Concen: 3.568 ug/L
 RT: 13.249 min Scan# 1861
 Delta R.T. -0.000 min
 Lab File: VW023415.D
 Acq: 07 Jun 2022 16:21

Tgt Ion:105 Resp: 4612
 Ion Ratio Lower Upper
 105 100
 120 46.2 37.4 56.2

