

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060722\
 Data File : VW023419.D
 Acq On : 07 Jun 2022 18:04
 Operator : SY/VA
 Sample : VIBLK493
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK493

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 06/08/2022
 Supervised By :Mahesh Dadoda 06/08/2022

Quant Time: Jun 08 01:23:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 08 01:20:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	322763	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	302926	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	133210	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	126023	25.224	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 100.880%			
7) Chloroethane-d5	2.885	69	87492	24.859	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 99.440%			
11) 1,1-Dichloroethene-d2	4.013	63	121827	16.238	ug/L	-0.01
Spiked Amount 25.000	Range 45 - 110		Recovery = 64.960%			
21) 2-Butanone-d5	7.080	46	53276	55.292	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 110.580%			
24) Chloroform-d	7.647	84	205731	23.638	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 94.560%			
26) 1,2-Dichloroethane-d4	8.305	65	120073m	26.263	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 105.040%			
32) Benzene-d6	8.275	84	406211	24.157	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 96.640%			
36) 1,2-Dichloropropane-d6	9.274	67	121330	25.743	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 102.960%			
41) Toluene-d8	10.323	98	377025	23.542	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 94.160%			
43) trans-1,3-Dichloroprop...	10.579	79	48905	23.257	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 93.040%			
47) 2-Hexanone-d5	10.927	63	38548	54.640	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 109.280%			
56) 1,1,2,2-Tetrachloroeth...	12.688	84	104172	25.832	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 103.320%			
66) 1,2-Dichlorobenzene-d4	13.853	152	124872	25.899	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 103.600%			
Target Compounds					Qvalue	
13) Acetone	4.129	43	2794	3.866	ug/L	60

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060722\
Data File : VW023419.D
Acq On : 07 Jun 2022 18:04
Operator : SY/VA
Sample : VIBLK493
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
VIBLK493

Quant Time: Jun 08 01:23:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060622SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 08 01:20:30 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By : Semsettin Yesilyurt 06/08/2022
Supervised By : Mahesh Dadoda 06/08/2022

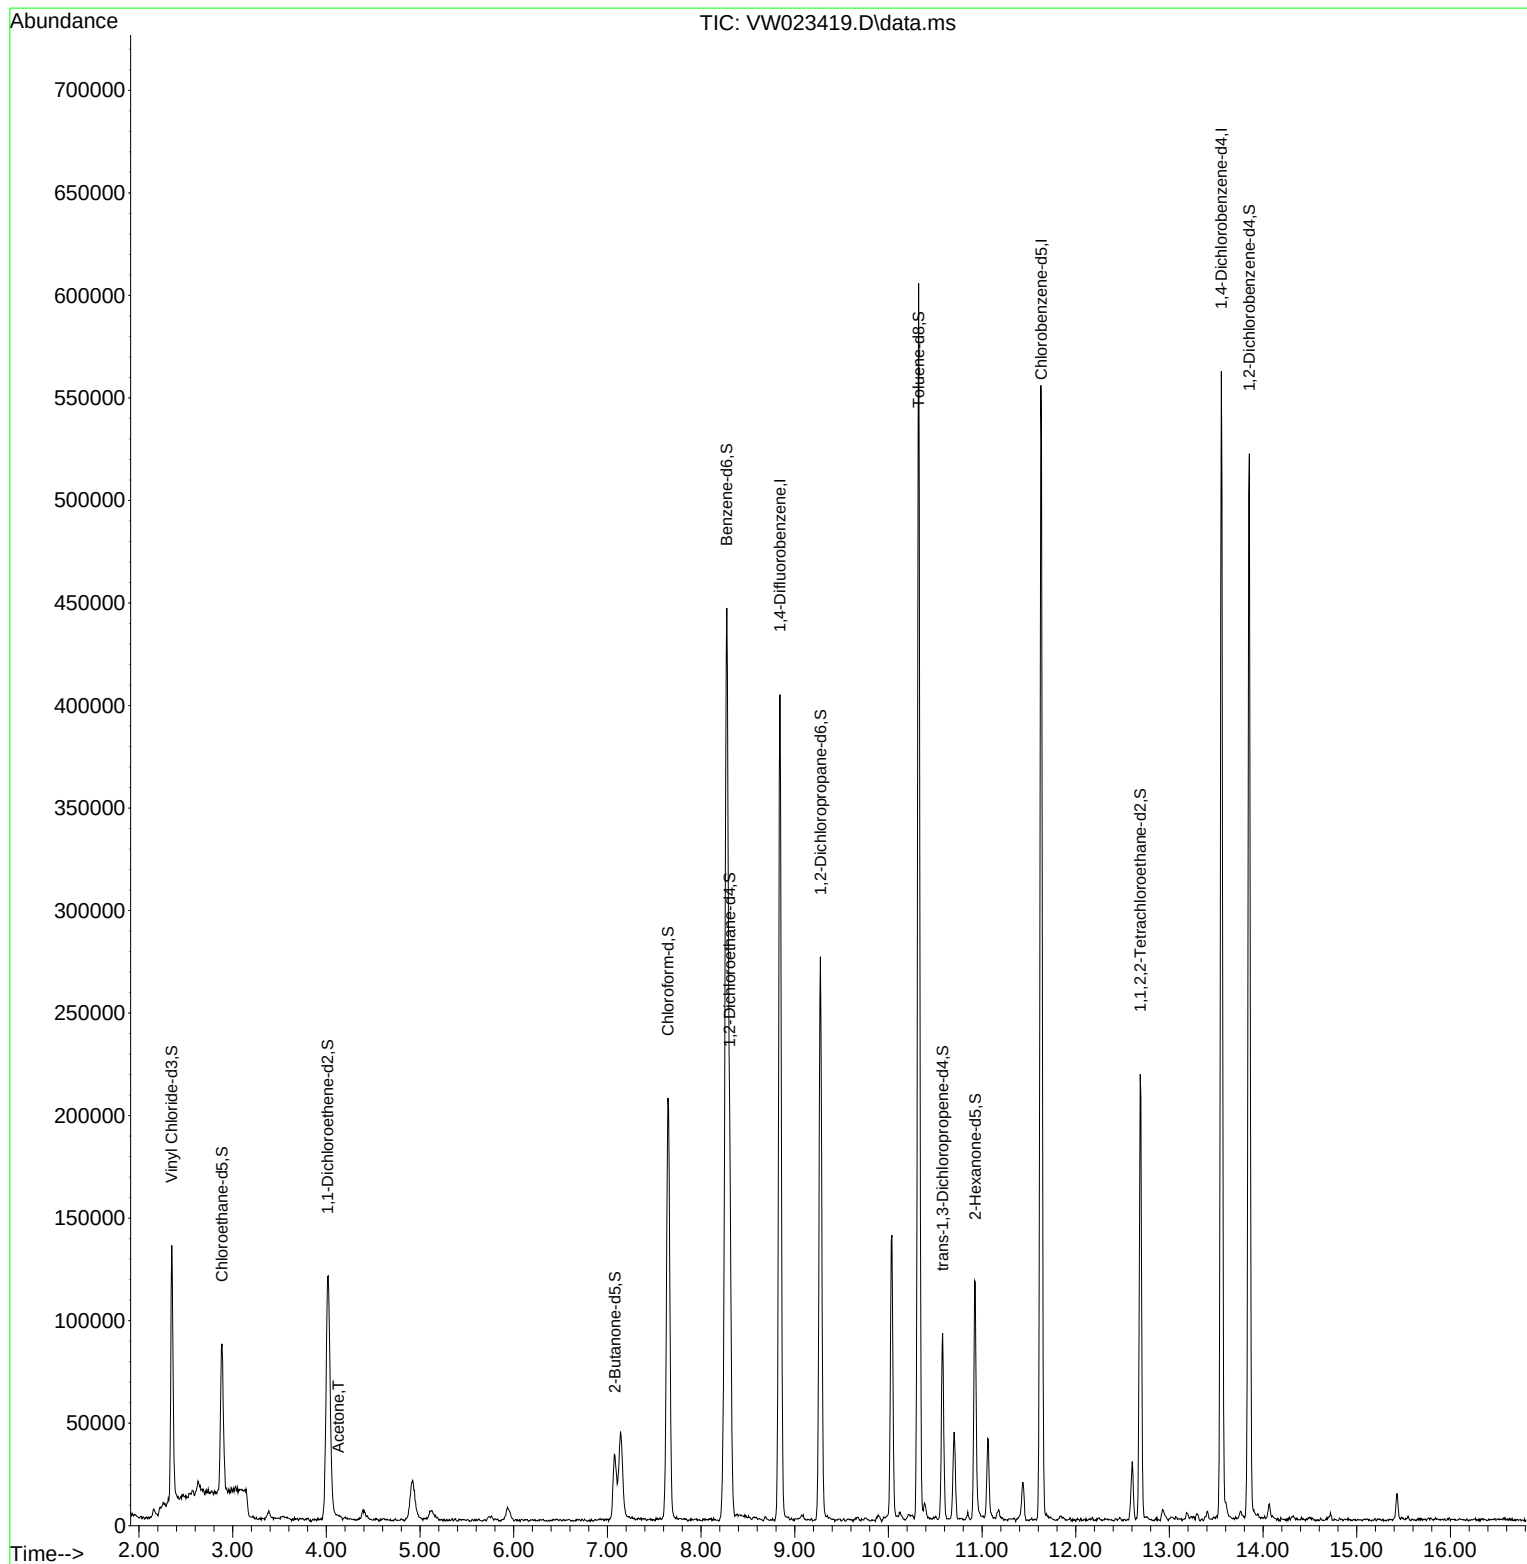

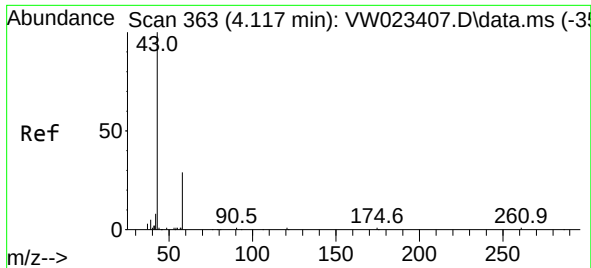

#13
 Acetone
 Concen: 3.866 ug/L
 RT: 4.129 min Scan# 30
 Delta R.T. 0.012 min
 Lab File: VW023419.D
 Acq: 07 Jun 2022 18:04

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK493

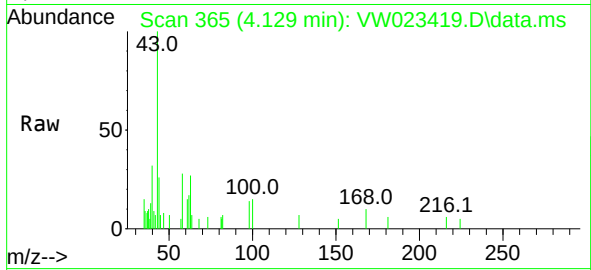

Tgt Ion: 43 Resp: 2794
 Ion Ratio Lower Upper
 43 100
 58 9.7 0.0 64.0

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 06/08/2022
 Supervised By :Mahesh Dadoda 06/08/2022

