

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060723\
 Data File : VW026122.D
 Acq On : 07 Jun 2023 10:14
 Operator : SY/MD
 Sample : 03062-07
 Misc : 5.75g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZEL3

Quant Time: Jun 08 00:21:23 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 08 00:20:42 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	1053395	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	948006	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	433003	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	300161	20.255	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.040%
7) Chloroethane-d5	2.893	69	251820	22.700	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.800%
11) 1,1-Dichloroethene-d2	4.021	65	147329	20.162	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	80.640%
21) 2-Butanone-d5	7.075	46	206719	47.914	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	95.820%
24) Chloroform-d	7.648	84	622218	20.171	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	80.680%
26) 1,2-Dichloroethane-d4	8.307	65	359965	21.340	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	85.360%
32) Benzene-d6	8.276	84	1259926	19.751	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	79.000%
36) 1,2-Dichloropropane-d6	9.276	67	420425	20.804	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	83.200%
41) Toluene-d8	10.325	98	1095748	19.369	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	77.480%
43) trans-1,3-Dichloroprop...	10.575	79	151981	18.978	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	75.920%
47) 2-Hexanone-d5	10.922	63	135971	42.670	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.340%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	322294	21.916	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	87.680%
66) 1,2-Dichlorobenzene-d4	13.848	152	342145	20.644	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	82.560%
Target Compounds						Qvalue
34) Trichloroethene	9.087	95	10982	0.660	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060723\
Data File : VW026122.D
Acq On : 07 Jun 2023 10:14
Operator : SY/MD
Sample : 03062-07
Misc : 5.75g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EZEL3

Quant Time: Jun 08 00:21:23 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jun 08 00:20:42 2023
Response via : Initial Calibration

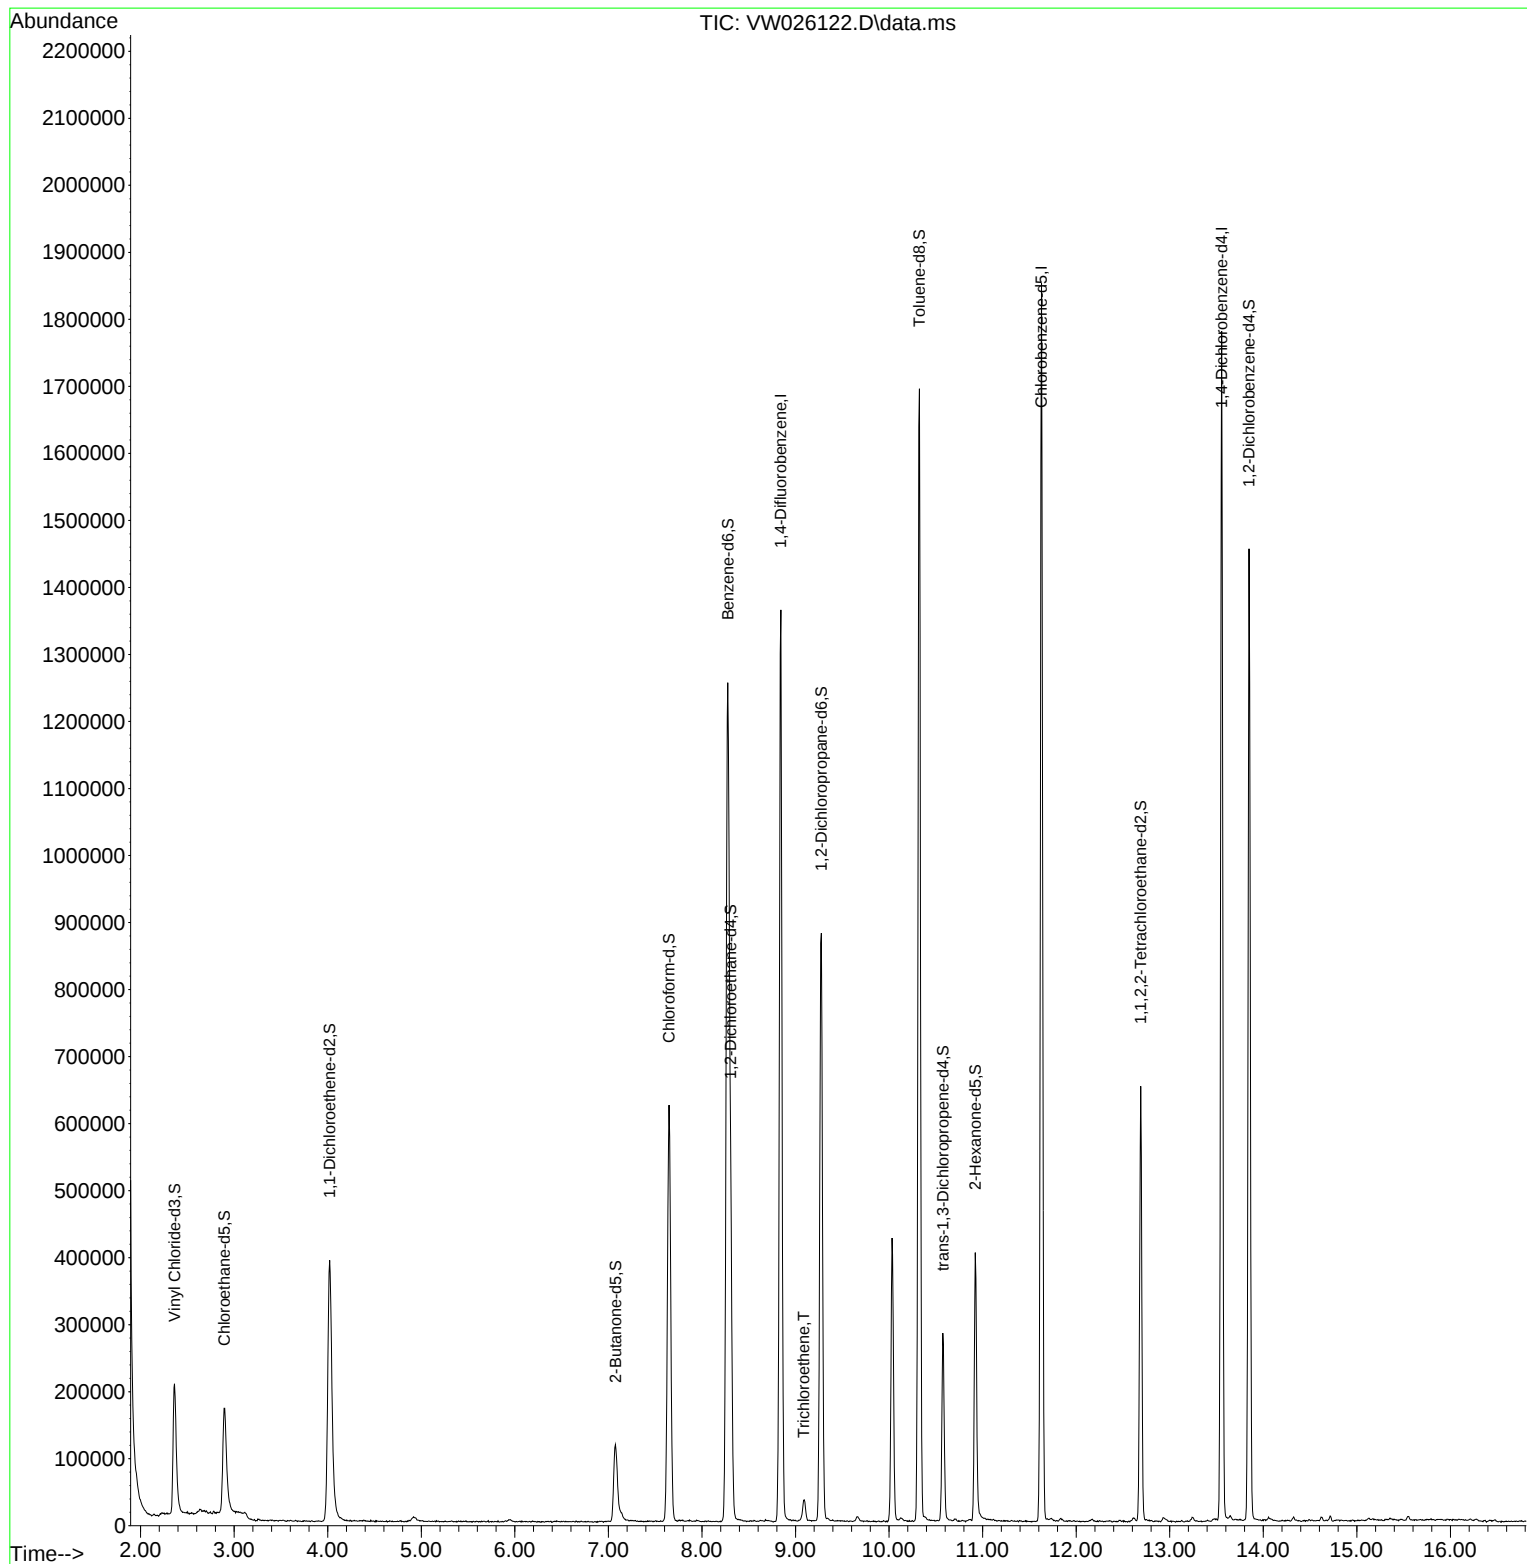

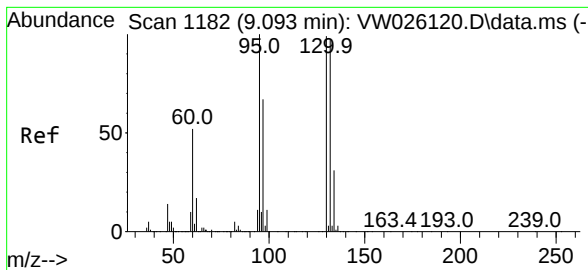

#34

Trichloroethene

Concen: 0.660 ug/L

RT: 9.087 min Scan# 11

Delta R.T. -0.006 min

Lab File: VW026122.D


Acq: 07 Jun 2023 10:14

Instrument :

MSVOA_W

ClientSampleId :

EZEL3

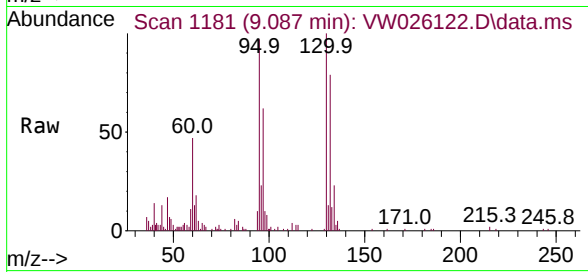

Tgt Ion: 95 Resp: 10982

Ion Ratio Lower Upper

95 100

97 63.5 45.9 85.3

132 81.3 67.1 124.7

130 103.0 68.0 126.2

