

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060723\
 Data File : VW026123.D
 Acq On : 07 Jun 2023 14:47
 Operator : SY/MD
 Sample : 03078-01
 Misc : 6.53g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 ESQW9

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 06/08/2023
 Supervised By :Mahesh Dadoda 06/08/2023

Quant Time: Jun 08 00:21:35 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 08 00:20:42 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	925288	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	755027	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	272271	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	274185	21.064	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	84.240%		
7) Chloroethane-d5	2.893	69	225954	23.189	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	92.760%		
11) 1,1-Dichloroethene-d2	4.021	65	129075	20.110	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	80.440%		
21) 2-Butanone-d5	7.069	46	200568	52.925	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	105.840%		
24) Chloroform-d	7.648	84	551655	20.359	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	81.440%		
26) 1,2-Dichloroethane-d4	8.301	65	322429m	21.762	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	87.040%		
32) Benzene-d6	8.276	84	1102219	21.695	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	86.800%		
36) 1,2-Dichloropropane-d6	9.270	67	363255	22.569	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	90.280%		
41) Toluene-d8	10.319	98	886976	19.686	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	78.760%		
43) trans-1,3-Dichloroprop...	10.575	79	128779	20.191	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	80.760%		
47) 2-Hexanone-d5	10.922	63	126917	50.008	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	100.020%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	277537	23.696	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	94.800%		
66) 1,2-Dichlorobenzene-d4	13.849	152	220587	21.167	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	84.680%		
Target Compounds					Qvalue	
13) Acetone	4.119	43	14601m	4.979	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060723\
Data File : VW026123.D
Acq On : 07 Jun 2023 14:47
Operator : SY/MD
Sample : 03078-01
Misc : 6.53g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
ESQW9

Quant Time: Jun 08 00:21:35 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jun 08 00:20:42 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/08/2023
Supervised By :Mahesh Dadoda 06/08/2023

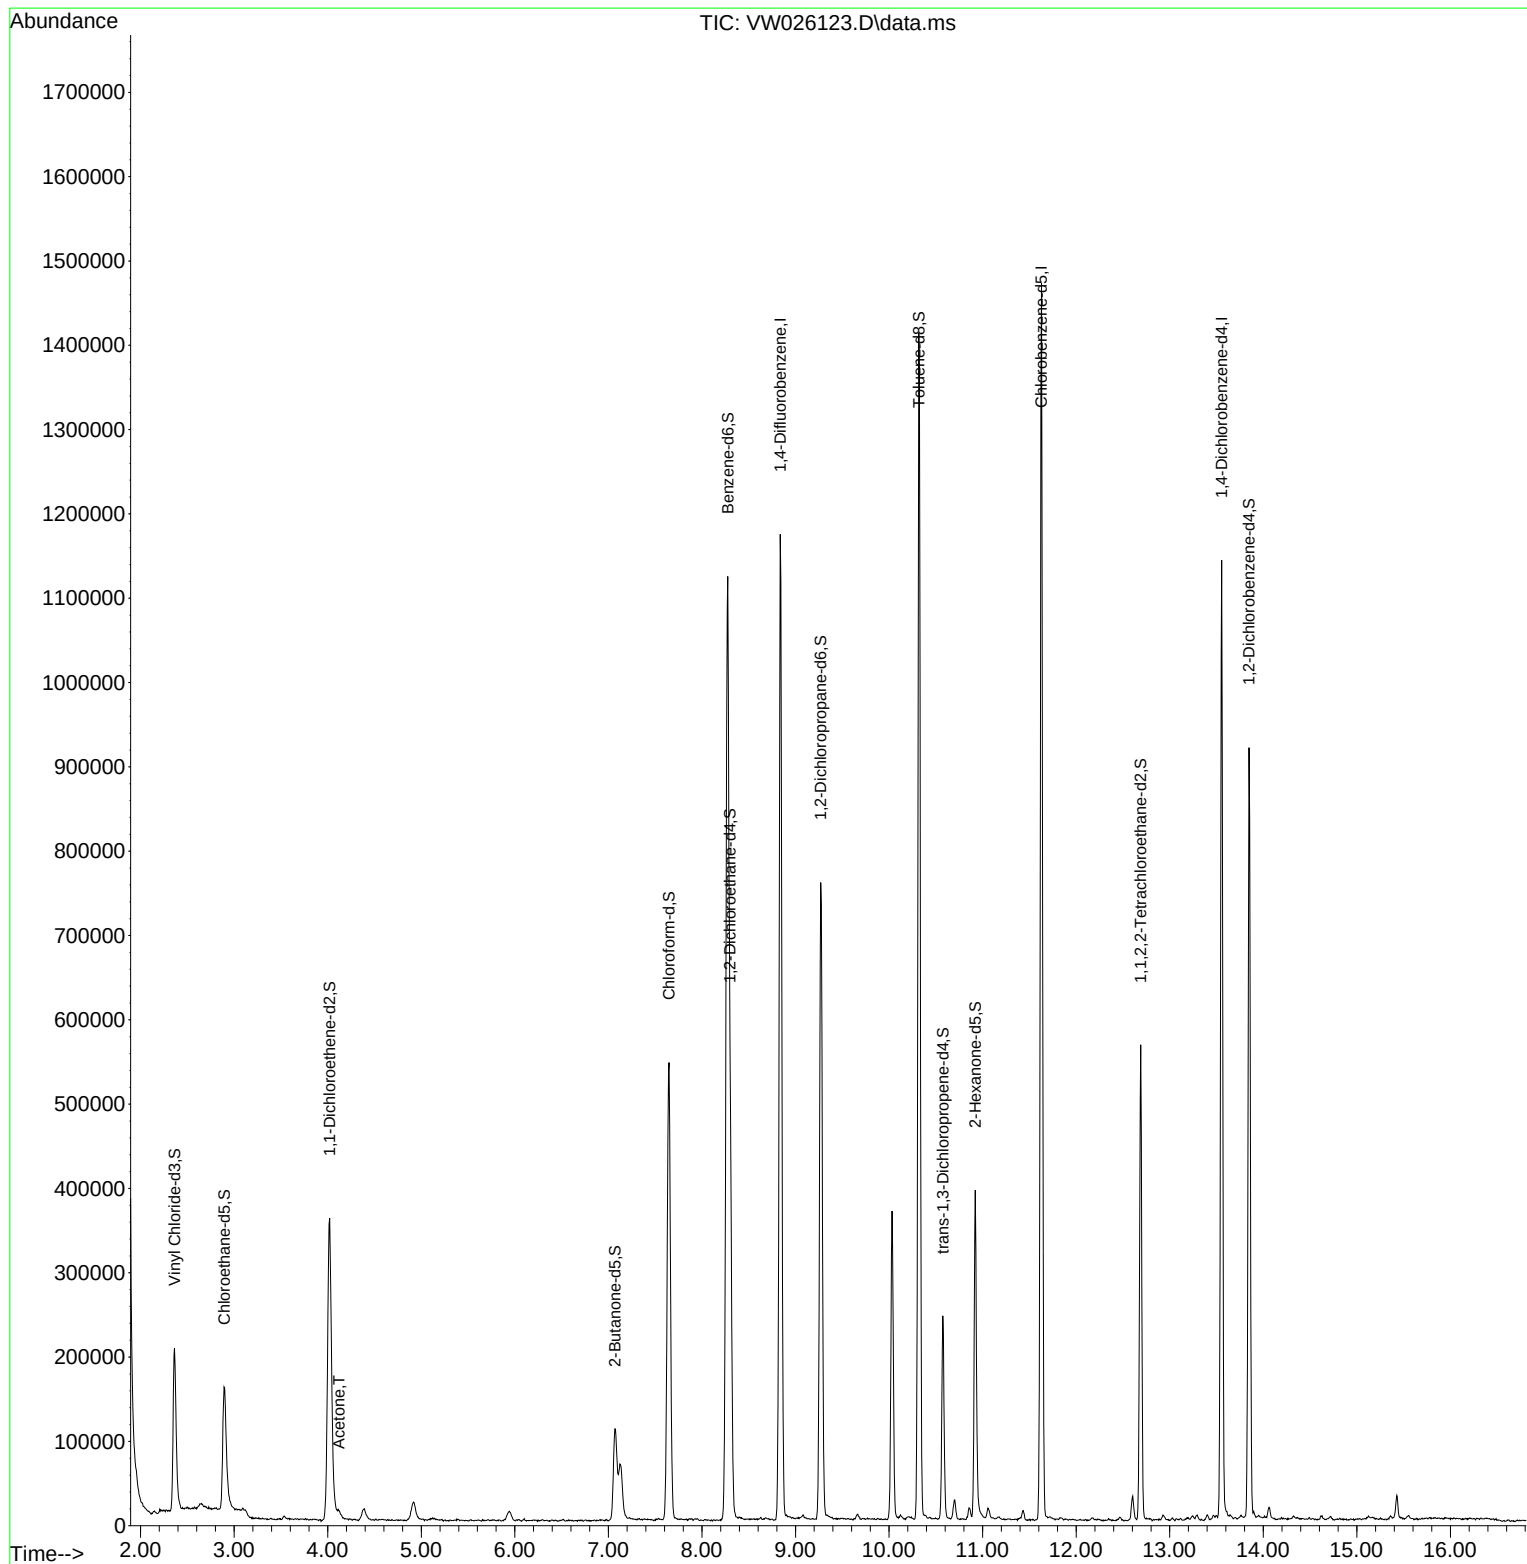

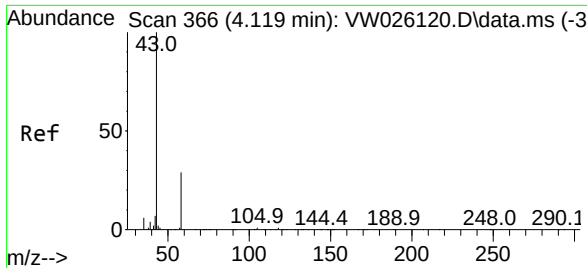

#13
Acetone
Concen: 4.979 ug/L m
RT: 4.119 min Scan# 30
Delta R.T. -0.000 min
Lab File: VW026123.D
Acq: 07 Jun 2023 14:47

Instrument :
MSVOA_W
ClientSampleId :
ESQW9

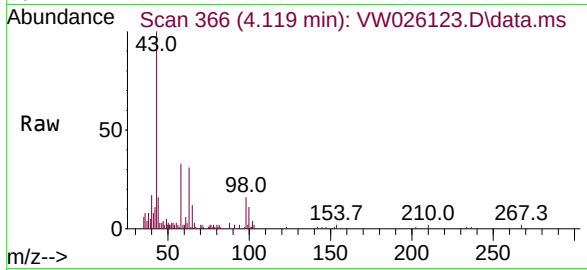

Tgt Ion: 43 Resp: 1460
Ion Ratio Lower Upper
43 100
58 0.4 0.0 58.2

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 06/08/2023
Supervised By :Mahesh Dadoda 06/08/2023

