

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060723\
 Data File : VW026125.D
 Acq On : 07 Jun 2023 15:35
 Operator : SY/MD
 Sample : 03078-04
 Misc : 6.53g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 ESQX2

Quant Time: Jun 08 00:22:01 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 08 00:20:42 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	819255	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	639222	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	192759	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	246404	21.380	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	85.520%
7) Chloroethane-d5	2.899	69	208007	24.110	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	96.440%
11) 1,1-Dichloroethene-d2	4.027	65	114332	20.118	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	80.480%
21) 2-Butanone-d5	7.075	46	186376	55.545	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	111.100%
24) Chloroform-d	7.648	84	506809	21.125	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	84.520%
26) 1,2-Dichloroethane-d4	8.307	65	303730	23.153	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	92.600%
32) Benzene-d6	8.276	84	1019501	23.703	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	94.800%
36) 1,2-Dichloropropane-d6	9.270	67	338425	24.835	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	99.360%
41) Toluene-d8	10.325	98	789820	20.706	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	82.840%
43) trans-1,3-Dichloroprop...	10.575	79	115368	21.365	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	85.440%
47) 2-Hexanone-d5	10.922	63	118157	54.991	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	109.980%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	254658	25.681	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	102.720%
66) 1,2-Dichlorobenzene-d4	13.848	152	160428	21.744	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	86.960%
Target Compounds					Qvalue	
13) Acetone	4.131	43	30693	11.822	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060723\
Data File : VW026125.D
Acq On : 07 Jun 2023 15:35
Operator : SY/MD
Sample : 03078-04
Misc : 6.53g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
ESQX2

Quant Time: Jun 08 00:22:01 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jun 08 00:20:42 2023
Response via : Initial Calibration

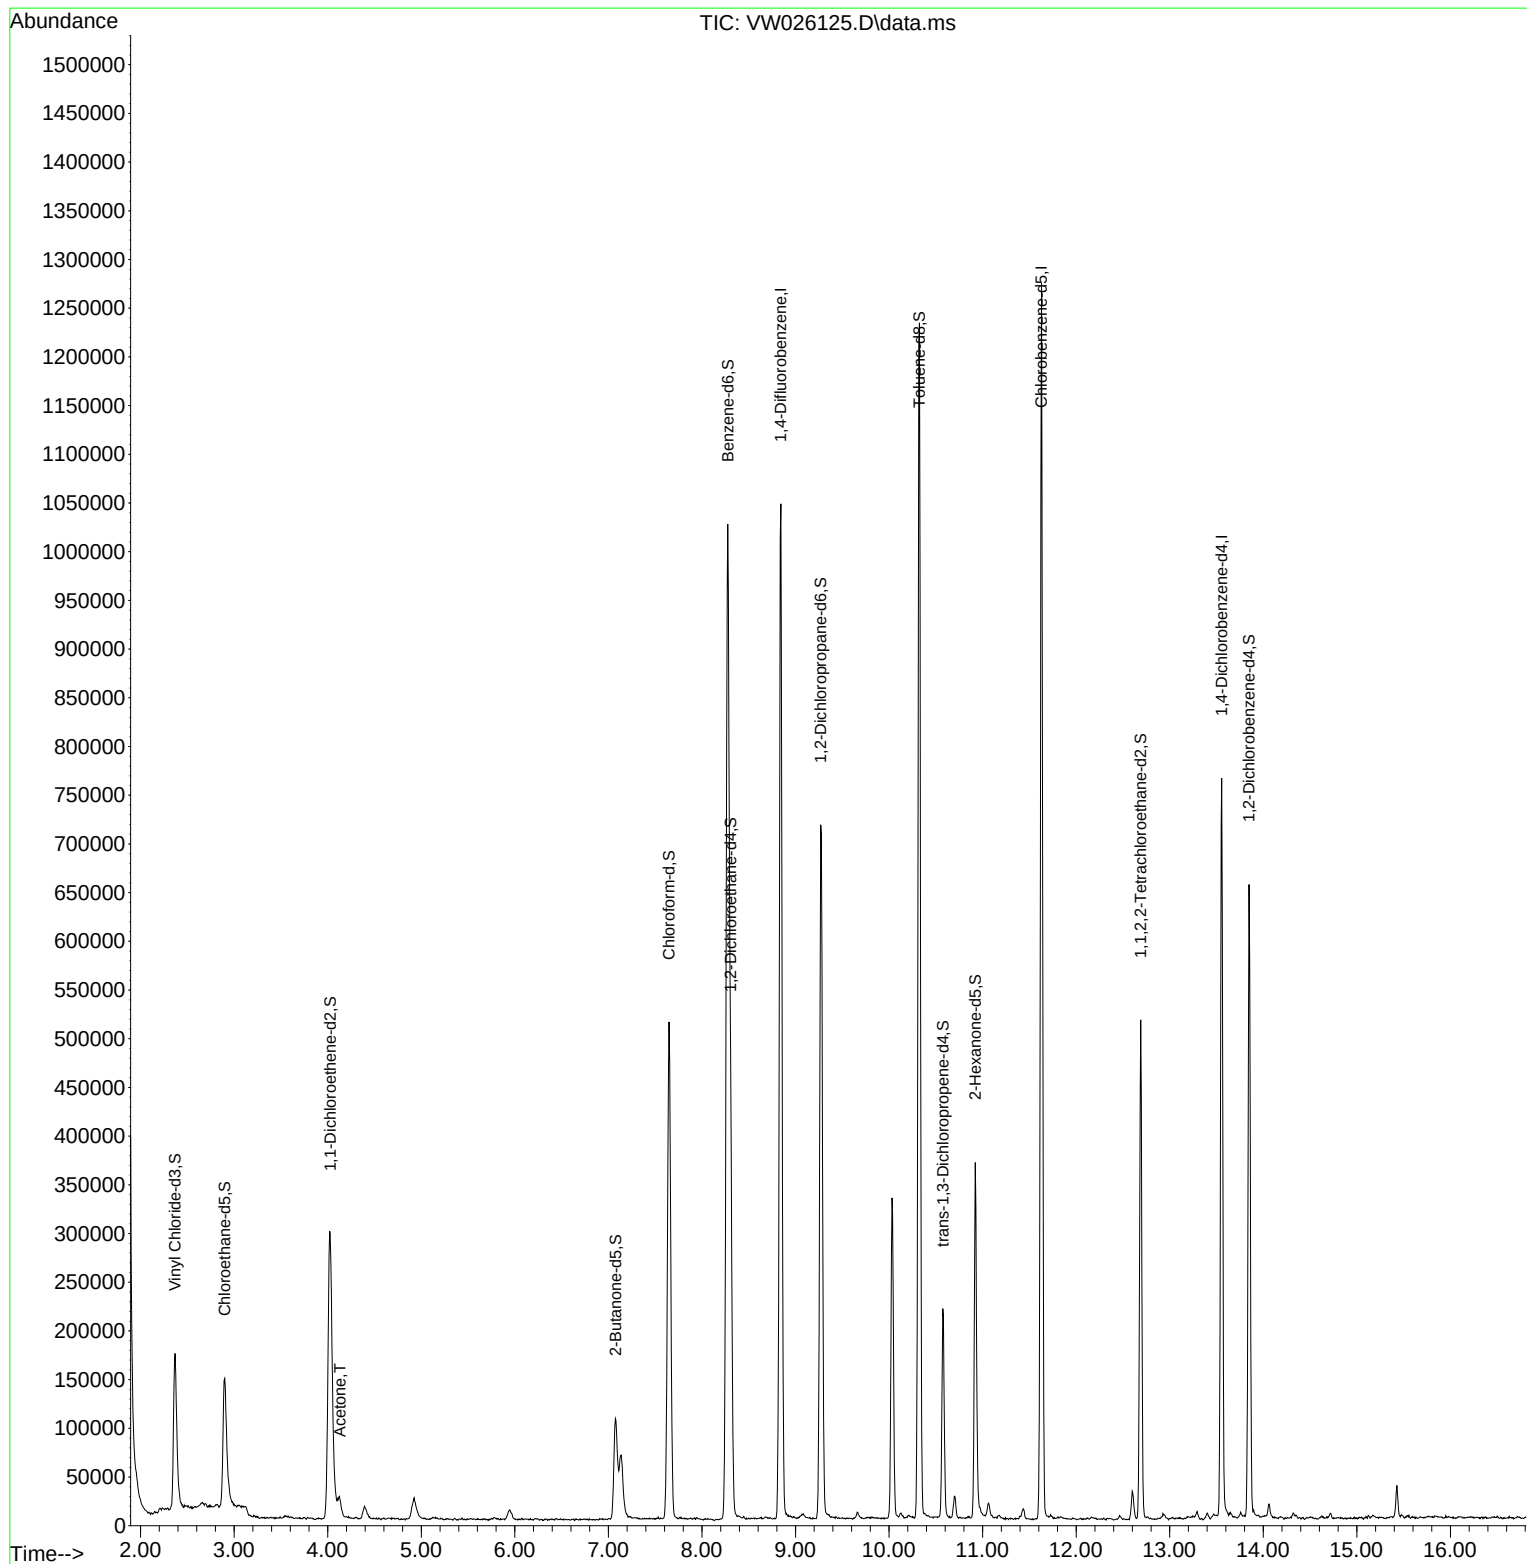

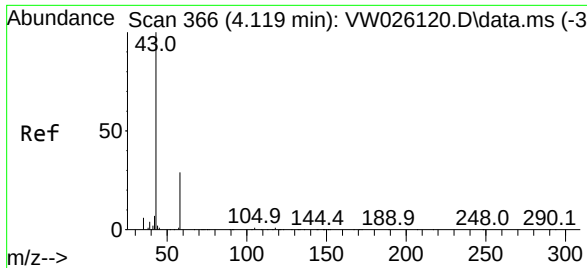

#13
 Acetone
 Concen: 11.822 ug/L
 RT: 4.131 min Scan# 30
 Delta R.T. 0.012 min
 Lab File: VW026125.D
 Acq: 07 Jun 2023 15:35

Instrument :
 MSVOA_W
 ClientSampleId :
 ESQX2

Tgt Ion: 43 Resp: 30693
 Ion Ratio Lower Upper
 43 100
 58 29.6 0.0 58.2

