

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060724\
 Data File : VW029051.D
 Acq On : 07 Jun 2024 10:41
 Operator : SY/MD
 Sample : P2696-12
 Misc : 4.57g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Jun 07 23:06:42 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 07 23:05:54 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	654377	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	581835	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	248016	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	199733	19.213	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	76.840%
7) Chloroethane-d5	2.899	69	164646	20.625	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.520%
11) 1,1-Dichloroethene-d2	4.021	65	92864	20.324	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	81.280%
21) 2-Butanone-d5	7.075	46	87883	41.376	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	82.760%
24) Chloroform-d	7.648	84	397940	21.316	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	85.280%
26) 1,2-Dichloroethane-d4	8.307	65	210676	21.435	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	85.760%
32) Benzene-d6	8.276	84	826552	23.145	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	92.600%
36) 1,2-Dichloropropane-d6	9.270	67	247362	22.845	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	91.400%
41) Toluene-d8	10.319	98	737041	23.128	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	92.520%
43) trans-1,3-Dichloroprop...	10.575	79	90146	21.667	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	86.680%
47) 2-Hexanone-d5	10.922	63	65298	45.699	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.400%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	162237	21.568	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	86.280%
66) 1,2-Dichlorobenzene-d4	13.848	152	204423	23.227	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	92.920%
Target Compounds						
39) cis-1,3-Dichloropropene	10.032	75	6715	0.488	ug/L	Qvalue # 49


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060724\
Data File : VW029051.D
Acq On : 07 Jun 2024 10:41
Operator : SY/MD
Sample : P2696-12
Misc : 4.57g/10mL/MSVOA_W/SOIL/B
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Jun 07 23:06:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 07 23:05:54 2024
Response via : Initial Calibration

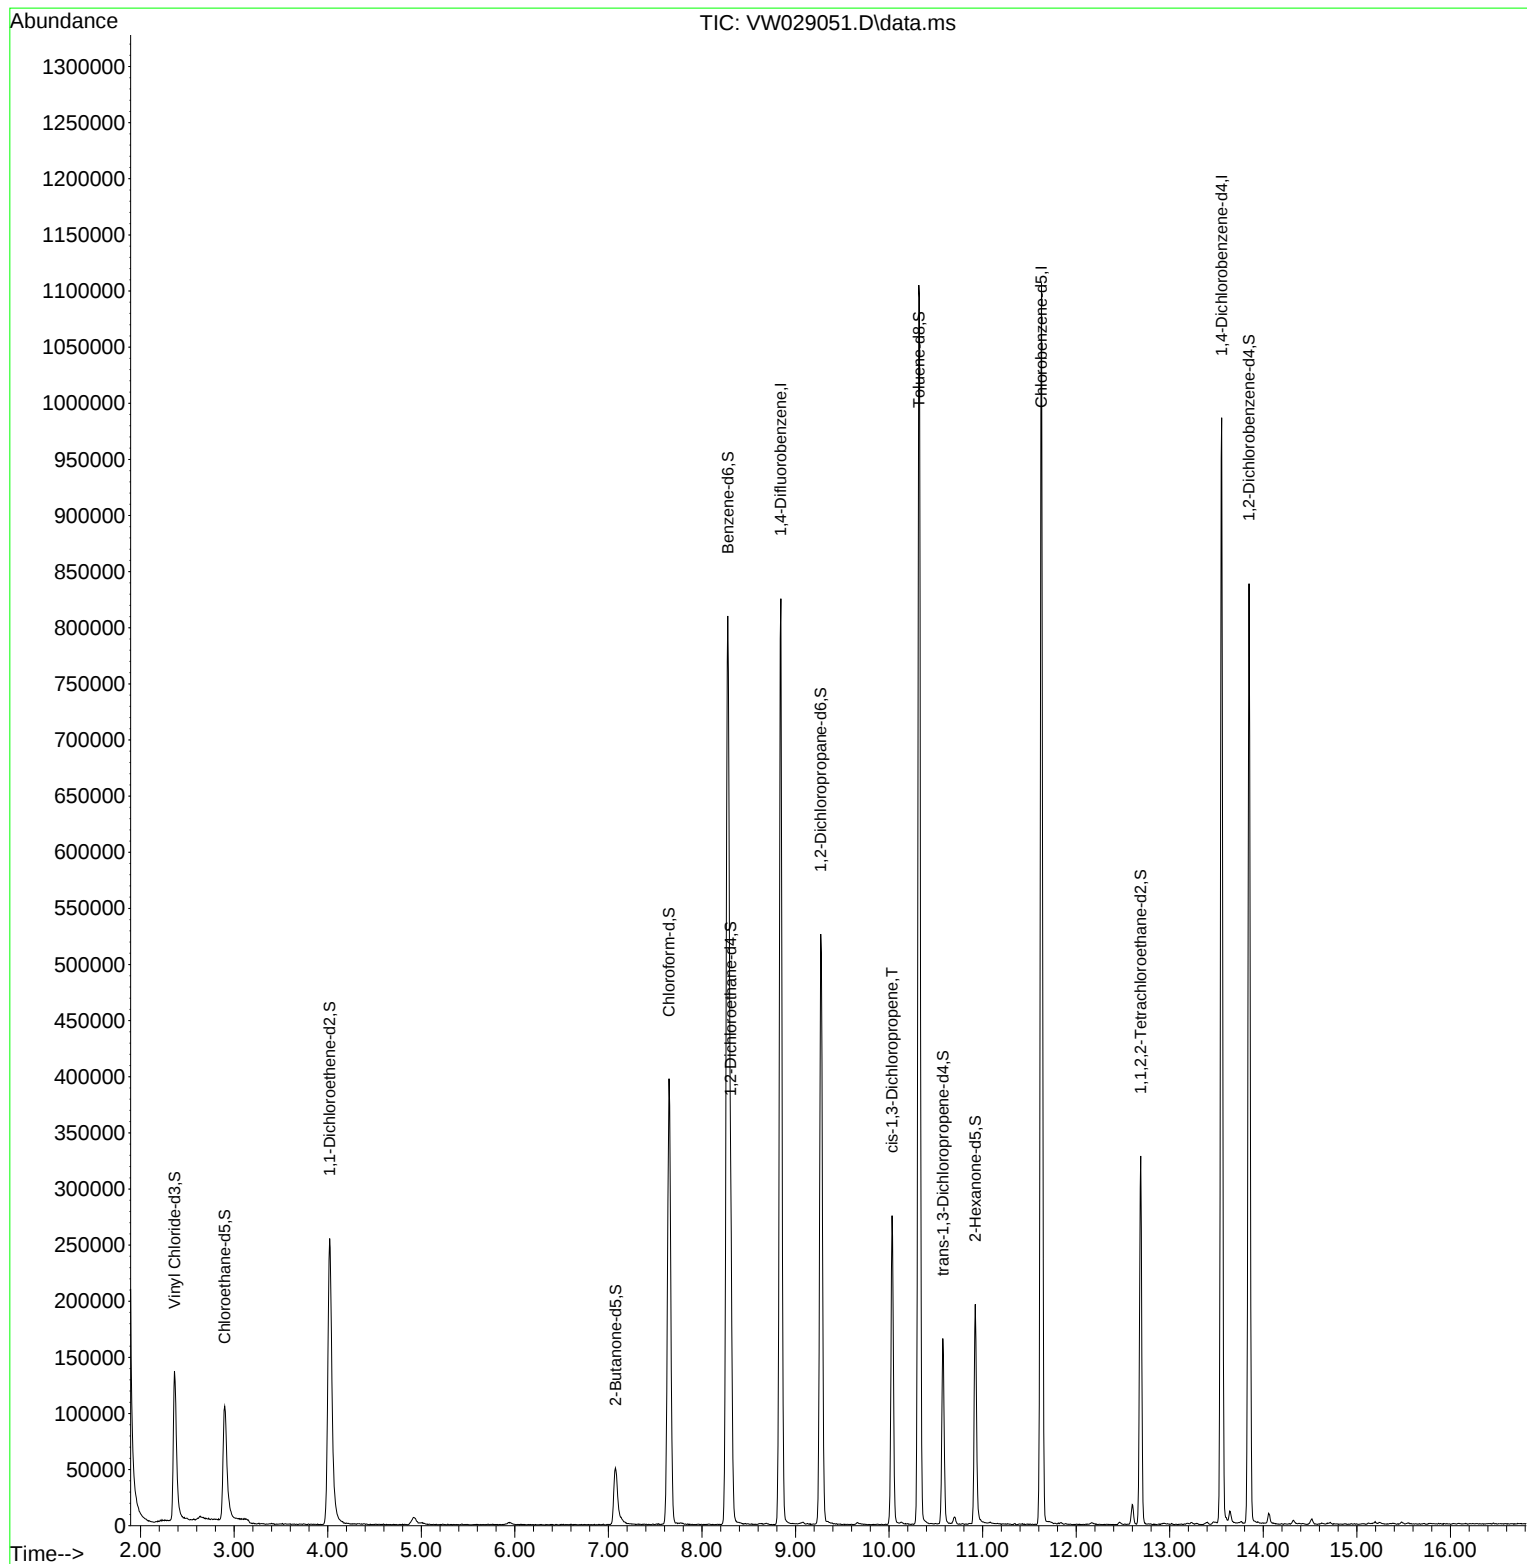

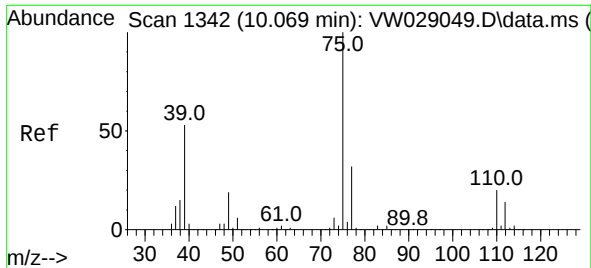

#39
 cis-1,3-Dichloropropene
 Concen: 0.488 ug/L
 RT: 10.032 min Scan# 14
 Delta R.T. -0.037 min
 Lab File: VW029051.D
 Acq: 07 Jun 2024 10:41

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 6715
 Ion Ratio Lower Upper
 75 100
 77 57.4 21.0 39.0#

