

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060724\
 Data File : VW029052.D
 Acq On : 07 Jun 2024 11:05
 Operator : SY/MD
 Sample : P2696-23
 Misc : 5.31g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Jun 07 23:06:55 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 07 23:05:54 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	513182	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	368581	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	110245	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	166959	20.479	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.920%
7) Chloroethane-d5	2.899	69	135393	21.627	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	86.520%
11) 1,1-Dichloroethene-d2	4.021	65	73681	20.563	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	82.240%
21) 2-Butanone-d5	7.075	46	84195	50.546	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	101.100%
24) Chloroform-d	7.648	84	312406	21.338	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	85.360%
26) 1,2-Dichloroethane-d4	8.490	65	112	0.015	ug/L	0.18
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.040%#
32) Benzene-d6	8.276	84	627958	27.758	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	111.040%
36) 1,2-Dichloropropane-d6	9.276	67	194534	28.361	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	113.440%
41) Toluene-d8	10.325	98	493862	24.463	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	97.840%
43) trans-1,3-Dichloroprop...	10.575	79	67260	25.519	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	102.080%
47) 2-Hexanone-d5	10.922	63	57277	63.279	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	126.560%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	114295	23.986	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	95.960%
66) 1,2-Dichlorobenzene-d4	13.848	152	82057	20.975	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	83.880%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.038	75	5170	0.593	ug/L #	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060724\
Data File : VW029052.D
Acq On : 07 Jun 2024 11:05
Operator : SY/MD
Sample : P2696-23
Misc : 5.31g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Jun 07 23:06:55 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 07 23:05:54 2024
Response via : Initial Calibration

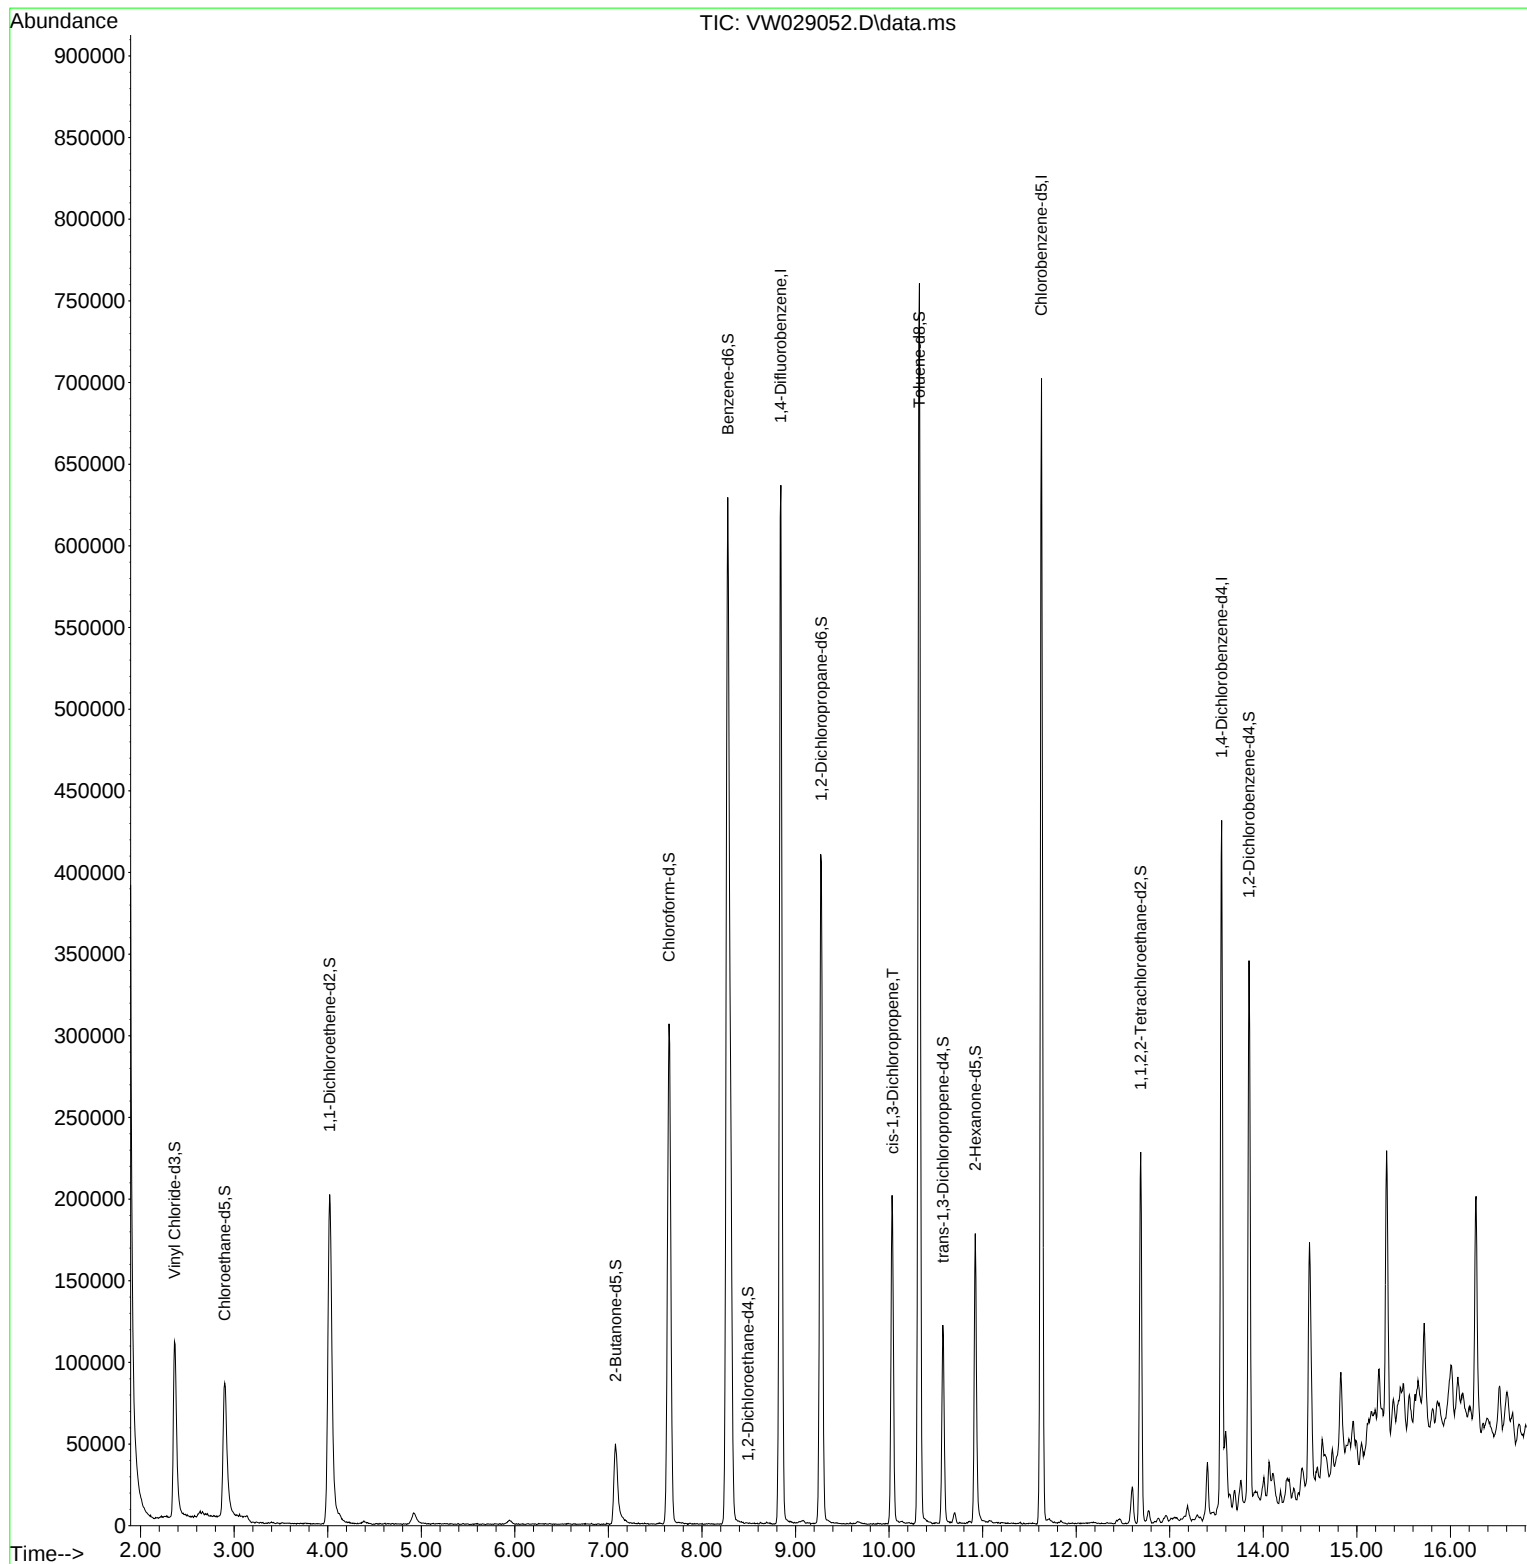

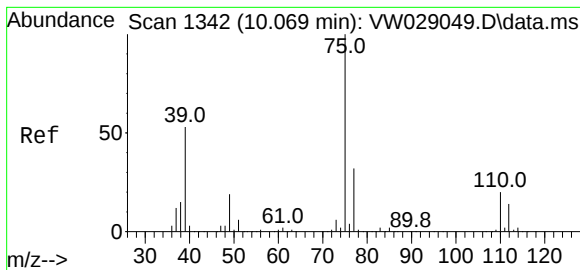

#39
 cis-1,3-Dichloropropene
 Concen: 0.593 ug/L
 RT: 10.038 min Scan# 14
 Delta R.T. -0.031 min
 Lab File: VW029052.D
 Acq: 07 Jun 2024 11:05

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 5170
 Ion Ratio Lower Upper
 75 100
 77 42.8 21.0 39.0#

