

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060724\
 Data File : VW029068.D
 Acq On : 07 Jun 2024 17:29
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Jun 07 23:12:10 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 07 23:05:54 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	334441	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	310829	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	143804	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	87822	16.530	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	66.120%
7) Chloroethane-d5	2.899	69	69932	17.141	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	68.560%
11) 1,1-Dichloroethene-d2	4.021	65	39130	16.756	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	67.040%
21) 2-Butanone-d5	7.075	46	53711	49.479	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.960%
24) Chloroform-d	7.648	84	177207	18.573	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	74.280%
26) 1,2-Dichloroethane-d4	8.307	65	103106	20.526	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	82.120%
32) Benzene-d6	8.276	84	362513	19.002	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	76.000%
36) 1,2-Dichloropropane-d6	9.270	67	114444	19.785	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	79.160%
41) Toluene-d8	10.325	98	320660	18.835	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	75.360%
43) trans-1,3-Dichloroprop...	10.575	79	42706	19.214	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	76.840%
47) 2-Hexanone-d5	10.922	63	37831	49.561	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	99.120%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	89501	22.273	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	89.080%
66) 1,2-Dichlorobenzene-d4	13.848	152	107998	21.164	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	84.640%
Target Compounds						
39) cis-1,3-Dichloropropene	10.032	75	3170	0.431	ug/L	Qvalue # 58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060724\
Data File : VW029068.D
Acq On : 07 Jun 2024 17:29
Operator : SY/MD
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Jun 07 23:12:10 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 07 23:05:54 2024
Response via : Initial Calibration

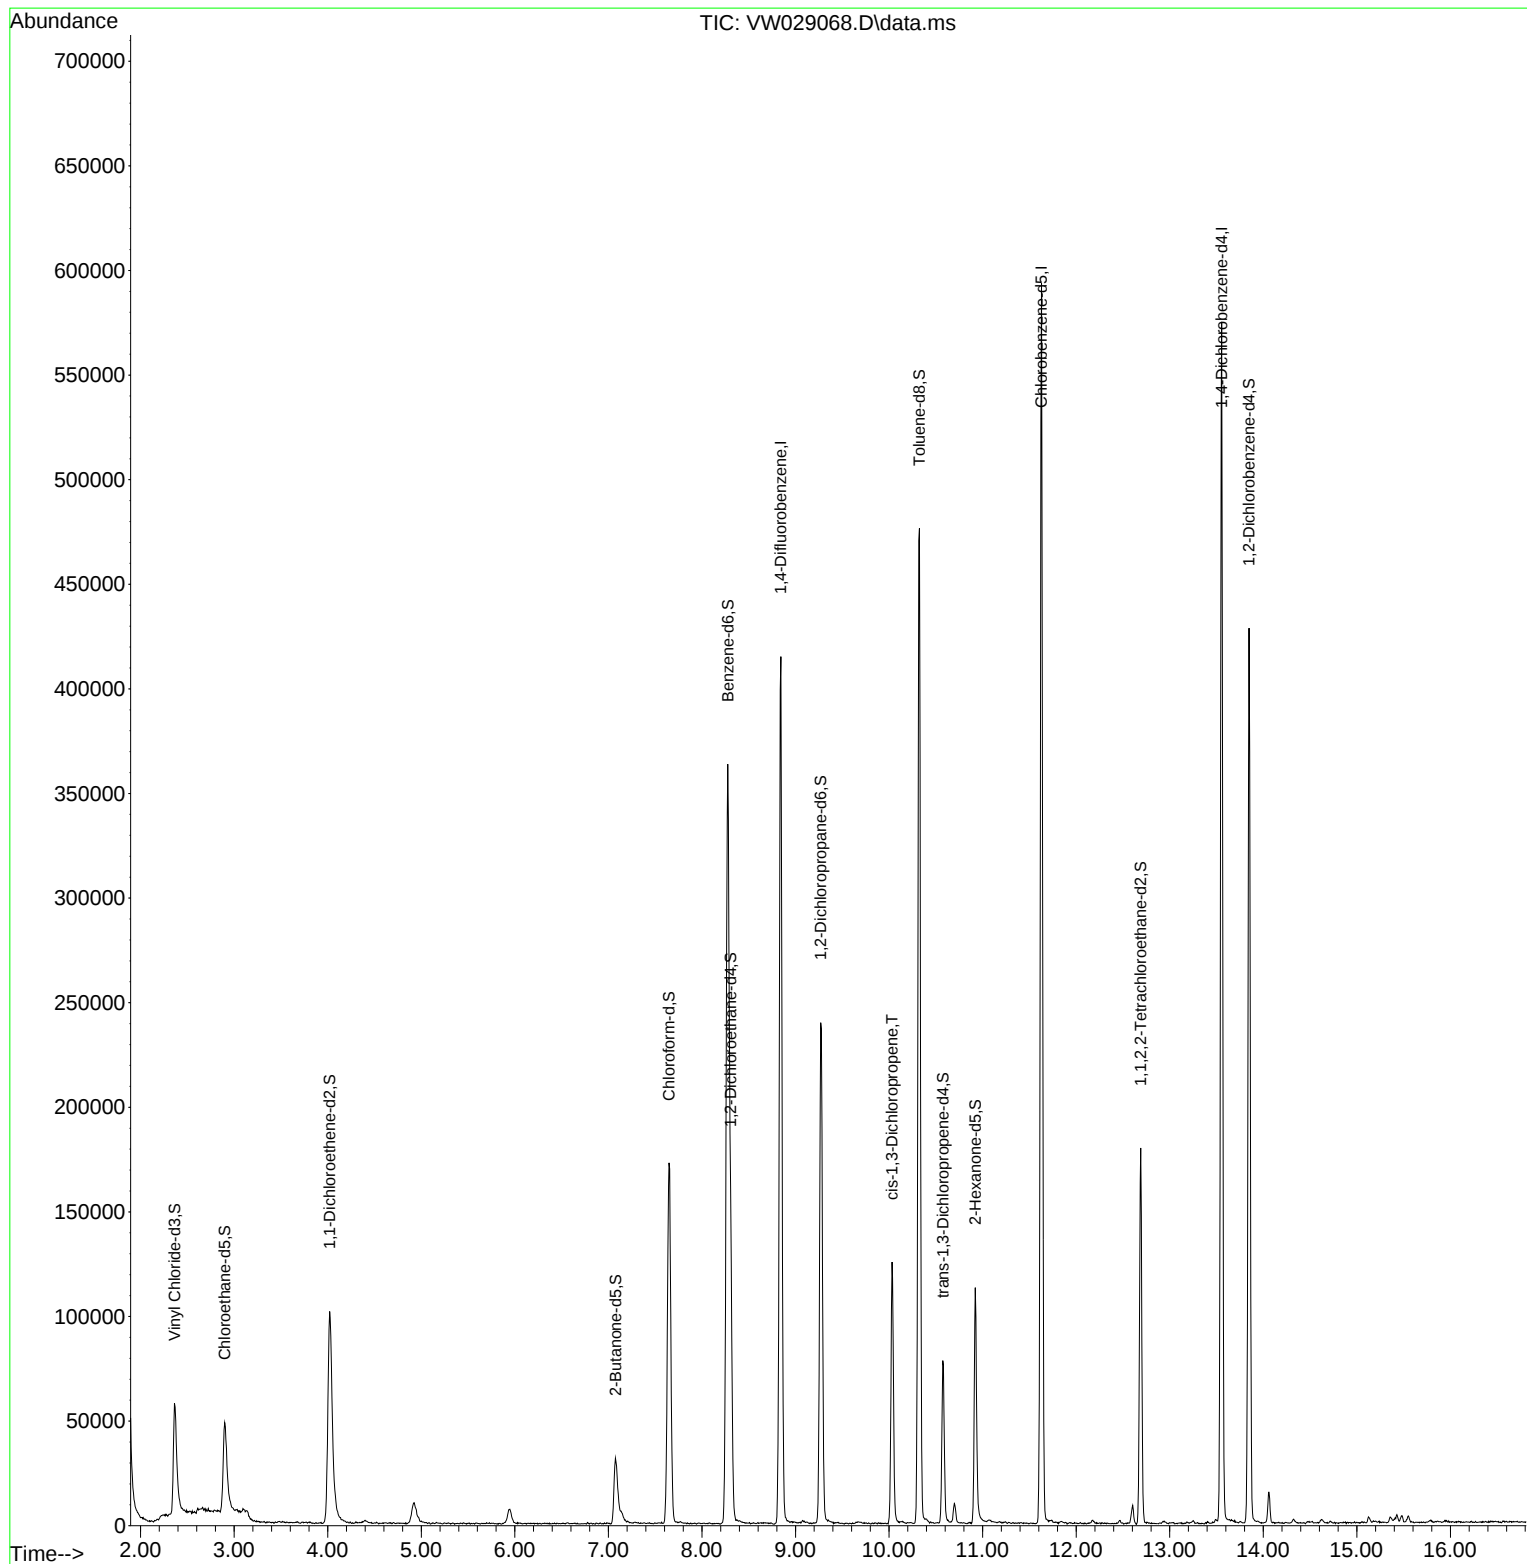

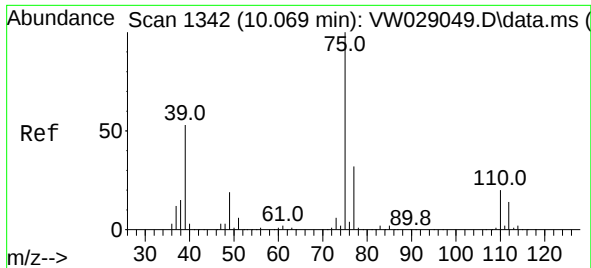

#39
 cis-1,3-Dichloropropene
 Concen: 0.431 ug/L
 RT: 10.032 min Scan# 14
 Delta R.T. -0.037 min
 Lab File: VW029068.D
 Acq: 07 Jun 2024 17:29

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 3170
 Ion Ratio Lower Upper
 75 100
 77 52.5 21.0 39.0#

