

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060724\
 Data File : VW029069.D
 Acq On : 07 Jun 2024 17:53
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Jun 07 23:12:23 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 07 23:05:54 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	305789	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	294962	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	132899	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	90229	18.574	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	74.280%		
7) Chloroethane-d5	2.899	69	73669	19.749	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	79.000%		
11) 1,1-Dichloroethene-d2	4.021	65	42090	19.713	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	78.840%		
21) 2-Butanone-d5	7.075	46	58769	59.211	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	118.420%		
24) Chloroform-d	7.648	84	193575	22.189	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	88.760%		
26) 1,2-Dichloroethane-d4	8.307	65	111408	24.257	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	97.040%		
32) Benzene-d6	8.276	84	391944	21.650	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	86.600%		
36) 1,2-Dichloropropane-d6	9.270	67	122733	22.359	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	89.440%		
41) Toluene-d8	10.319	98	339363	21.006	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	84.040%		
43) trans-1,3-Dichloroprop...	10.575	79	45790	21.709	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	86.840%		
47) 2-Hexanone-d5	10.922	63	40897	56.459	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	112.920%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	100547	26.367	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	105.480%		
66) 1,2-Dichlorobenzene-d4	13.849	152	114683	24.318	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	97.280%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	3514	0.503	ug/L	# 83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060724\
Data File : VW029069.D
Acq On : 07 Jun 2024 17:53
Operator : SY/MD
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Jun 07 23:12:23 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 07 23:05:54 2024
Response via : Initial Calibration

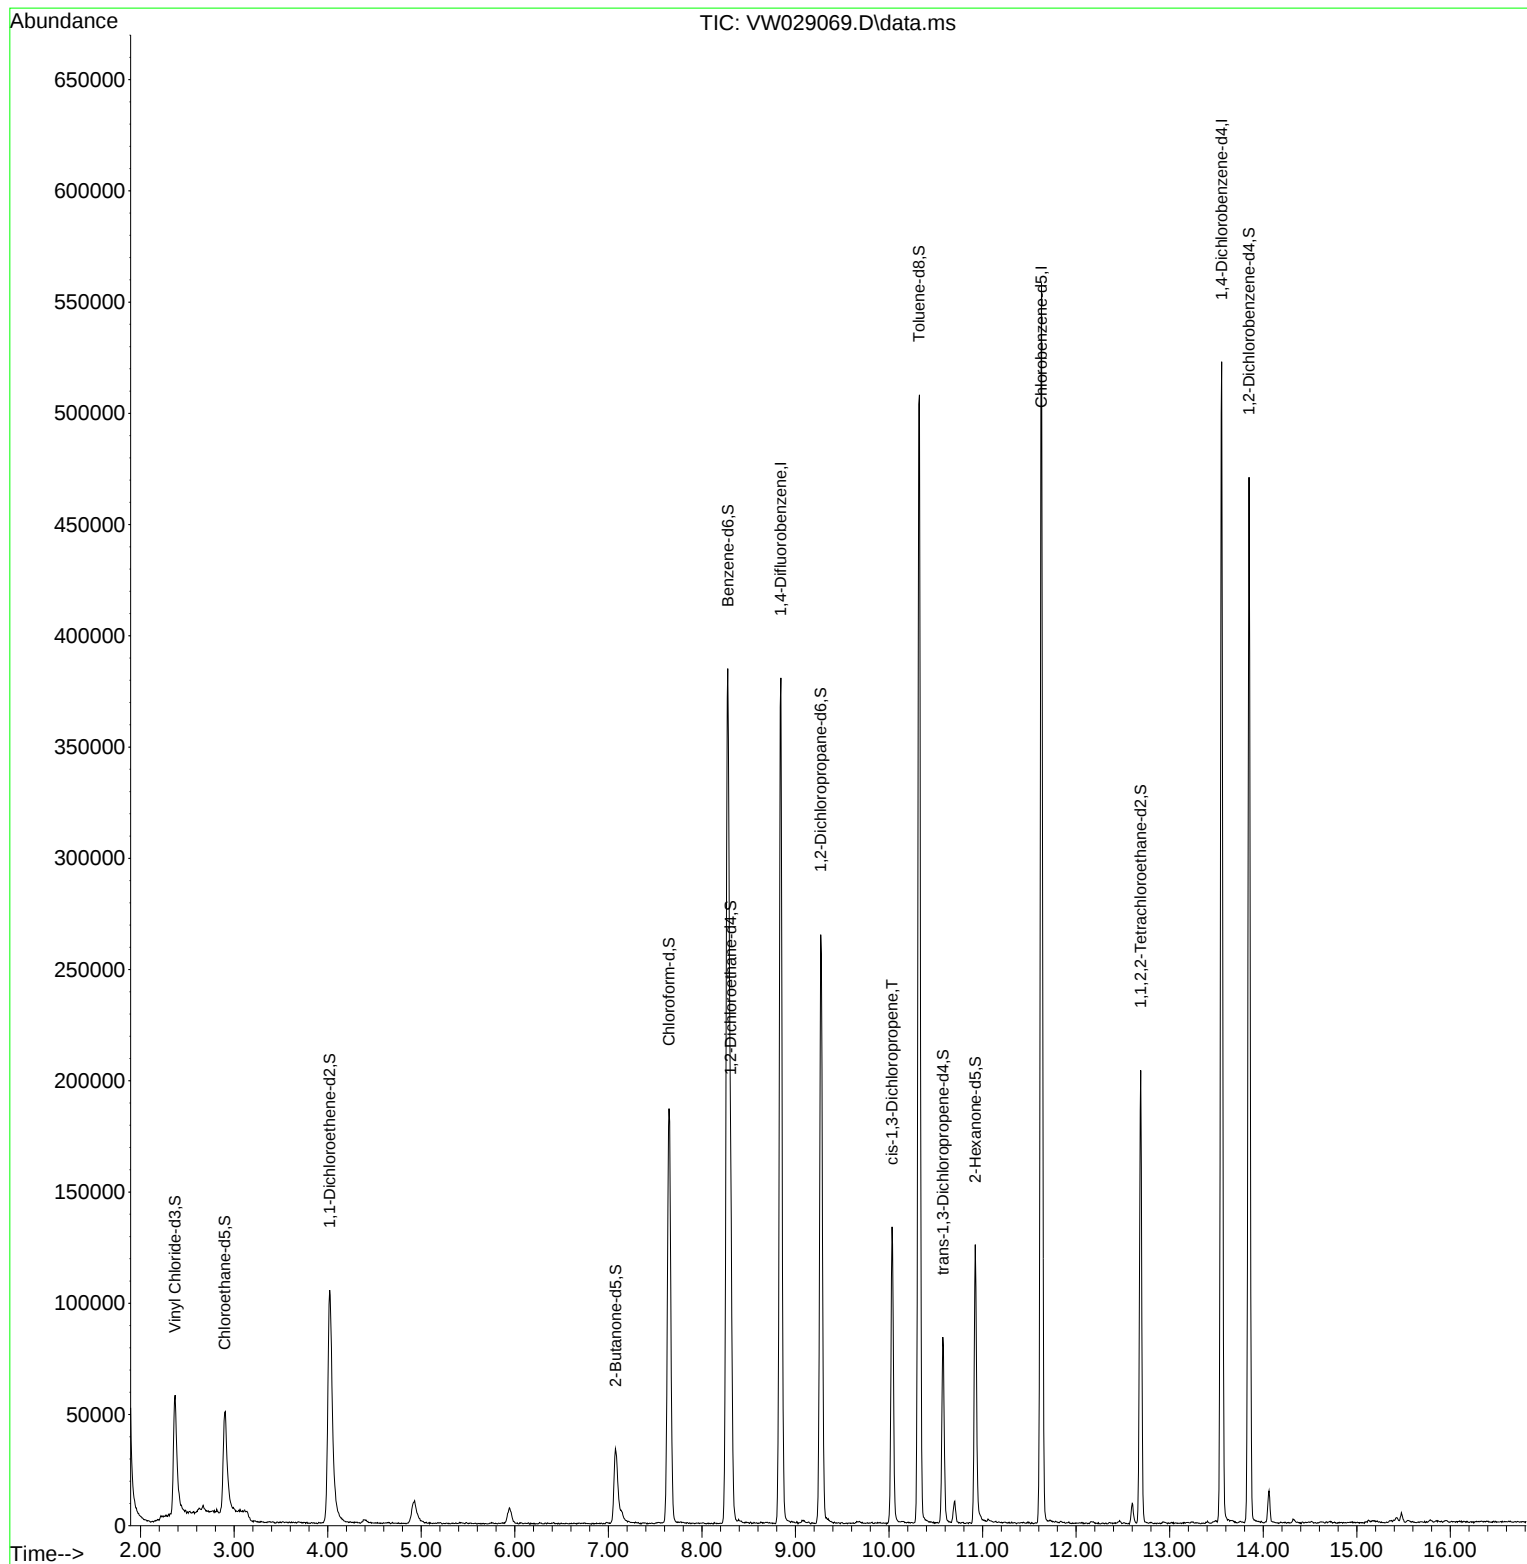

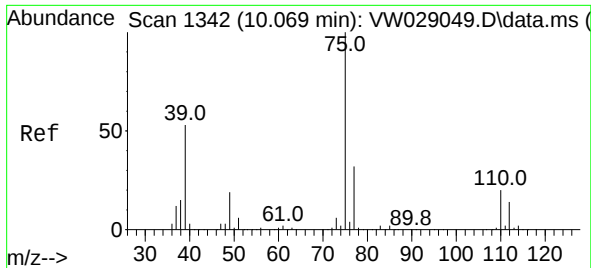

#39
 cis-1,3-Dichloropropene
 Concen: 0.503 ug/L
 RT: 10.032 min Scan# 14
 Delta R.T. -0.037 min
 Lab File: VW029069.D
 Acq: 07 Jun 2024 17:53

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 3514
 Ion Ratio Lower Upper
 75 100
 77 39.3 21.0 39.0#

