




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060724\
 Data File : VW029053.D
 Acq On : 07 Jun 2024 11:29
 Operator : SY/MD
 Sample : P2696-21
 Misc : 5.47g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4B90

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/10/2024
 Supervised By :Mahesh Dadoda 06/10/2024

Quant Time: Jun 07 23:07:08 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 07 23:05:54 2024
 Response via : Initial Calibration

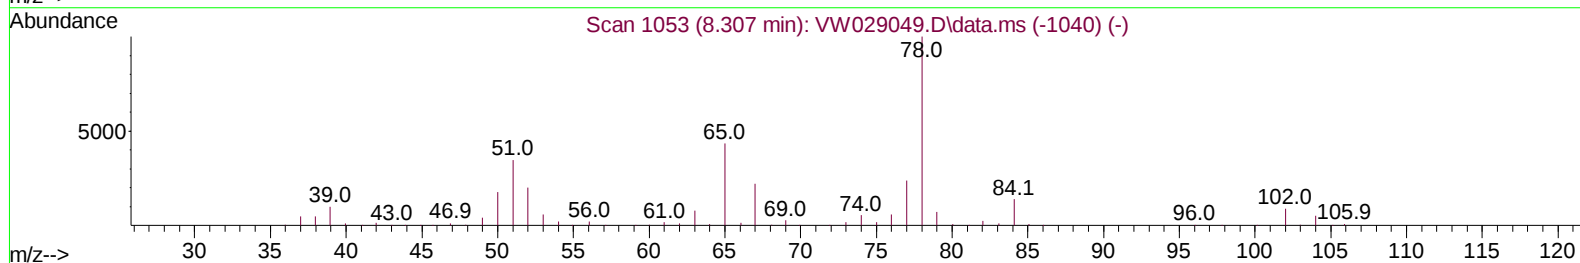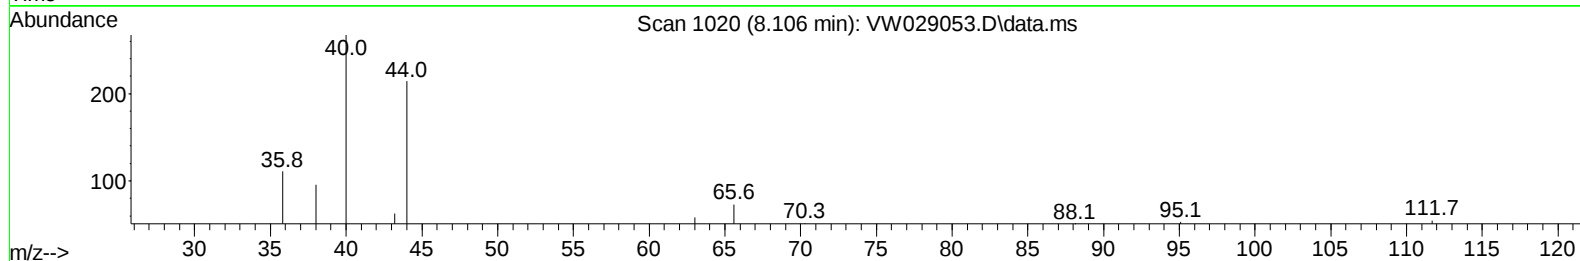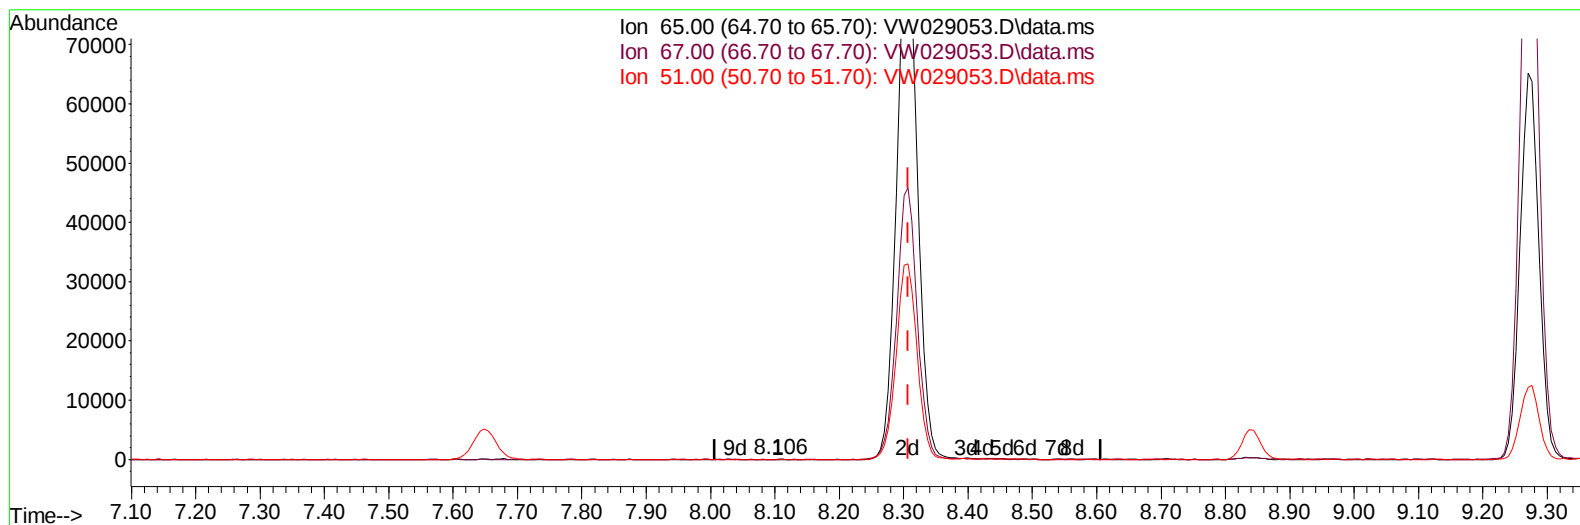

TIC: VW029053.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.106min (-0.201) 0.01 ug/L

response 48

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.90	52.08
51.00	105.10	118.75
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060724\
 Data File : VW029053.D
 Acq On : 07 Jun 2024 11:29
 Operator : SY/MD
 Sample : P2696-21
 Misc : 5.47g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4B90

Manual IntegrationsAPPROVED

Quant Time: Jun 07 23:07:08 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 07 23:05:54 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/10/2024
 Supervised By :Mahesh Dadoda 06/10/2024

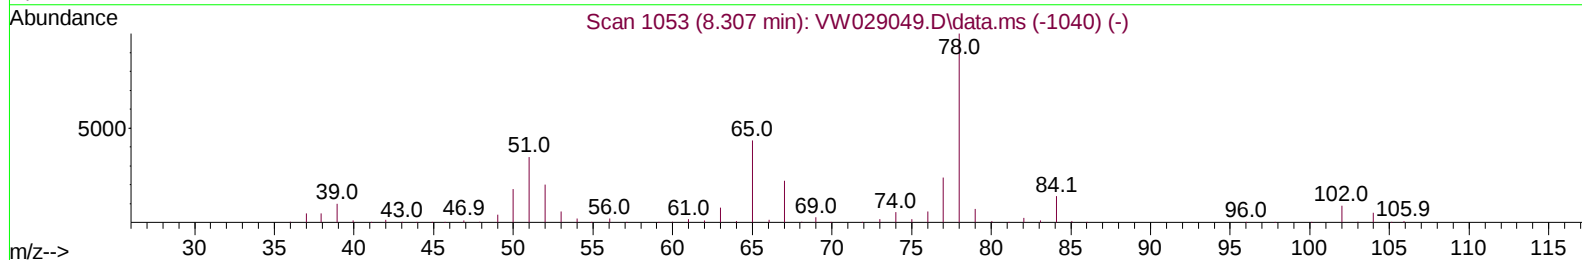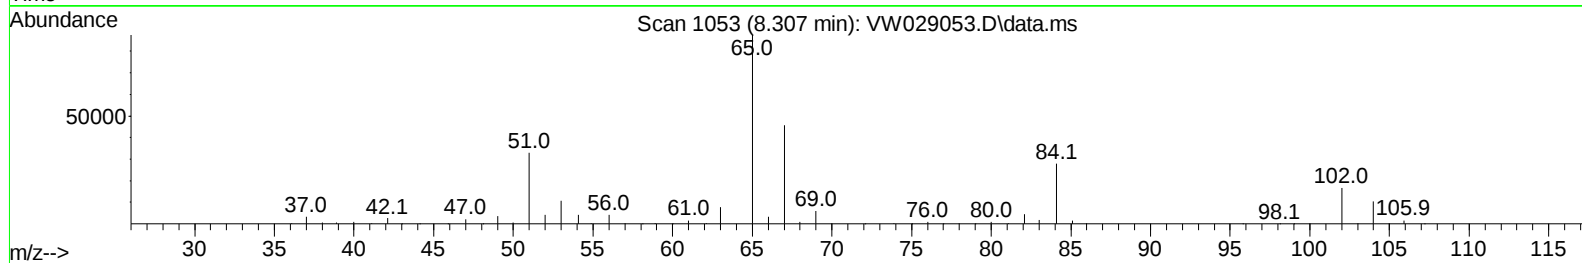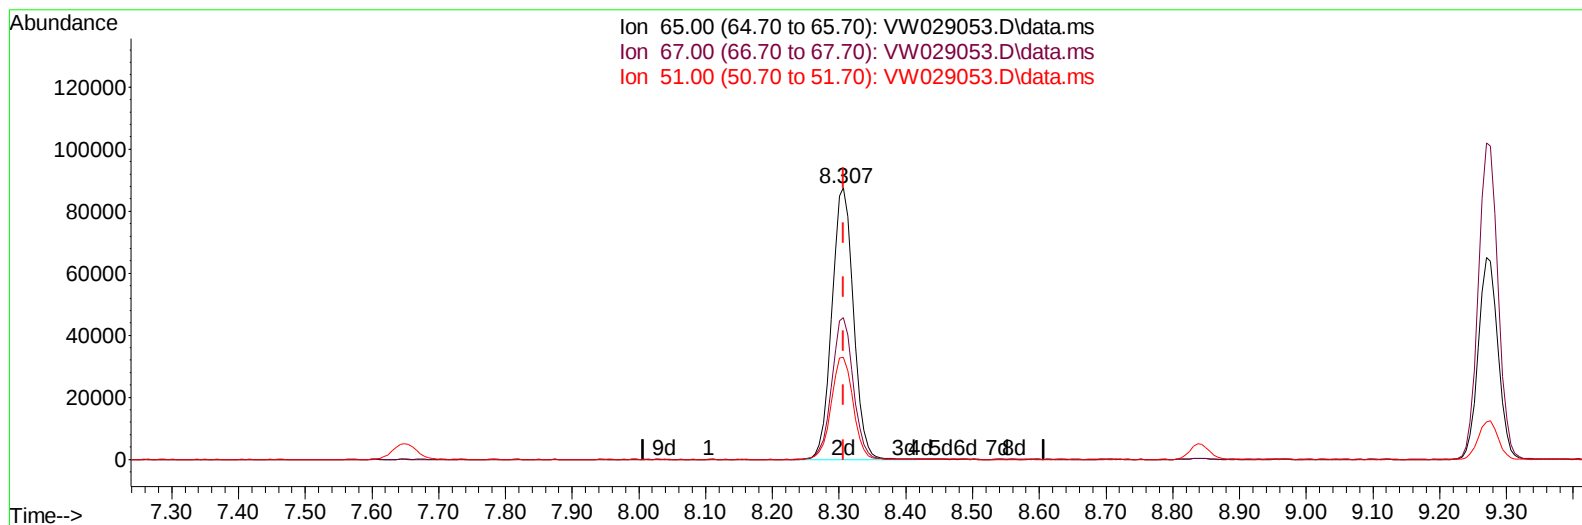

TIC: VW029053.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (-0.000) 28.09 ug/L m

response 196978

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.90	0.01#
51.00	105.10	0.03#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060724\
 Data File : VW029053.D
 Acq On : 07 Jun 2024 11:29
 Operator : SY/MD
 Sample : P2696-21
 Misc : 5.47g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4B90

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/10/2024
 Supervised By :Mahesh Dadoda 06/10/2024

Quant Time: Jun 07 23:07:08 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 07 23:05:54 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		466847	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		373740	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		120746	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		165863	22.364	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	89.440%	
7) Chloroethane-d5	2.899	69		136600	23.985	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	95.960%	
11) 1,1-Dichloroethene-d2	4.021	65		72481	22.235	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	88.960%	
21) 2-Butanone-d5	7.081	46		100437	66.282	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	132.560%	
24) Chloroform-d	7.648	84		323305	24.274	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	97.080%	
26) 1,2-Dichloroethane-d4	8.307	65		196978m	28.092	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	112.360%	
32) Benzene-d6	8.276	84		655021	28.555	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	114.200%	
36) 1,2-Dichloropropane-d6	9.270	67		208072	29.916	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	119.680%	
41) Toluene-d8	10.325	98		530887	25.934	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	103.720%	
43) trans-1,3-Dichloroprop...	10.575	79		73761	27.599	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	110.400%	
47) 2-Hexanone-d5	10.922	63		74576	81.253	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	162.500%#	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		147302	30.486	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	121.960%#	
66) 1,2-Dichlorobenzene-d4	13.848	152		108201	25.252	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	101.000%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060724\
Data File : VW029053.D
Acq On : 07 Jun 2024 11:29
Operator : SY/MD
Sample : P2696-21
Misc : 5.47g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4B90

Manual IntegrationsAPPROVED

Quant Time: Jun 07 23:07:08 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 07 23:05:54 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/10/2024
Supervised By :Mahesh Dadoda 06/10/2024

