

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060822\
 Data File : VW023433.D
 Acq On : 08 Jun 2022 17:16
 Operator : SY/VA
 Sample : N3226-10RE
 Misc : 5.05g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4N0

Quant Time: Jun 09 00:42:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 09 00:39:51 2022
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		8.842	114	323098	25.000	ug/L	0.00
28) Chlorobenzene-d5		11.634	117	279661	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		13.554	152	107769	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		2.349	65	136602	27.314	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	= 109.240%		
7) Chloroethane-d5		2.879	69	95552	27.121	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	= 108.480%		
11) 1,1-Dichloroethene-d2		4.013	63	123468	16.439	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	= 65.760%		
21) 2-Butanone-d5		7.074	46	56620	58.702	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	= 117.400%		
24) Chloroform-d		7.647	84	218078	25.031	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	= 100.120%		
26) 1,2-Dichloroethane-d4		8.305	65	131295	28.688	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	= 114.760%		
32) Benzene-d6		8.275	84	404715	26.070	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	= 104.280%		
36) 1,2-Dichloropropane-d6		9.274	67	125591	28.864	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	= 115.440%		
41) Toluene-d8		10.323	98	359330	24.304	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	= 97.200%		
43) trans-1,3-Dichloroprop...		10.579	79	48647	25.059	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	= 100.240%		
47) 2-Hexanone-d5		10.920	63	43680	67.065	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	= 134.120%		
56) 1,1,2,2-Tetrachloroeth...		12.688	84	112912	30.328	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	= 121.320%#		
66) 1,2-Dichlorobenzene-d4		13.853	152	97866	25.089	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	= 100.360%		
Target Compounds							Qvalue
39) cis-1,3-Dichloropropene		10.036	75	4421	0.734	ug/L	86
53) m,p-Xylene		11.841	106	4740	0.601	ug/L	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060822\
Data File : VW023433.D
Acq On : 08 Jun 2022 17:16
Operator : SY/VA
Sample : N3226-10RE
Misc : 5.05g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW4N0

Quant Time: Jun 09 00:42:56 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060622SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jun 09 00:39:51 2022
Response via : Initial Calibration

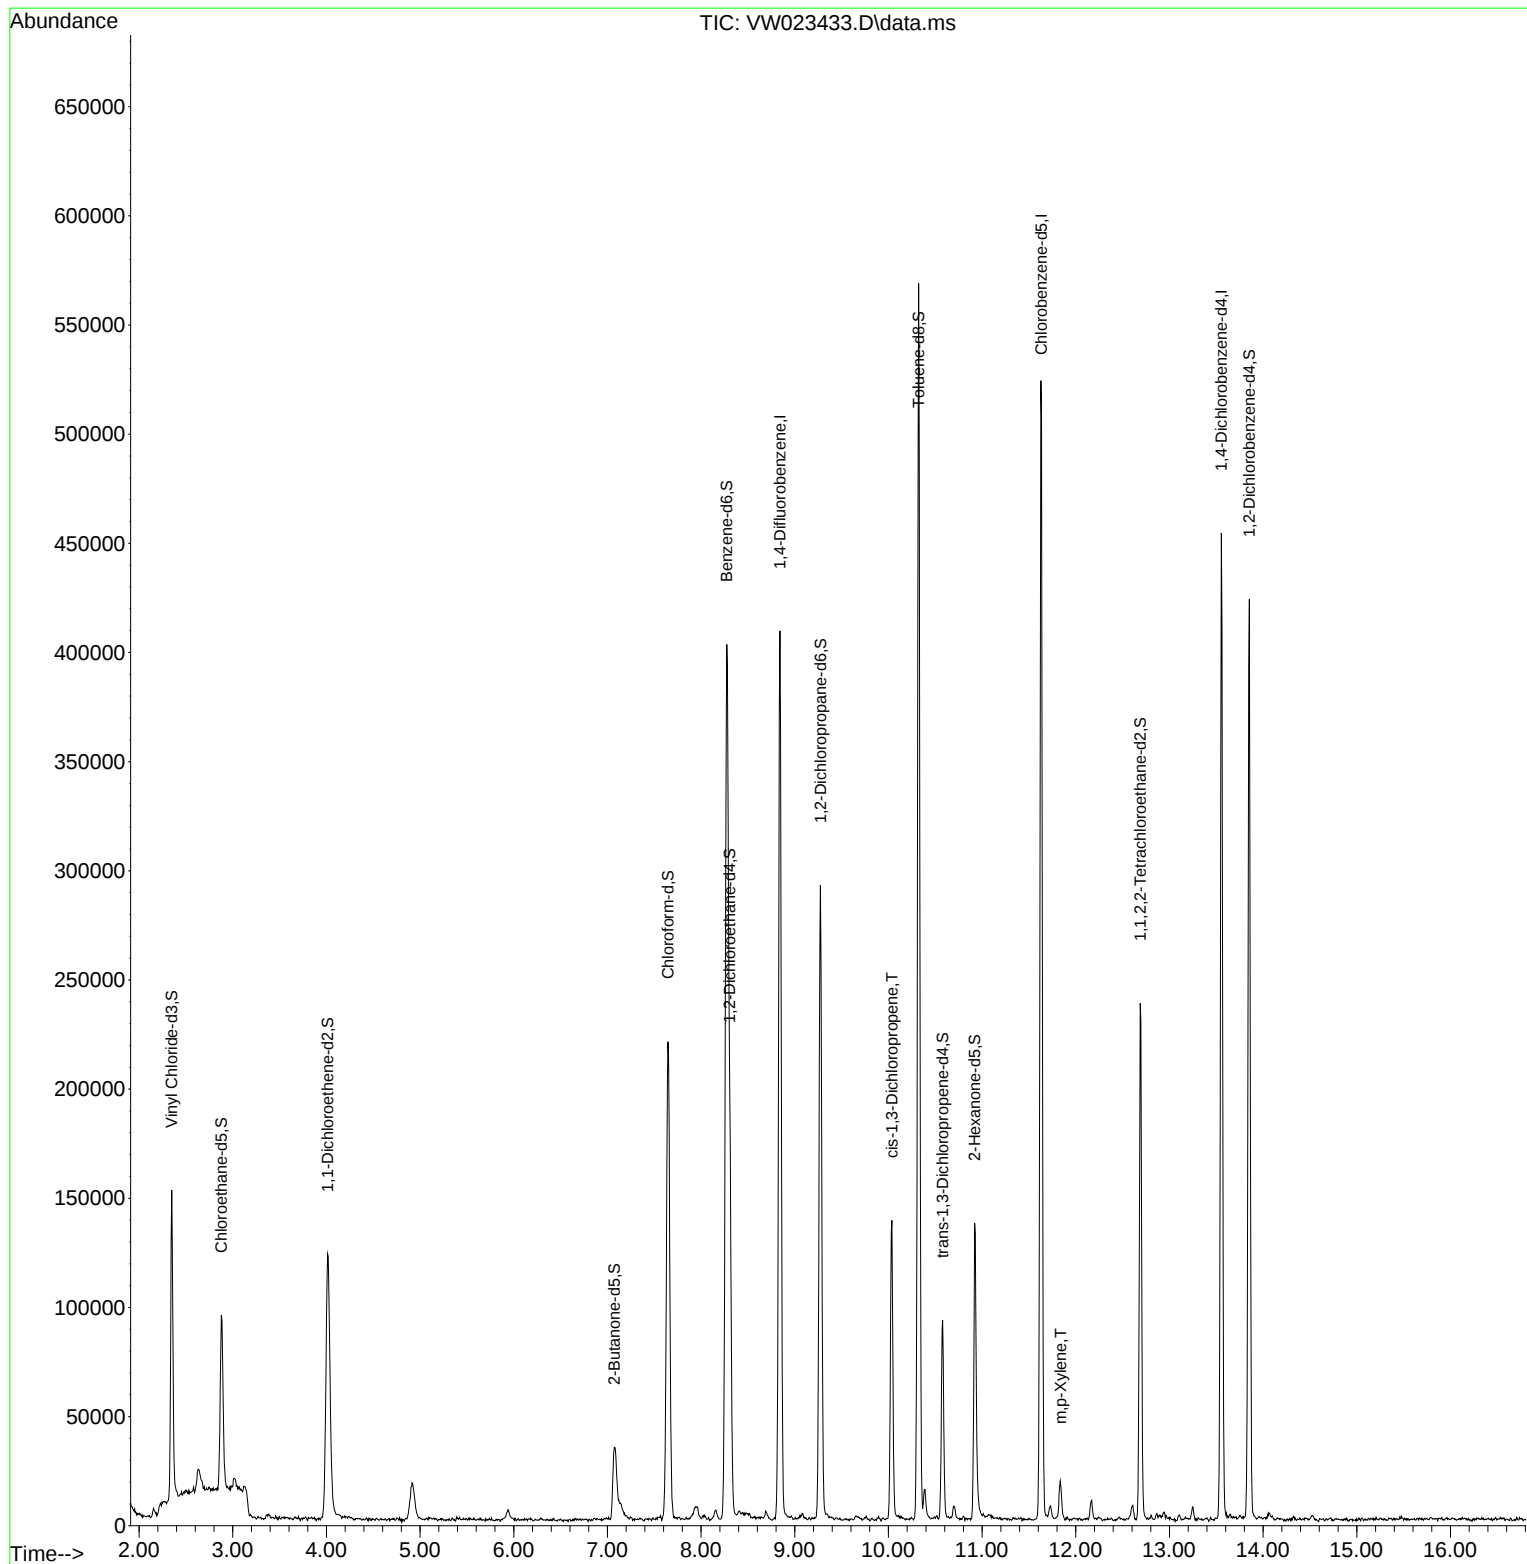

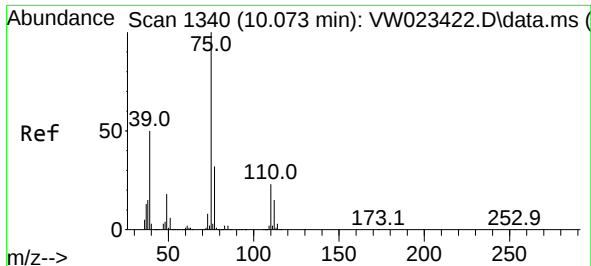

#39

cis-1,3-Dichloropropene

Concen: 0.734 ug/L

RT: 10.036 min Scan# 11

Delta R.T. -0.037 min

Lab File: VW023433.D

Acq: 08 Jun 2022 17:16

Instrument :

MSVOA_W

ClientSampleId :





EW4N0

Tgt Ion: 75 Resp: 4421

Ion Ratio Lower Upper

75 100

77 39.6 22.1 41.1

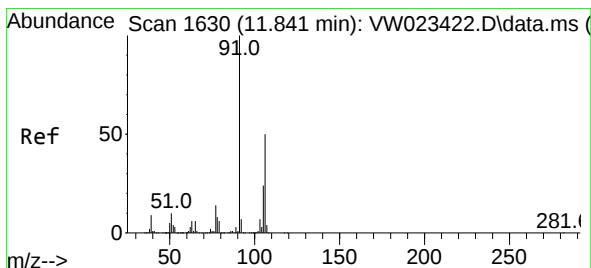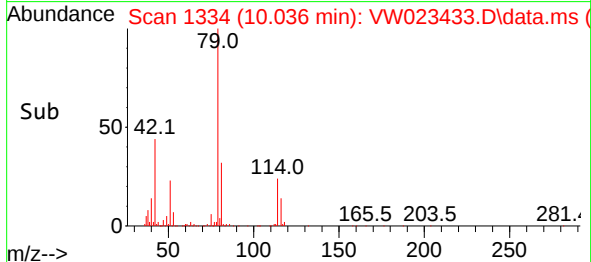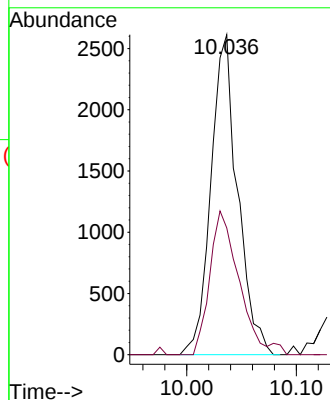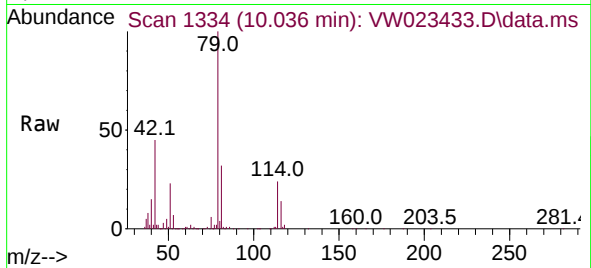

#53

m,p-Xylene

Concen: 0.601 ug/L

RT: 11.841 min Scan# 1630

Delta R.T. -0.000 min

Lab File: VW023433.D

Acq: 08 Jun 2022 17:16

Tgt Ion: 106 Resp: 4740

Ion Ratio Lower Upper

106 100

91 169.2 136.8 254.0

