

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060822\
Data File : VW023426.D
Acq On : 08 Jun 2022 14:27
Operator : SY/VA
Sample : N3226-09
Misc : 5.58g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1




Instrument :
MSVOA_W
ClientSampleId :
EW4M9

Manual IntegrationsAPPROVED

Quant Time: Jun 09 00:41:21 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060622SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jun 09 00:39:51 2022
Response via : Initial Calibration

Reviewed By :Semsettin
Yesilyurt

06/09/2022
Supervised By :Mahesh
Dadoda

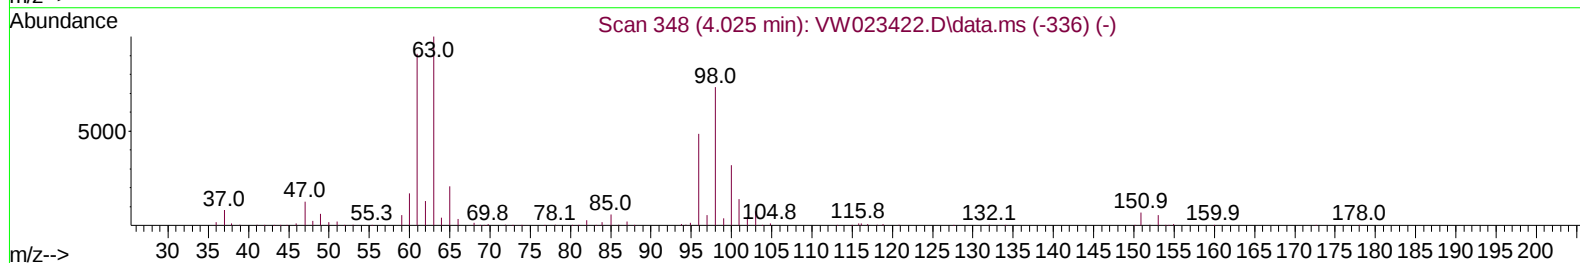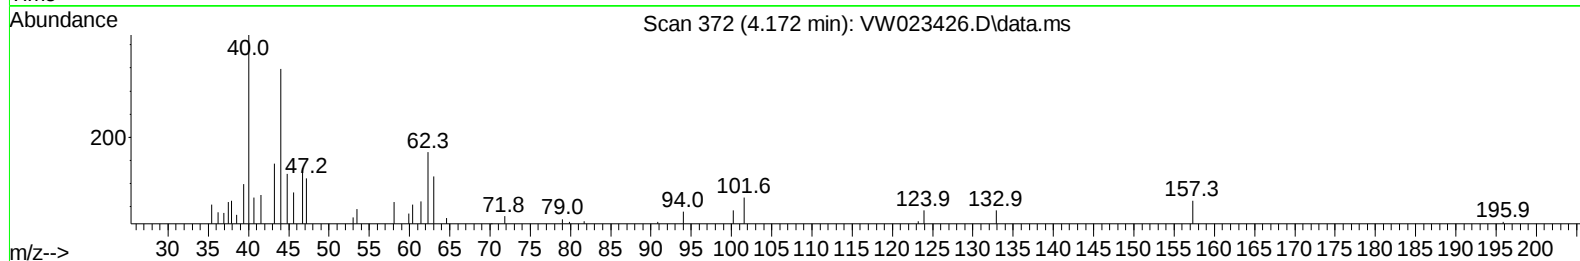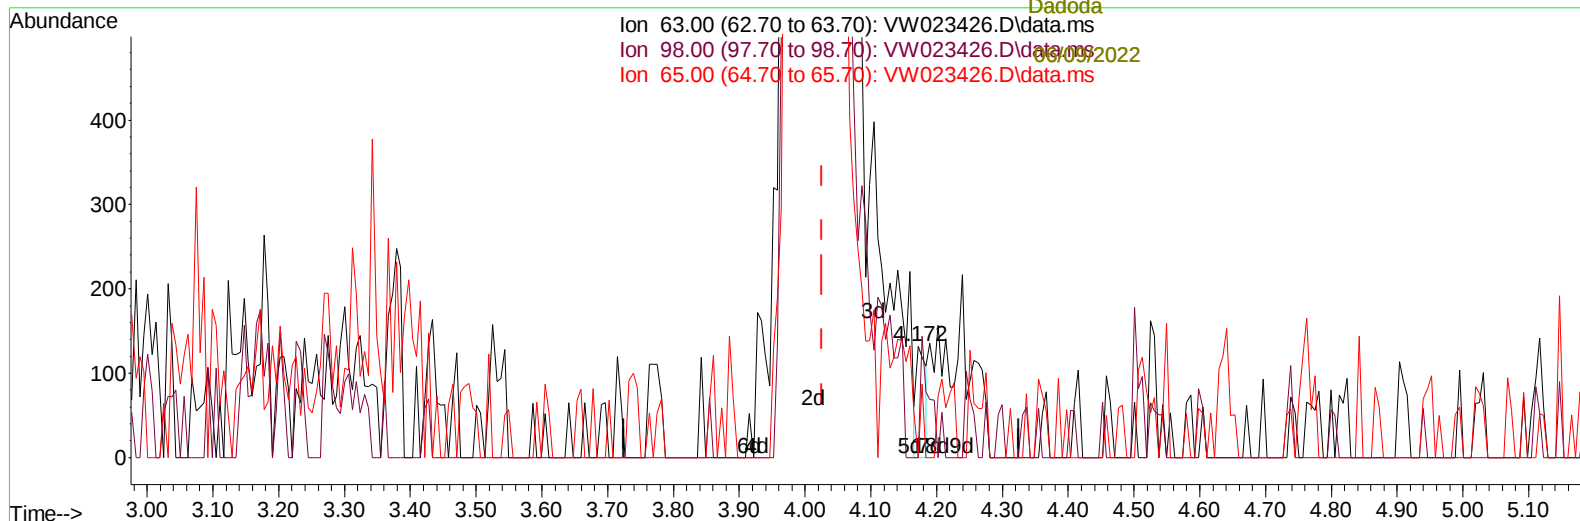

TIC: VW023426.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.172min (+ 0.146) 0.02 ug/L

response 131

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	72.80	81.68
65.00	23.30	24.43
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060822\
 Data File : VW023426.D
 Acq On : 08 Jun 2022 14:27
 Operator : SY/VA
 Sample : N3226-09
 Misc : 5.58g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4M9




Manual IntegrationsAPPROVED

Quant Time: Jun 09 00:41:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 09 00:39:51 2022
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

06/09/2022
 Supervised By :Mahesh
 Dadoda

Ion 63.00 (62.70 to 63.70): VW023426.D\data.ms
 Ion 98.00 (97.70 to 98.70): VW023426.D\data.ms
 Ion 65.00 (64.70 to 65.70): VW023426.D\data.ms

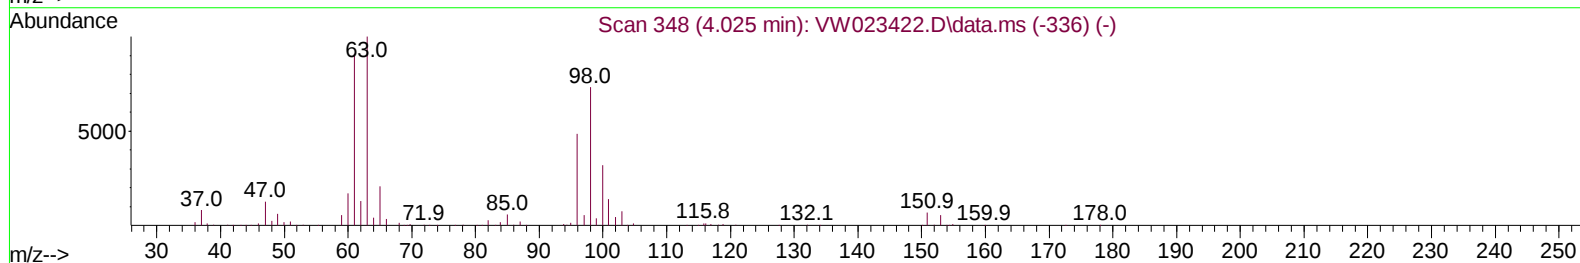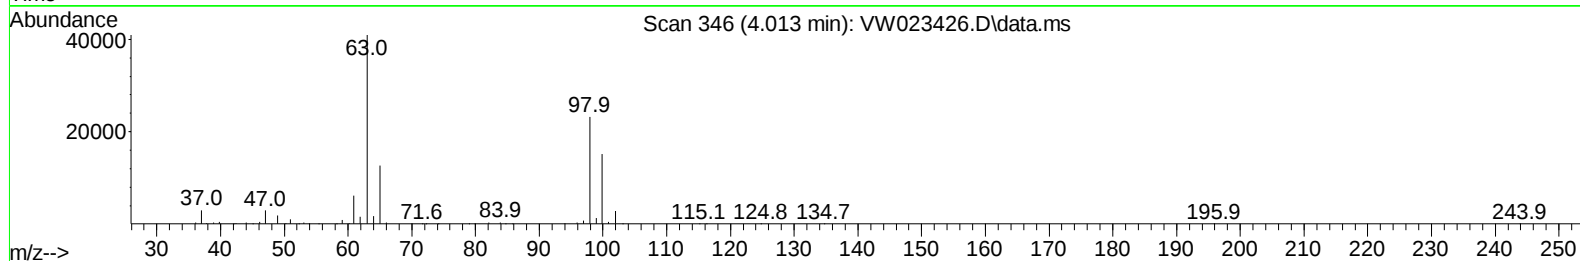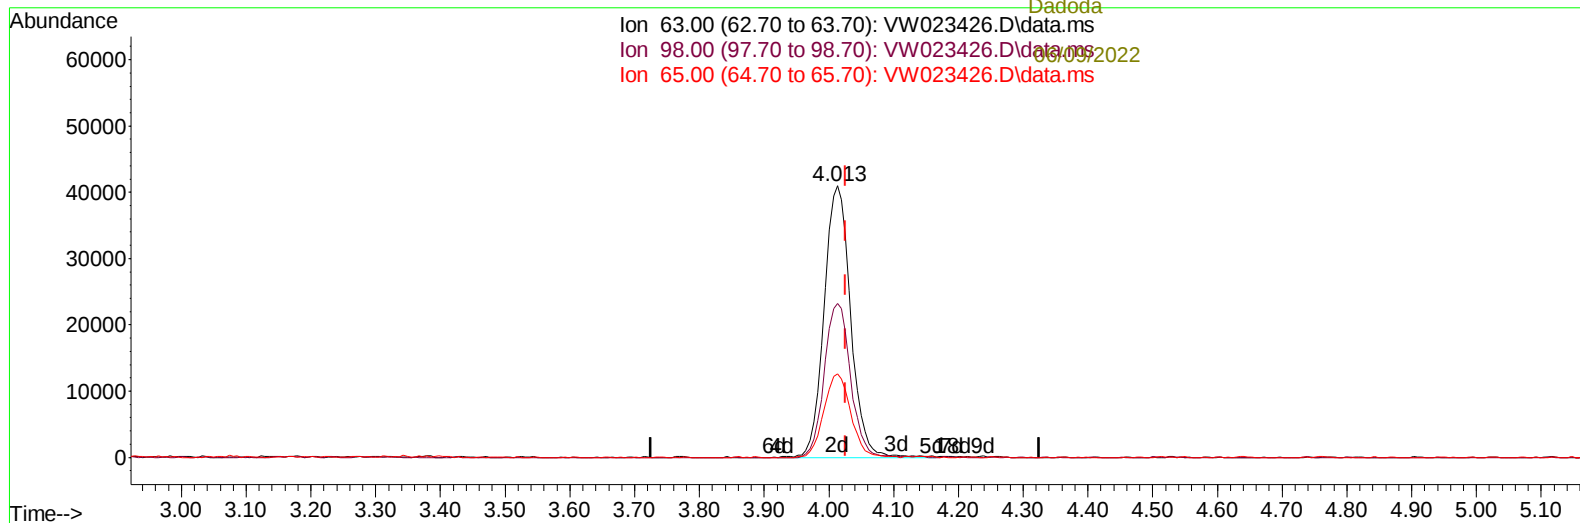

TIC: VW023426.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.013min (-0.012) 16.34 ug/L m

response 116711

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	72.80	0.09#
65.00	23.30	0.03#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060822\
 Data File : VW023426.D
 Acq On : 08 Jun 2022 14:27
 Operator : SY/VA
 Sample : N3226-09
 Misc : 5.58g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 EW4M9

Manual IntegrationsAPPROVED

Quant Time: Jun 09 00:41:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 09 00:39:51 2022
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

06/09/2022
 Supervised By :Mahesh
 Dadoda

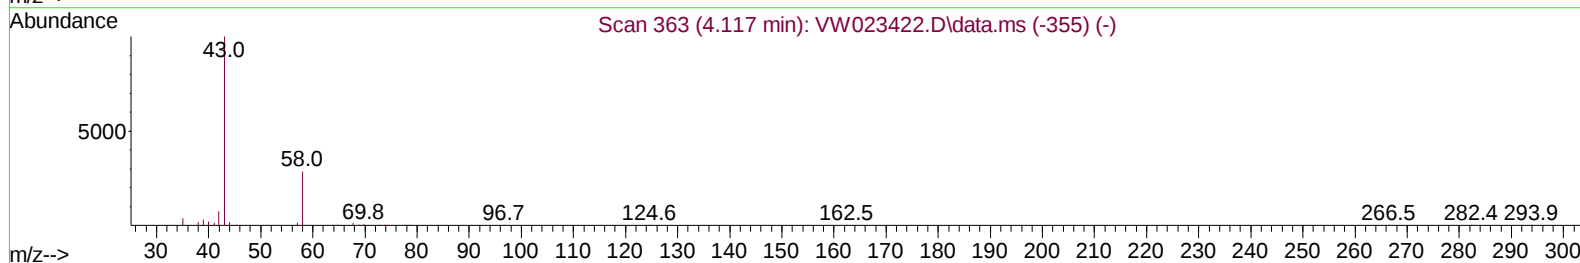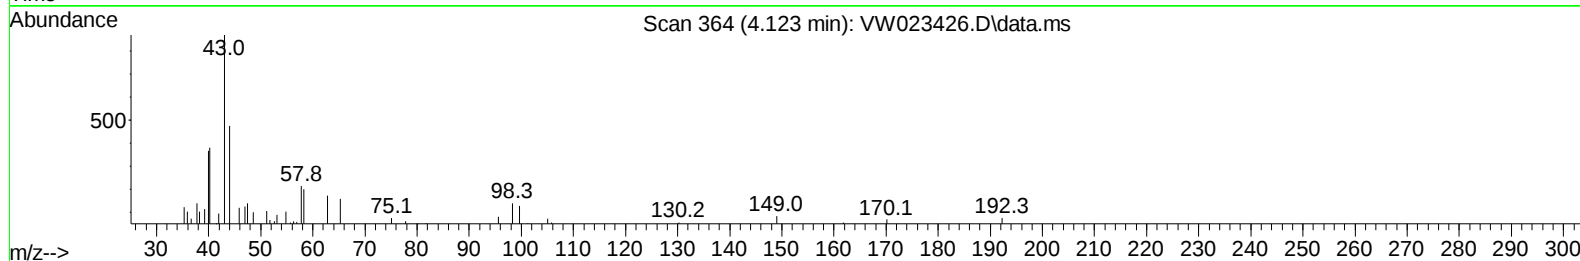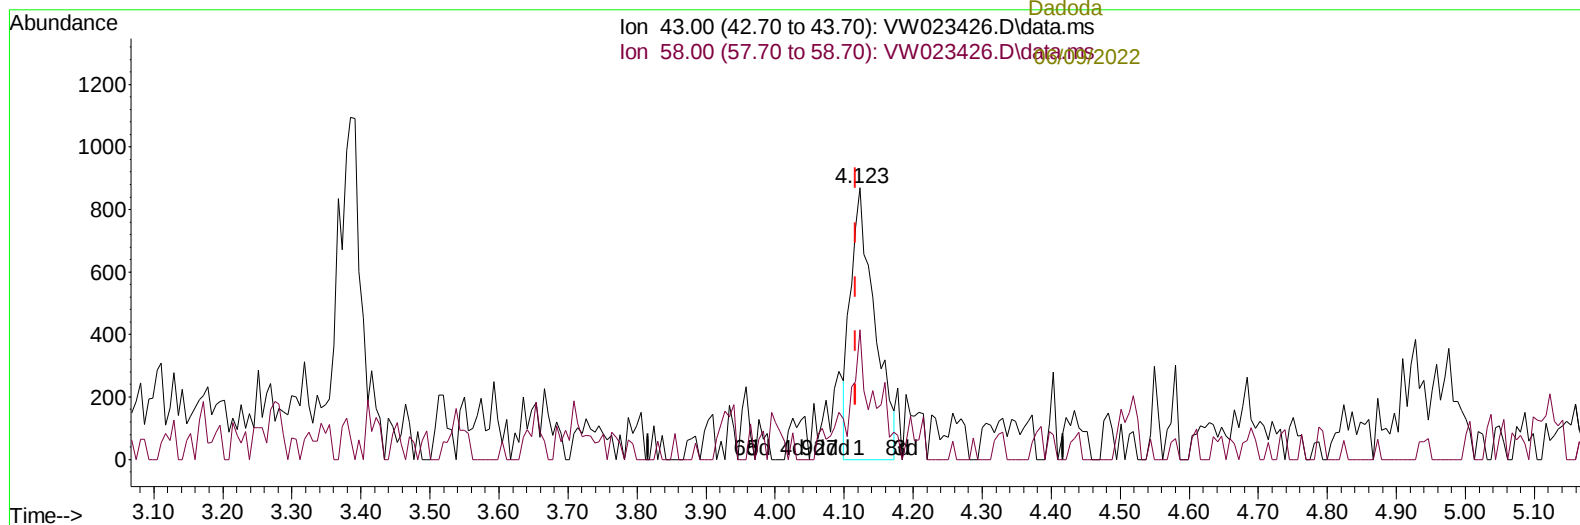

TIC: VW023426.D\data.ms

(13) Acetone (T)

4.123min (+ 0.006) 3.06 ug/L

response 2103

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	22.11
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060822\
 Data File : VW023426.D
 Acq On : 08 Jun 2022 14:27
 Operator : SY/VA
 Sample : N3226-09
 Misc : 5.58g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 EW4M9

Manual IntegrationsAPPROVED

Quant Time: Jun 09 00:41:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 09 00:39:51 2022
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

06/09/2022
 Supervised By :Mahesh
 Dadoda

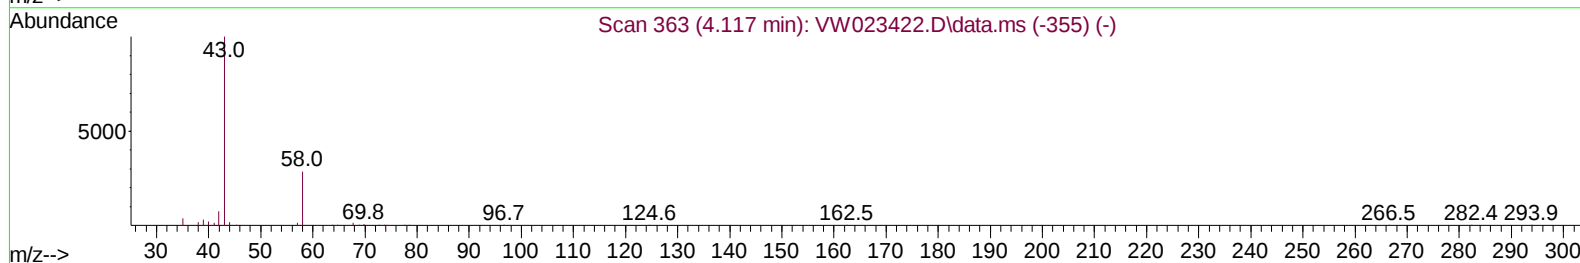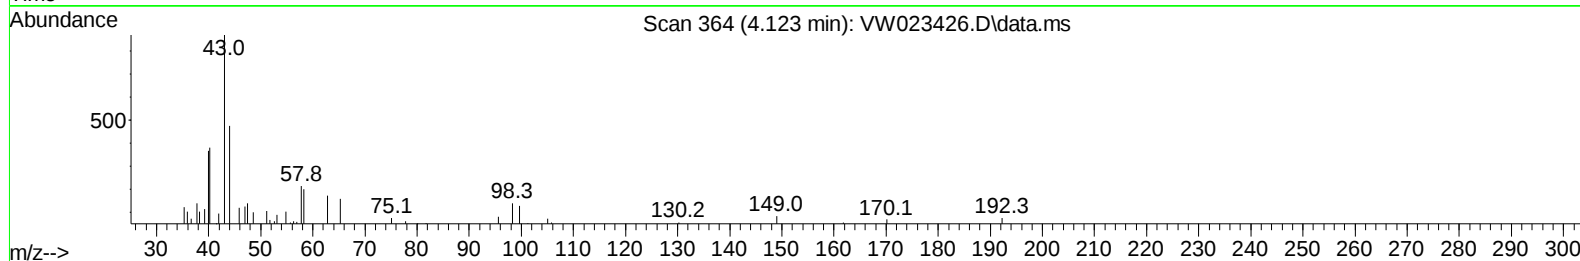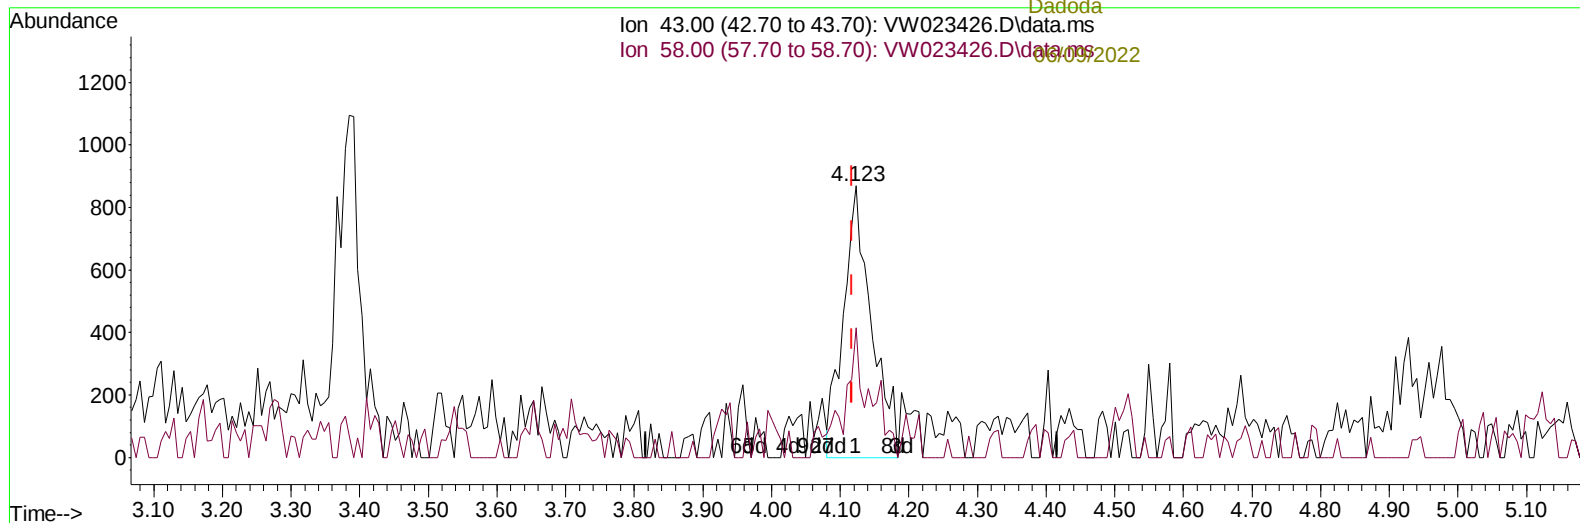

TIC: VW023426.D\data.ms

(13) Acetone (T)

4.123min (+ 0.006) 3.58 ug/L m

response 2465

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	18.86
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060822\
 Data File : VW023426.D
 Acq On : 08 Jun 2022 14:27
 Operator : SY/VA
 Sample : N3226-09
 Misc : 5.58g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 EW4M9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin
 Yesilyurt

06/09/2022
 Supervised By :Mahesh
 Dadoda

Quant Time: Jun 09 00:41:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 09 00:39:51 2022
 Response via : Initial Calibration

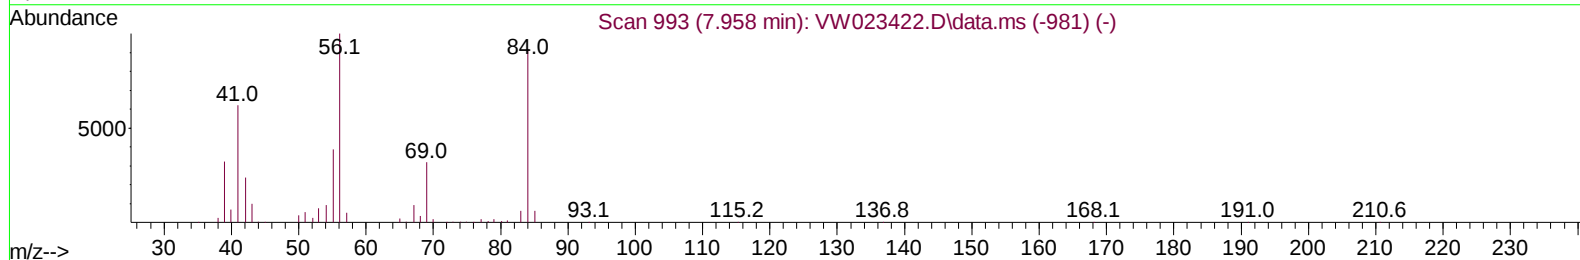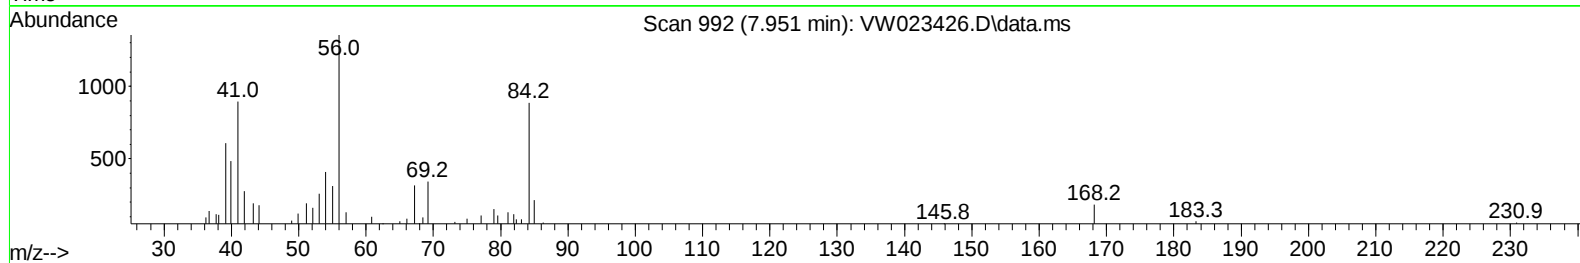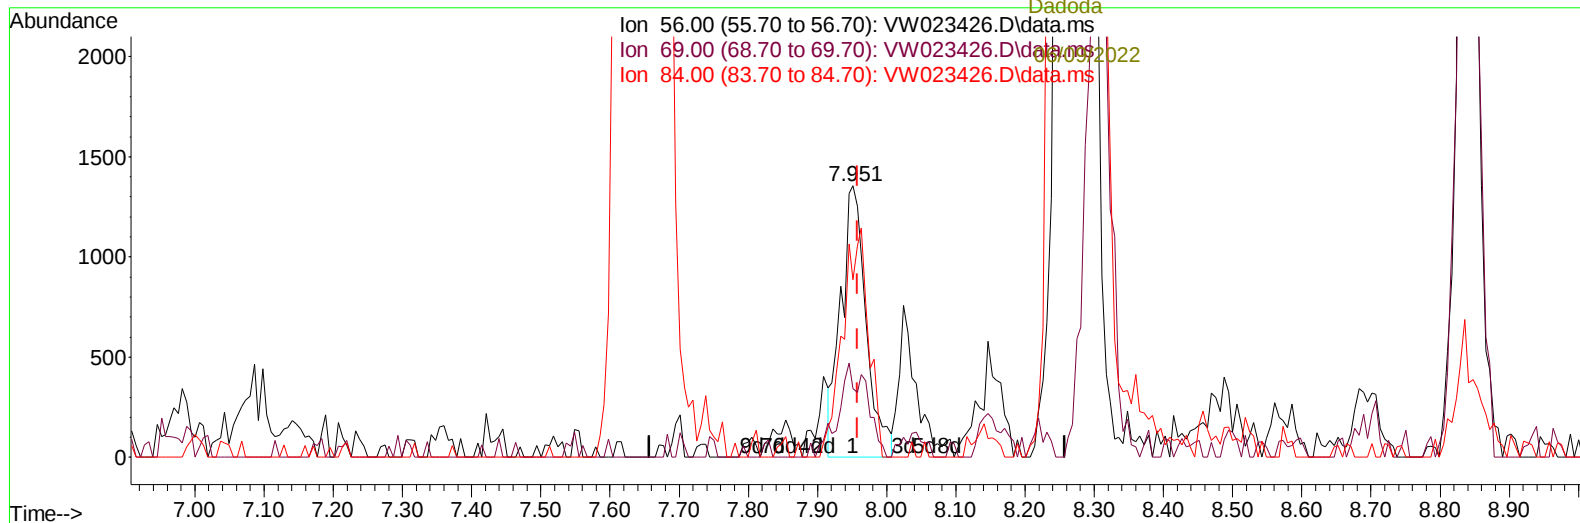

TIC: VW023426.D\data.ms

(29) Cyclohexane (T)

7.951min (-0.006) 0.72 ug/L

response 3447

Ion	Exp%	Act%
56.00	100.00	100.00
69.00	32.00	19.38#
84.00	97.80	42.30#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060822\
 Data File : VW023426.D
 Acq On : 08 Jun 2022 14:27
 Operator : SY/VA
 Sample : N3226-09
 Misc : 5.58g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 EW4M9

Manual IntegrationsAPPROVED

Quant Time: Jun 09 00:41:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 09 00:39:51 2022
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

06/09/2022
 Supervised By :Mahesh
 Dadoda

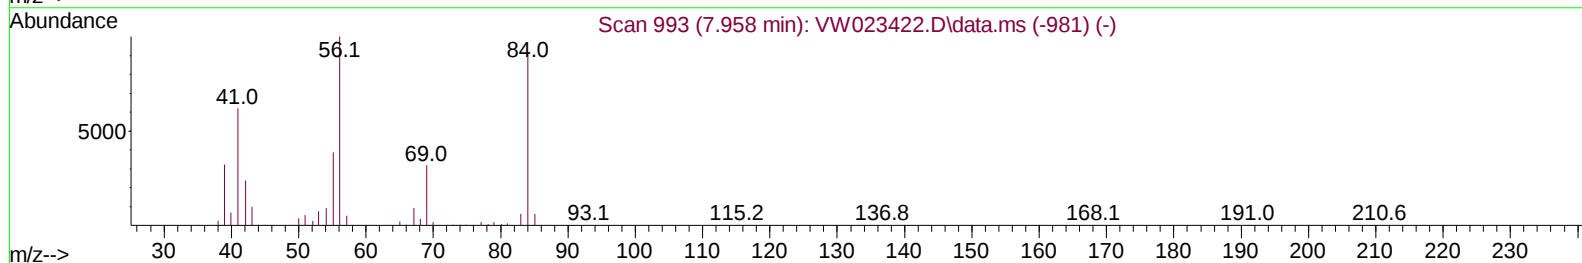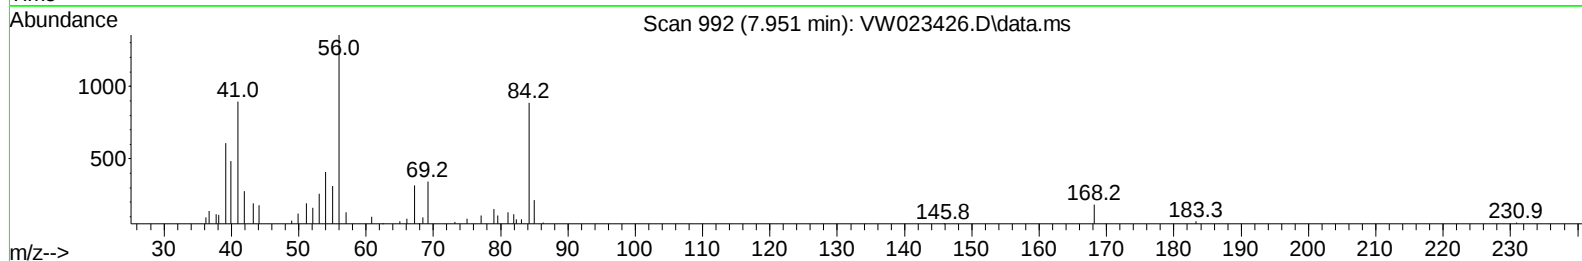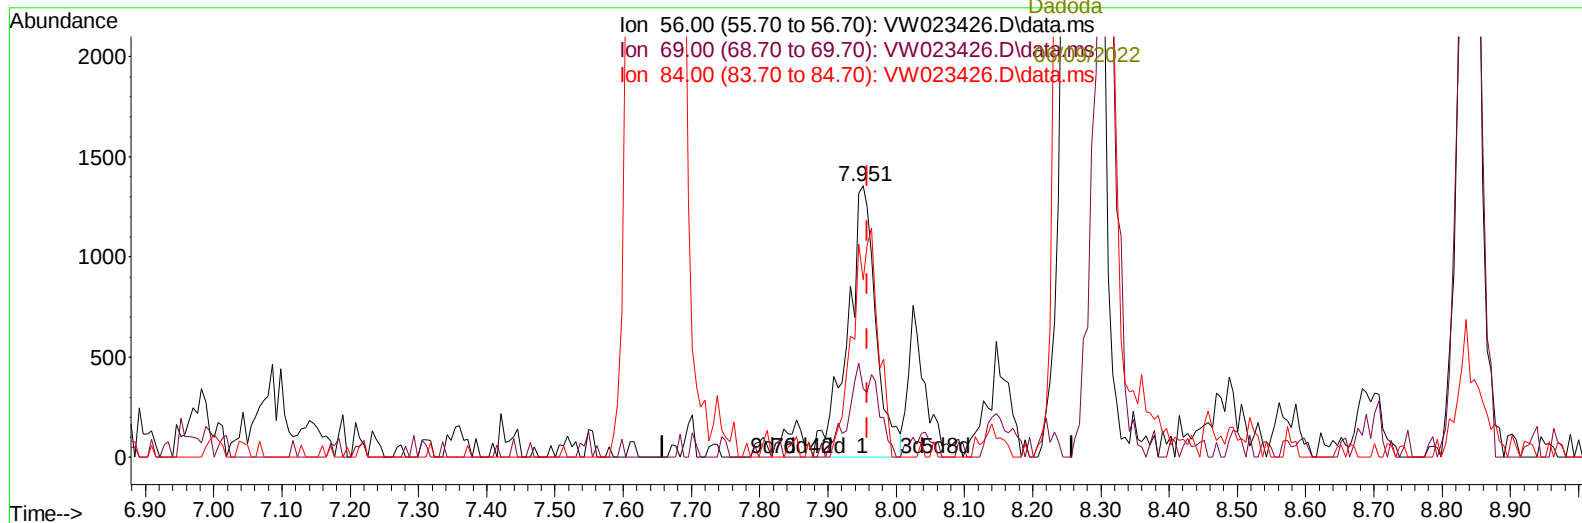

TIC: VW023426.D\data.ms

(29) Cyclohexane (T)

7.951min (-0.006) 0.82 ug/L m

response 3934

Ion	Exp%	Act%
56.00	100.00	100.00
69.00	32.00	16.98#
84.00	97.80	37.06#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060822\
 Data File : VW023426.D
 Acq On : 08 Jun 2022 14:27
 Operator : SY/VA
 Sample : N3226-09
 Misc : 5.58g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4M9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin
 Yesilyurt

06/09/2022
 Supervised By :Mahesh
 Dadoda

Quant Time: Jun 09 00:41:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 09 00:39:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----06/09/2022						
Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	307288	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	223451	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	56675	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	117560	24.716	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	98.880%	
7) Chloroethane-d5	2.885	69	78121	23.314	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	93.240%	
11) 1,1-Dichloroethene-d2	4.013	63	116711m	16.339	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110	Recovery	=	65.360%	
21) 2-Butanone-d5	7.080	46	44618	48.638	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	97.280%	
24) Chloroform-d	7.647	84	200779	24.231	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	96.920%	
26) 1,2-Dichloroethane-d4	8.305	65	113743	26.132	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	104.520%	
32) Benzene-d6	8.274	84	368746	29.728	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	118.920%	
36) 1,2-Dichloropropane-d6	9.274	67	114001	32.791	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	131.160%#	
41) Toluene-d8	10.323	98	303639	25.703	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	102.800%	
43) trans-1,3-Dichloroprop...	10.579	79	41202	26.563	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	106.240%	
47) 2-Hexanone-d5	10.920	63	31224	60.000	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	120.000%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	81425	27.373	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	109.480%	
66) 1,2-Dichlorobenzene-d4	13.853	152	48146	23.470	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	93.880%	
Target Compounds						
13) Acetone	4.123	43	2465m	3.583	ug/L	
29) Cyclohexane	7.951	56	3934m	0.824	ug/L	
53) m,p-Xylene	11.829	106	4507	0.715	ug/L	91
63) 1,2,4-Trimethylbenzene	13.249	105	3160	0.476	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060822\
Data File : VW023426.D
Acq On : 08 Jun 2022 14:27
Operator : SY/VA
Sample : N3226-09
Misc : 5.58g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW4M9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin
Yesilyurt

06/09/2022
Supervised By :Mahesh
Dadoda

Quant Time: Jun 09 00:41:21 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060622SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jun 09 00:39:51 2022
Response via : Initial Calibration

