




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060822\
Data File : VW023432.D
Acq On : 08 Jun 2022 16:52
Operator : SY/VA
Sample : N3226-09RE
Misc : 6.41g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW4M9RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/09/2022
Supervised By :Mahesh Dadoda 06/09/2022

Quant Time: Jun 09 00:42:41 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060622SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jun 09 00:39:51 2022
Response via : Initial Calibration

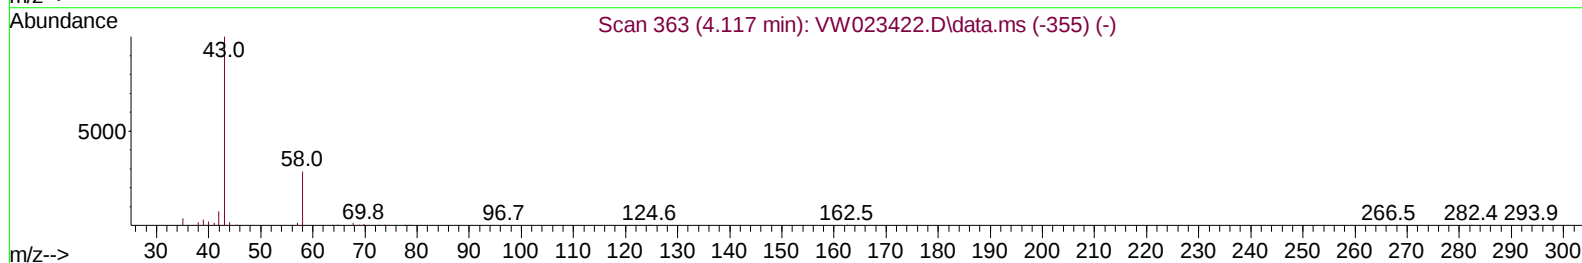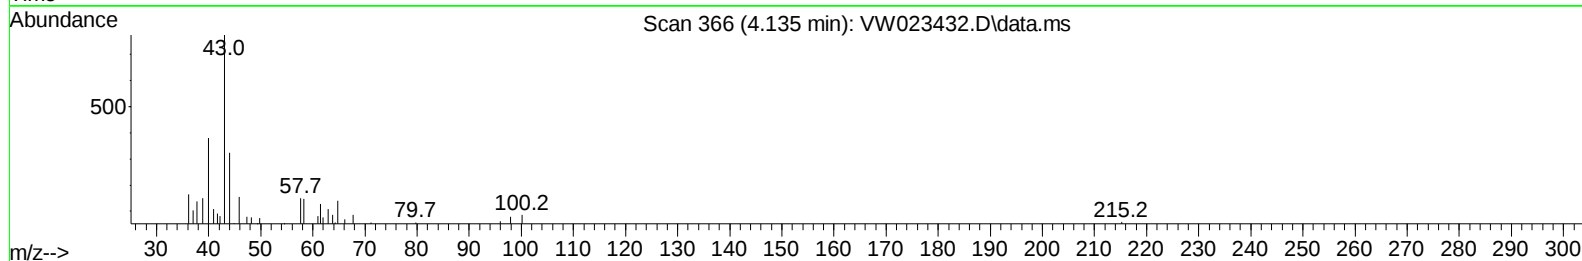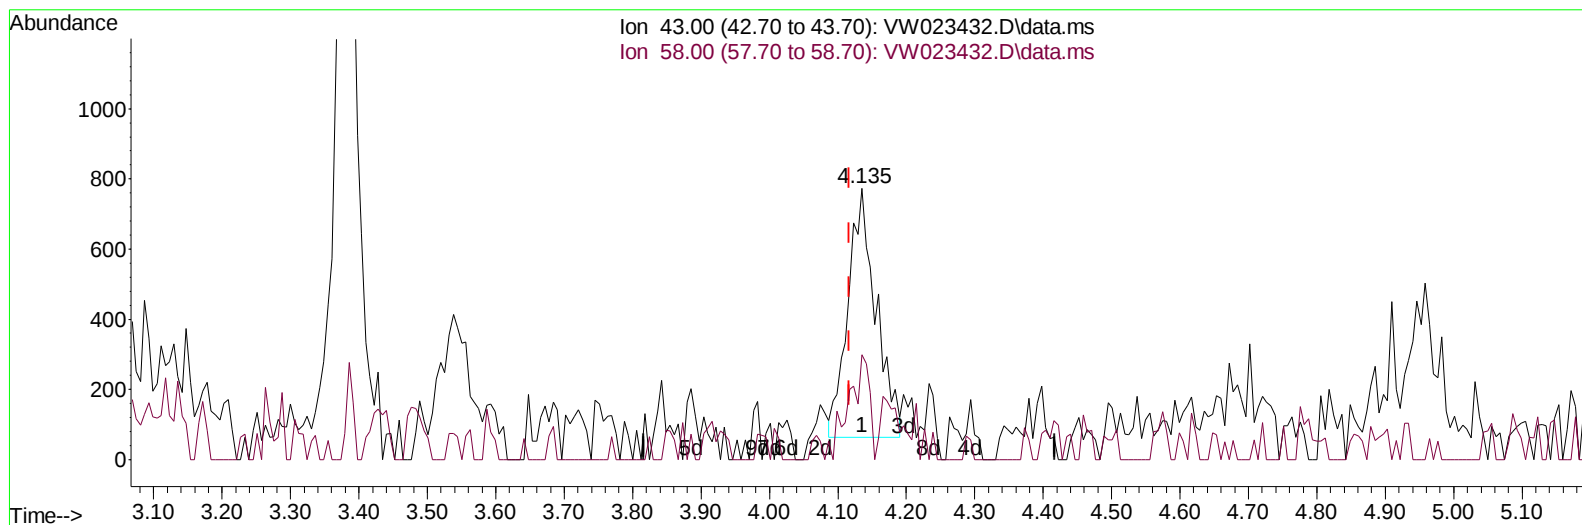

TIC: VW023432.D\data.ms

(13) Acetone (T)

4.135min (+ 0.018) 3.37 ug/L

response 2022

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	13.85
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060822\
 Data File : VW023432.D
 Acq On : 08 Jun 2022 16:52
 Operator : SY/VA
 Sample : N3226-09RE
 Misc : 6.41g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4M9RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/09/2022
 Supervised By :Mahesh Dadoda 06/09/2022

Quant Time: Jun 09 00:42:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 09 00:39:51 2022
 Response via : Initial Calibration

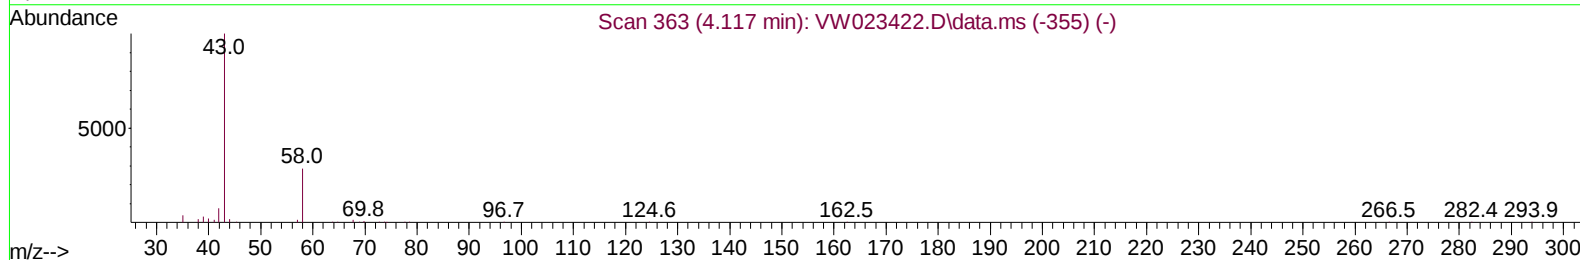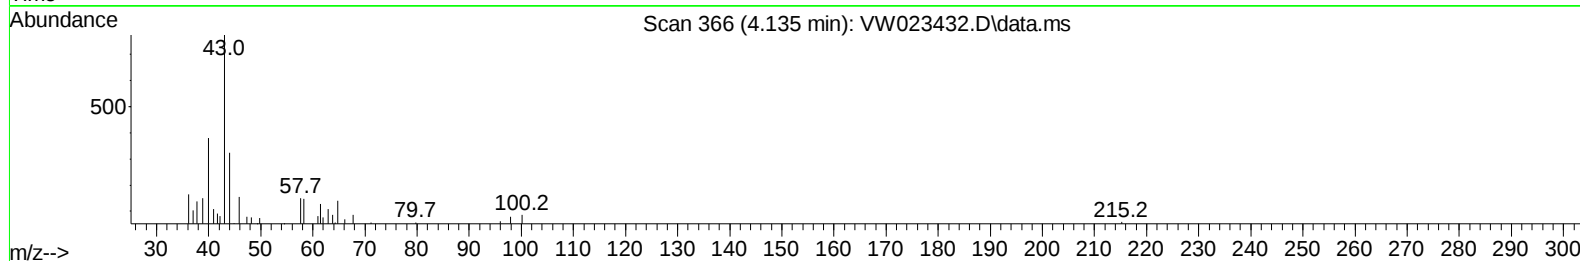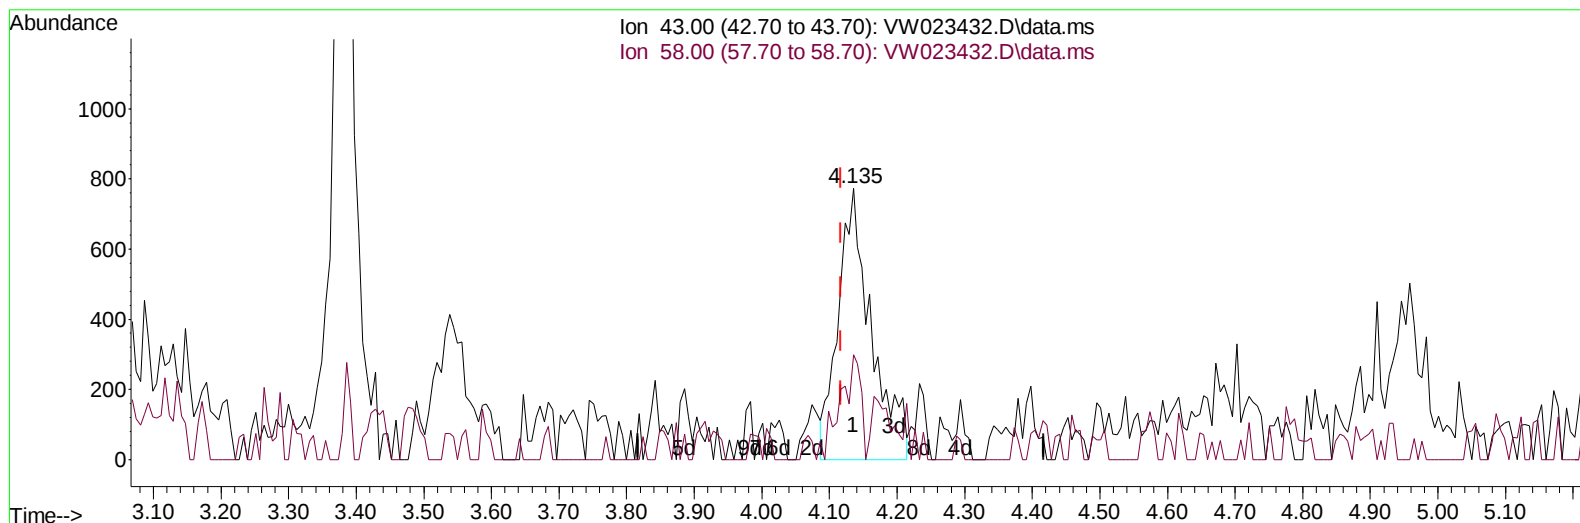

TIC: VW023432.D\data.ms

(13) Acetone (T)

4.135min (+ 0.018) 4.37 ug/L m

response 2627

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	10.66
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060822\
Data File : VW023432.D
Acq On : 08 Jun 2022 16:52
Operator : SY/VA
Sample : N3226-09RE
Misc : 6.41g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW4M9RE

Manual IntegrationsAPPROVED

Quant Time: Jun 09 00:42:41 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060622SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jun 09 00:39:51 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/09/2022
Supervised By :Mahesh Dadoda 06/09/2022

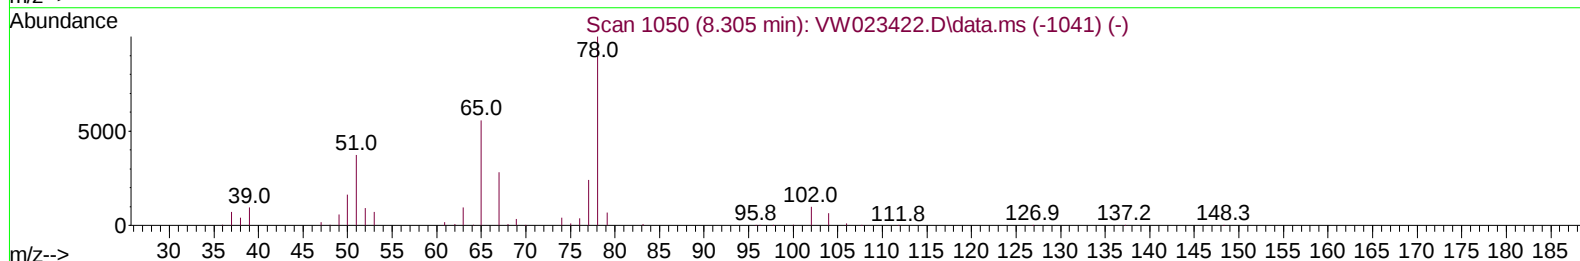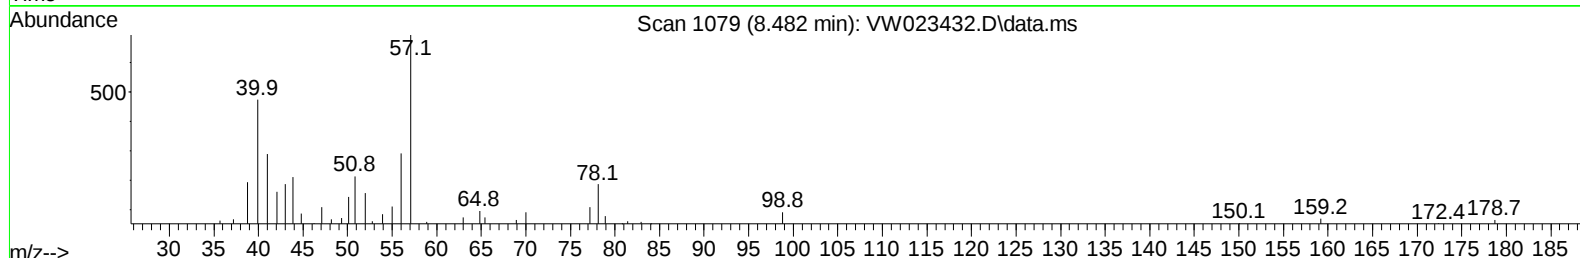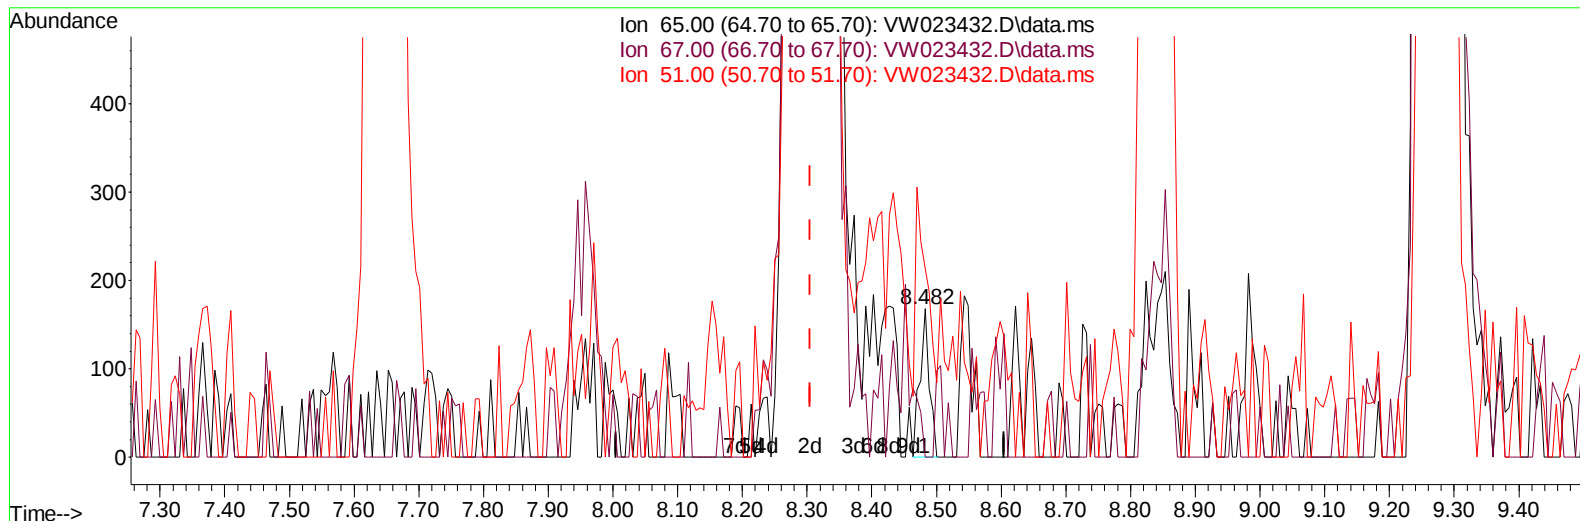

TIC: VW023432.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.482min (+ 0.177) 0.04 ug/L

response 169

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.10	43.79
51.00	92.30	84.02
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060822\
 Data File : VW023432.D
 Acq On : 08 Jun 2022 16:52
 Operator : SY/VA
 Sample : N3226-09RE
 Misc : 6.41g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4M9RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/09/2022
 Supervised By :Mahesh Dadoda 06/09/2022

Quant Time: Jun 09 00:42:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 09 00:39:51 2022
 Response via : Initial Calibration

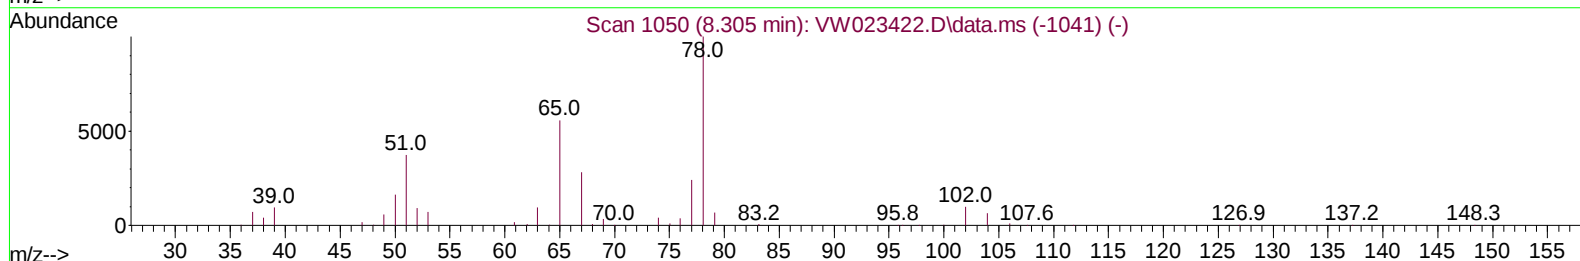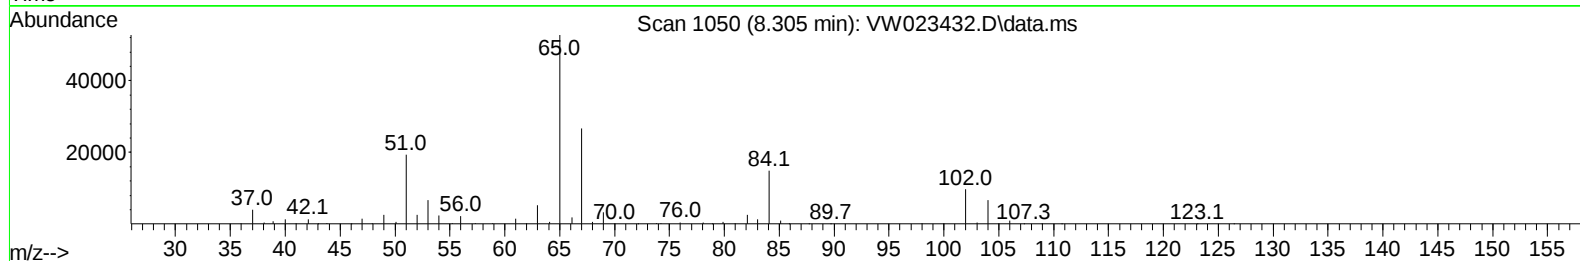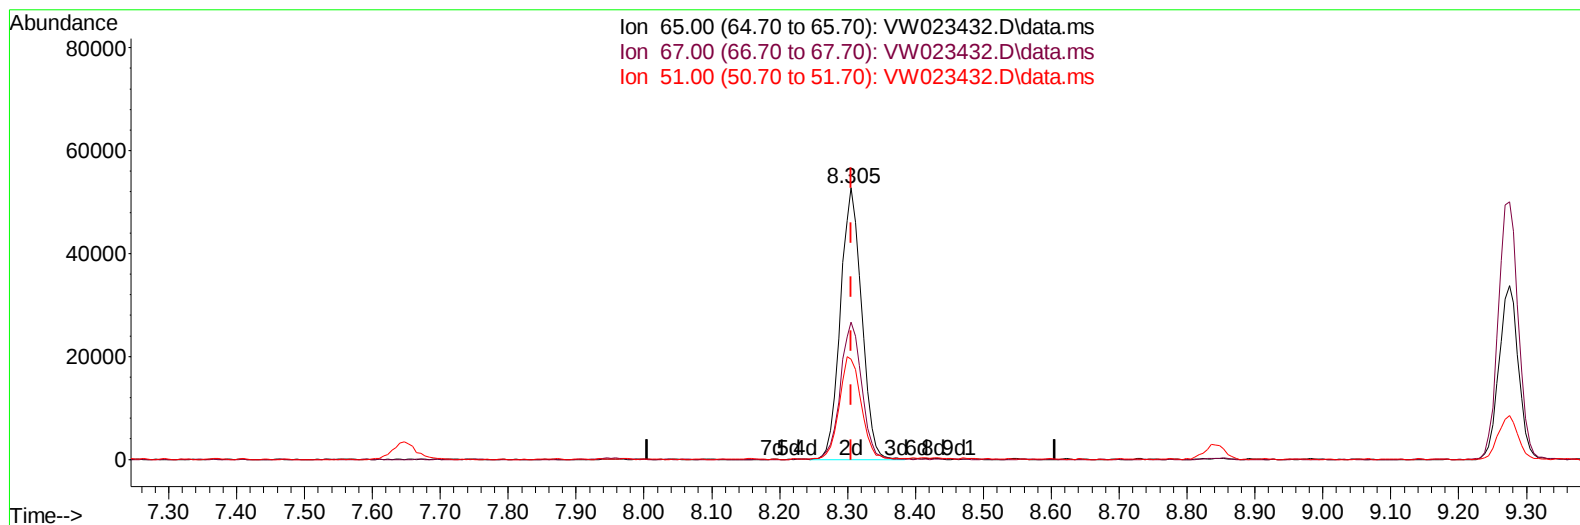

TIC: VW023432.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (+ 0.000) 29.99 ug/L m

response 113960

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.10	0.06#
51.00	92.30	0.12#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060822\
 Data File : VW023432.D
 Acq On : 08 Jun 2022 16:52
 Operator : SY/VA
 Sample : N3226-09RE
 Misc : 6.41g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4M9RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/09/2022
 Supervised By :Mahesh Dadoda 06/09/2022

Quant Time: Jun 09 00:42:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 09 00:39:51 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		268297	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		185683	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		41444	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.349	65		119201	28.702	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	114.800%	
7) Chloroethane-d5	2.879	69		86727	29.644	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	118.560%	
11) 1,1-Dichloroethene-d2	4.019	63		104957	16.829	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	67.320%	
21) 2-Butanone-d5	7.074	46		49459	61.751	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	123.500%	
24) Chloroform-d	7.647	84		182819	25.270	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	101.080%	
26) 1,2-Dichloroethane-d4	8.305	65		113960m	29.986	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	119.960%	
32) Benzene-d6	8.275	84		328103	31.832	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	127.320%	
36) 1,2-Dichloropropane-d6	9.275	67		103521	35.833	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	143.320%#	
41) Toluene-d8	10.323	98		254536	25.929	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	103.720%	
43) trans-1,3-Dichloroprop...	10.579	79		36650	28.435	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	113.720%	
47) 2-Hexanone-d5	10.921	63		35300	81.629	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	163.260%#	
56) 1,1,2,2-Tetrachloroeth...	12.689	84		86180	34.864	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	139.440%#	
66) 1,2-Dichlorobenzene-d4	13.853	152		38087	25.390	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	101.560%	
Target Compounds							
13) Acetone	4.135	43		2627m	4.373	ug/L	
53) m,p-Xylene	11.835	106		3485	0.665	ug/L	100
63) 1,2,4-Trimethylbenzene	13.249	105		2293	0.472	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060822\
Data File : VW023432.D
Acq On : 08 Jun 2022 16:52
Operator : SY/VA
Sample : N3226-09RE
Misc : 6.41g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW4M9RE

Manual IntegrationsAPPROVED

Quant Time: Jun 09 00:42:41 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060622SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jun 09 00:39:51 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/09/2022
Supervised By :Mahesh Dadoda 06/09/2022

