

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060822\
 Data File : VW023431.D
 Acq On : 08 Jun 2022 16:28
 Operator : SY/VA
 Sample : VIBLK494
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK494

Quant Time: Jun 09 00:42:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 09 00:39:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	316164	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	289150	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	124263	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	114167	23.328	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.320%
7) Chloroethane-d5	2.885	69	74909	21.728	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	86.920%
11) 1,1-Dichloroethene-d2	4.013	63	110667	15.058	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	60.240%
21) 2-Butanone-d5	7.080	46	47342	50.159	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	100.320%
24) Chloroform-d	7.647	84	191458	22.457	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.840%
26) 1,2-Dichloroethane-d4	8.305	65	110056	24.575	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.280%
32) Benzene-d6	8.275	84	369921	23.047	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	92.200%
36) 1,2-Dichloropropane-d6	9.274	67	110170	24.489	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	97.960%
41) Toluene-d8	10.323	98	345626	22.610	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.440%
43) trans-1,3-Dichloroprop...	10.579	79	43877	21.860	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	87.440%
47) 2-Hexanone-d5	10.920	63	35777	53.128	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	106.260%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	95356	24.772	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	99.080%
66) 1,2-Dichlorobenzene-d4	13.853	152	109120	24.261	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	97.040%
Target Compounds						Qvalue
16) Methylene chloride	4.915	84	18444	4.050	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060822\
Data File : VW023431.D
Acq On : 08 Jun 2022 16:28
Operator : SY/VA
Sample : VIBLK494
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK494


Quant Time: Jun 09 00:42:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060622SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jun 09 00:39:51 2022
Response via : Initial Calibration

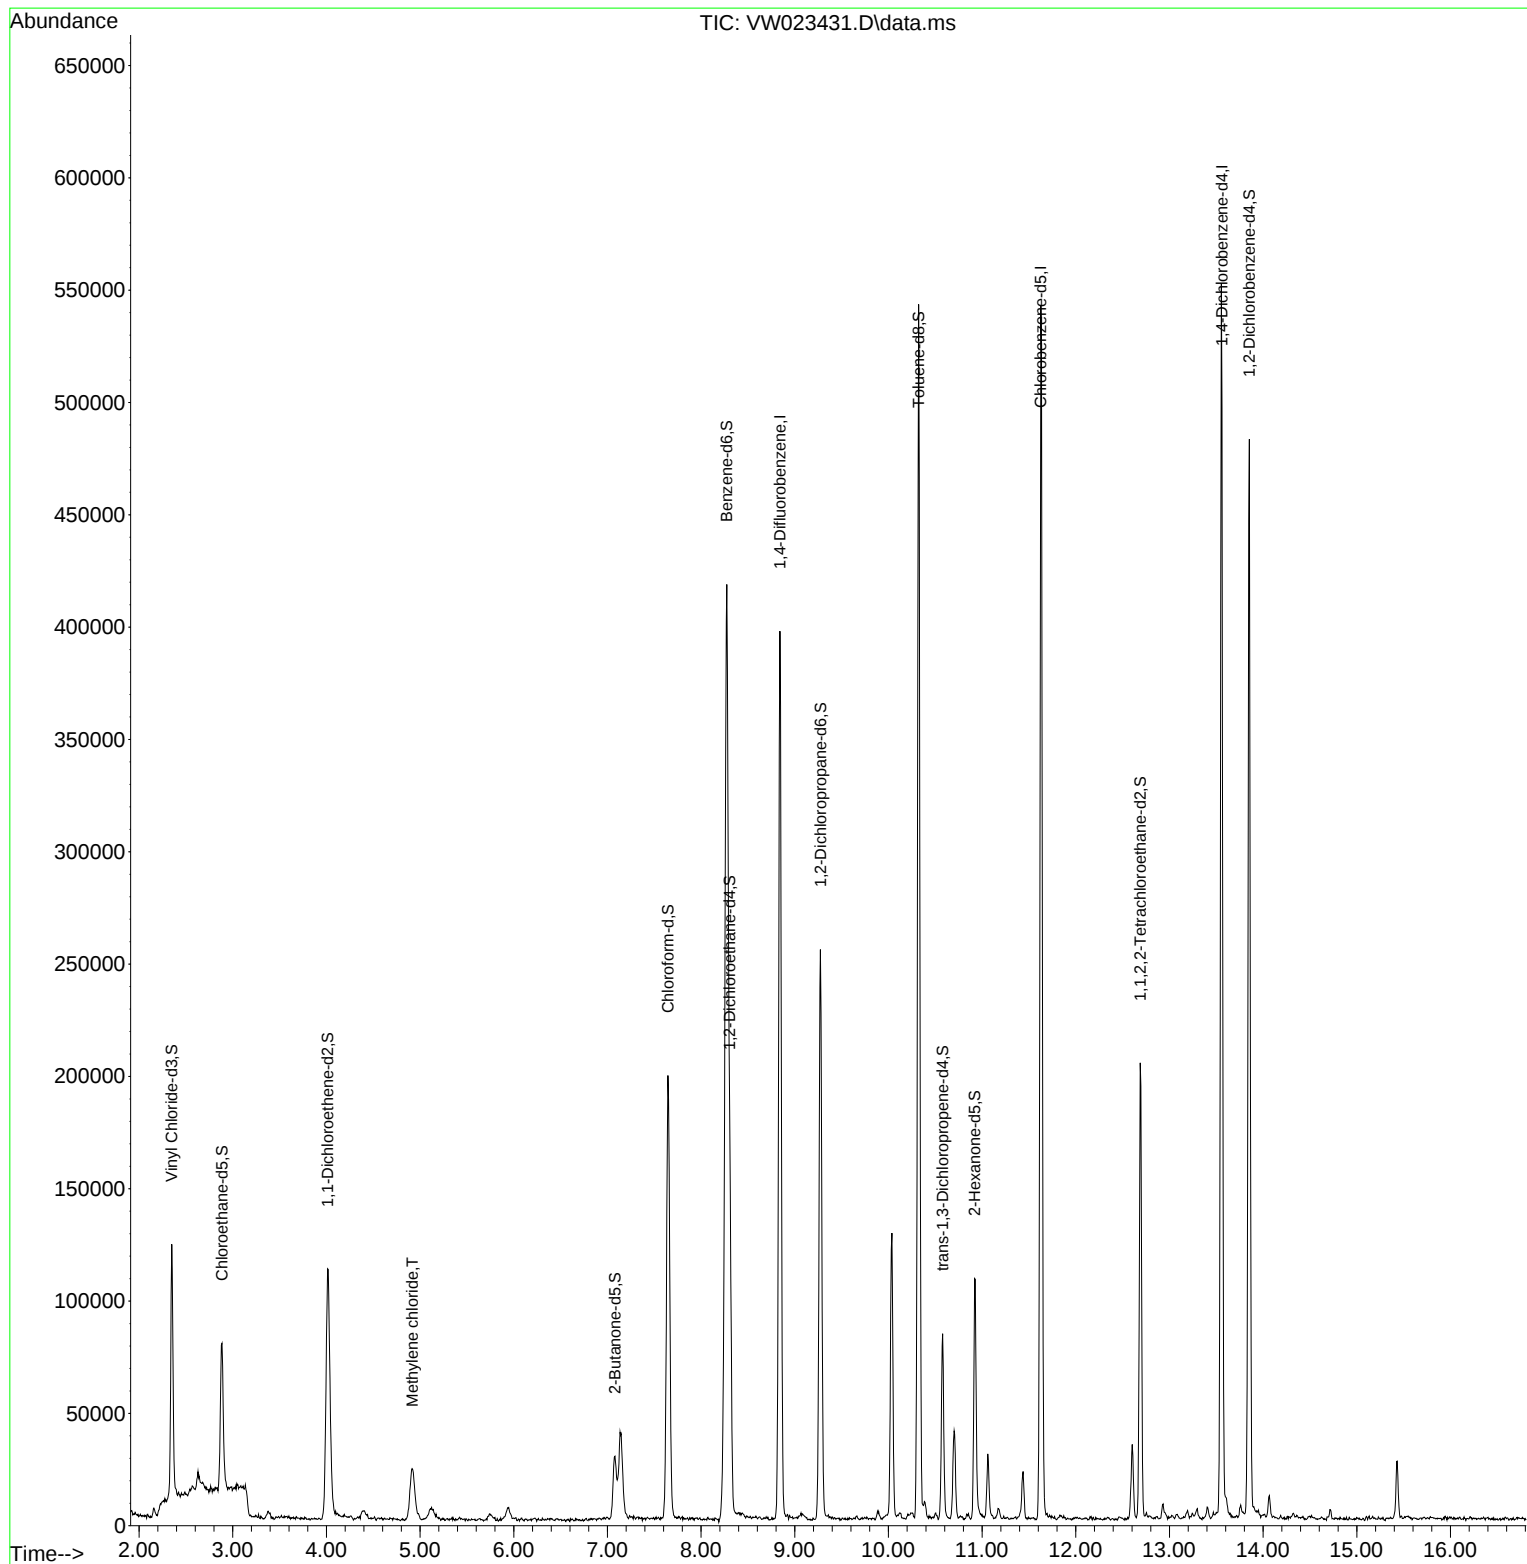

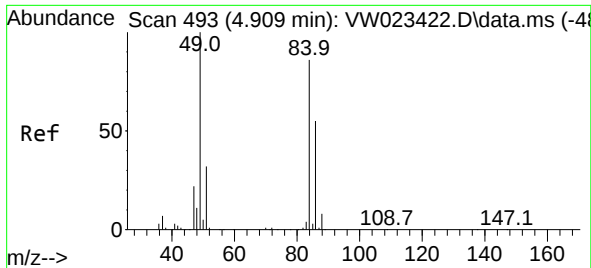

#16
Methylene chloride
Concen: 4.050 ug/L
RT: 4.915 min Scan# 49
Delta R.T. 0.006 min
Lab File: VW023431.D
Acq: 08 Jun 2022 16:28

Instrument :
MSVOA_W
ClientSampleId :
VIBLK494

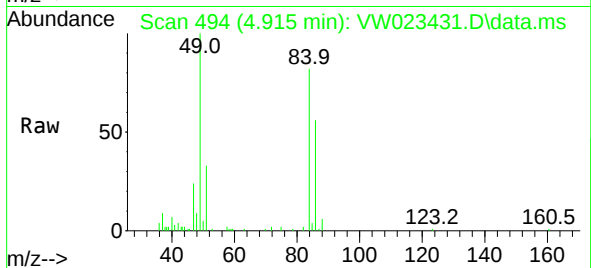

Tgt Ion: 84 Resp: 18444

Ion	Ratio	Lower	Upper
84	100		
86	67.3	45.4	84.4
49	121.2	82.5	153.1

