

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060823\
 Data File : VW026129.D
 Acq On : 08 Jun 2023 10:24
 Operator : SY/MD
 Sample : VW0608SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK513

Quant Time: Jun 09 01:24:06 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 09 01:23:25 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	692810	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	629426	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	268312	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	246762	25.318	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 101.280%			
7) Chloroethane-d5	2.899	69	208939	28.638	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 114.560%			
11) 1,1-Dichloroethene-d2	4.027	65	122474	25.484	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 101.920%			
21) 2-Butanone-d5	7.075	46	149177	52.573	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 105.140%			
24) Chloroform-d	7.648	84	489747	24.140	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 96.560%			
26) 1,2-Dichloroethane-d4	8.307	65	280056	25.244	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 100.960%			
32) Benzene-d6	8.276	84	1030022	24.320	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 97.280%			
36) 1,2-Dichloropropane-d6	9.276	67	326182	24.310	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 97.240%			
41) Toluene-d8	10.325	98	889216	23.674	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 94.680%			
43) trans-1,3-Dichloroprop...	10.575	79	117313	22.063	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 88.240%			
47) 2-Hexanone-d5	10.922	63	101444	47.948	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 95.900%			
56) 1,1,2,2-Tetrachloroeth...	12.690	84	242735	24.860	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 99.440%			
66) 1,2-Dichlorobenzene-d4	13.854	152	259569	25.275	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 101.080%			
Target Compounds						Qvalue
16) Methylene chloride	4.923	84	17895	1.618	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060823\
Data File : VW026129.D
Acq On : 08 Jun 2023 10:24
Operator : SY/MD
Sample : VW0608SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK513

Quant Time: Jun 09 01:24:06 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 09 01:23:25 2023
Response via : Initial Calibration

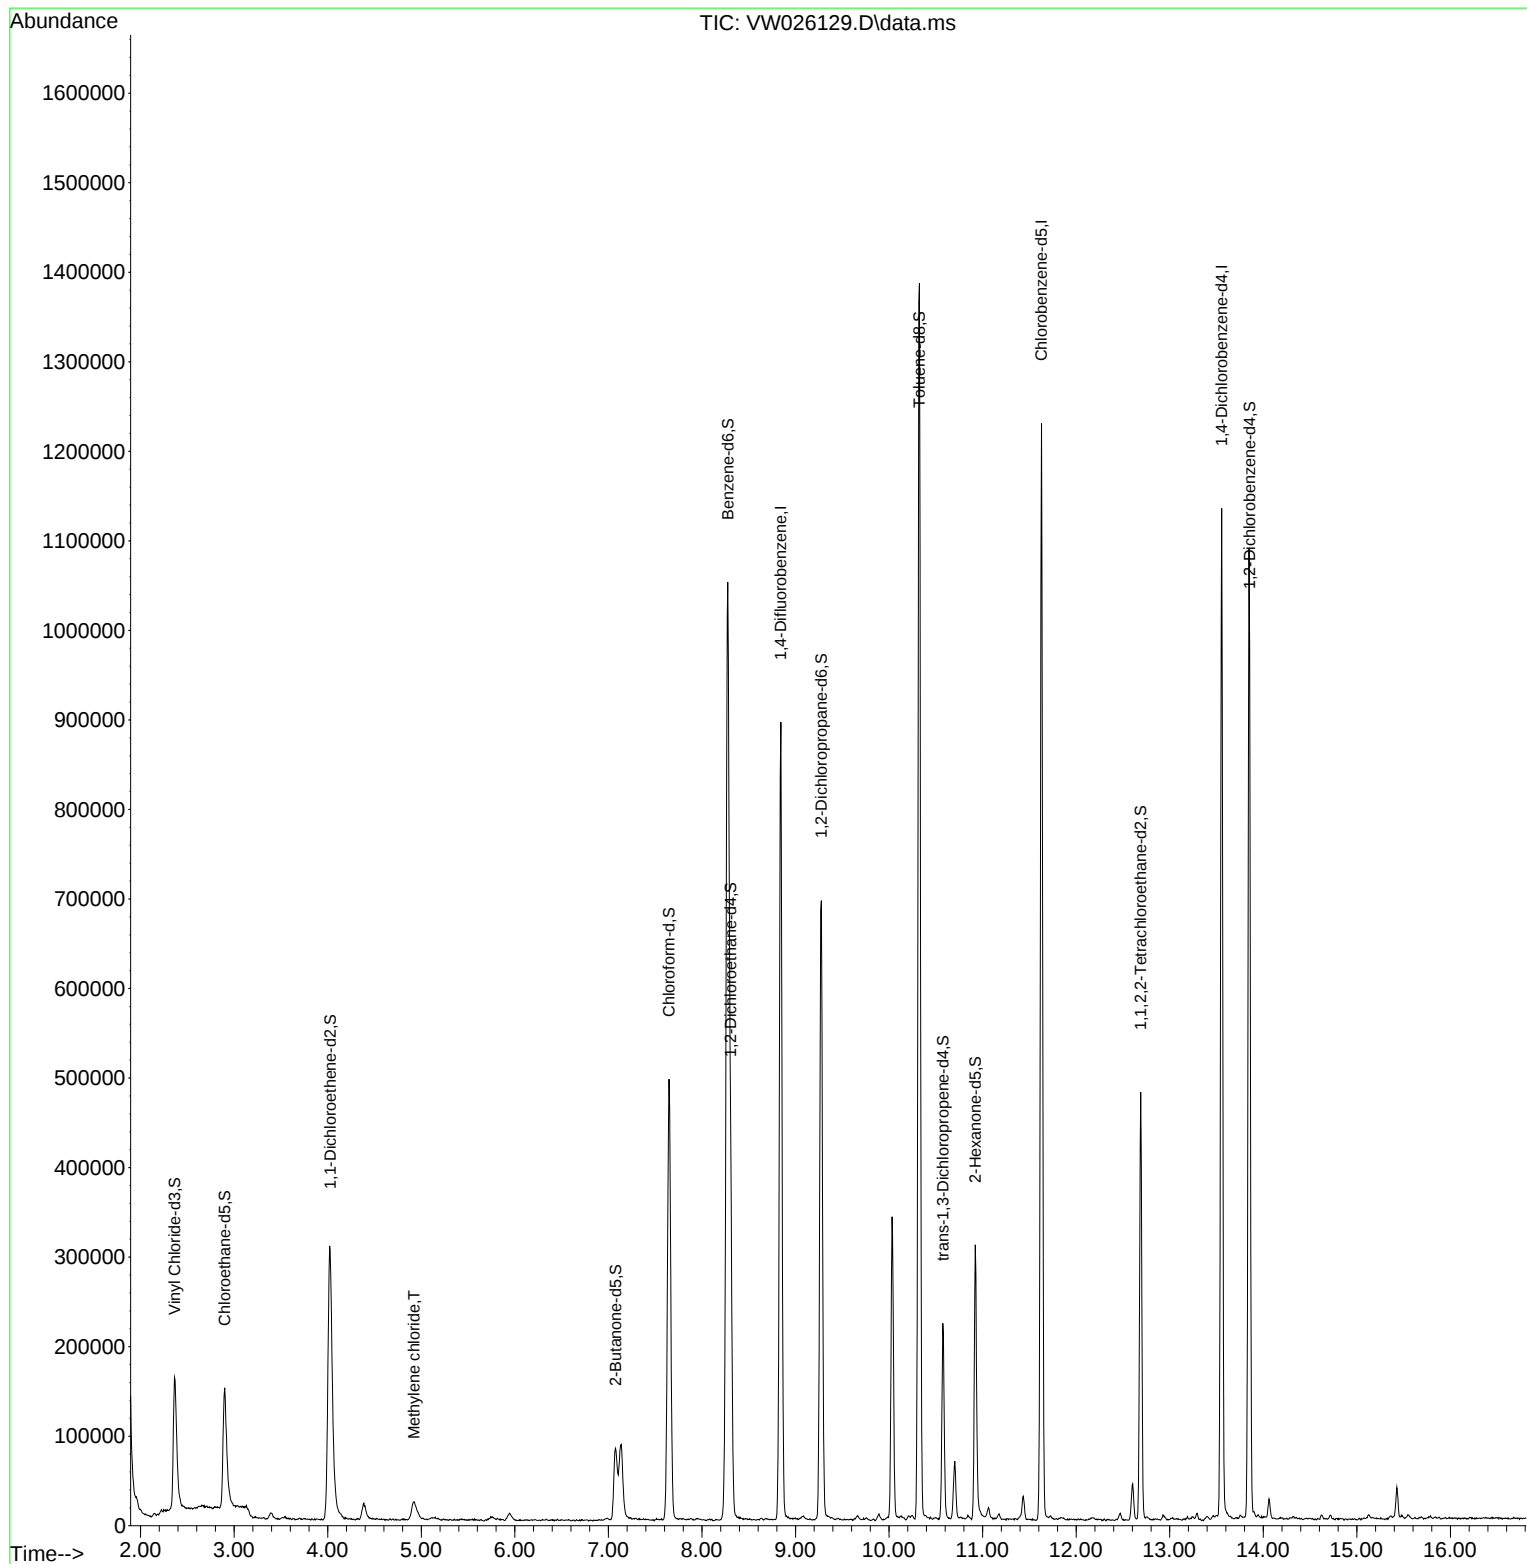

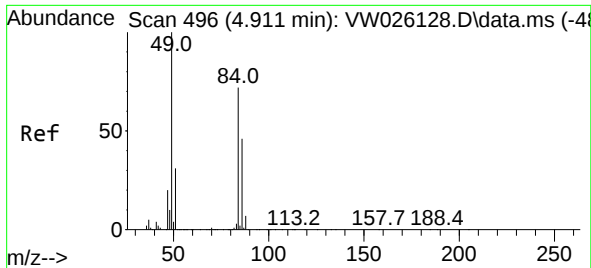

#16

Methylene chloride

Concen: 1.618 ug/L

RT: 4.923 min Scan# 49

Delta R.T. 0.012 min

Lab File: VW026129.D


Acq: 08 Jun 2023 10:24

Instrument :

MSVOA_W

ClientSampleId :

VBLK513

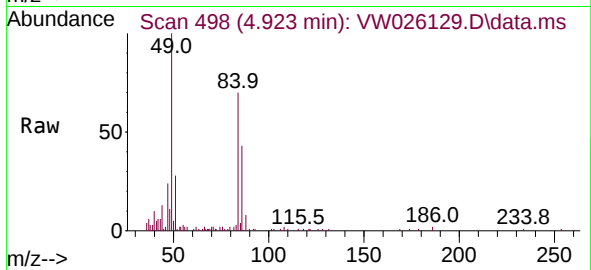

Tgt Ion: 84 Resp: 17895

Ion Ratio Lower Upper

84 100

86 61.0 44.2 82.0

49 142.4 98.8 183.6

