




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060823\
 Data File : VW026139.D
 Acq On : 08 Jun 2023 18:18
 Operator : SY/MD
 Sample : 03078-08
 Misc : 6.03g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 ESQX6

Manual IntegrationsAPPROVED

Quant Time: Jun 09 01:37:09 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 09 01:33:49 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/09/2023
 Supervised By :Mahesh Dadoda 06/09/2023

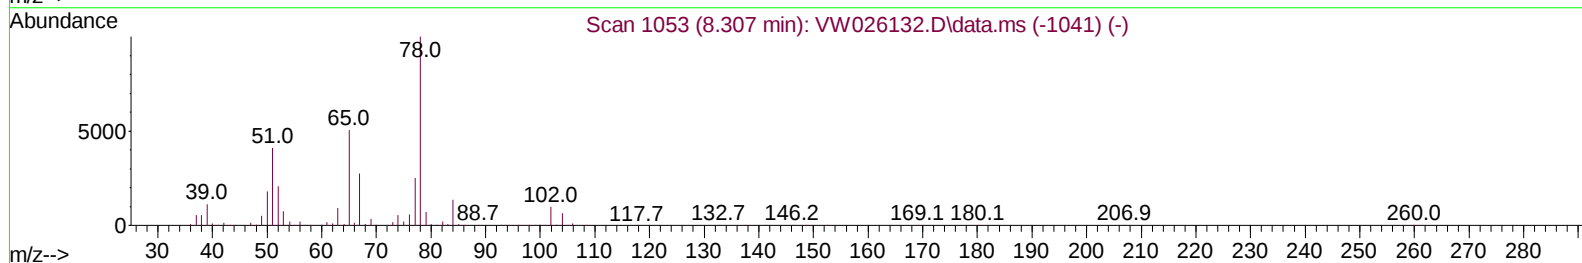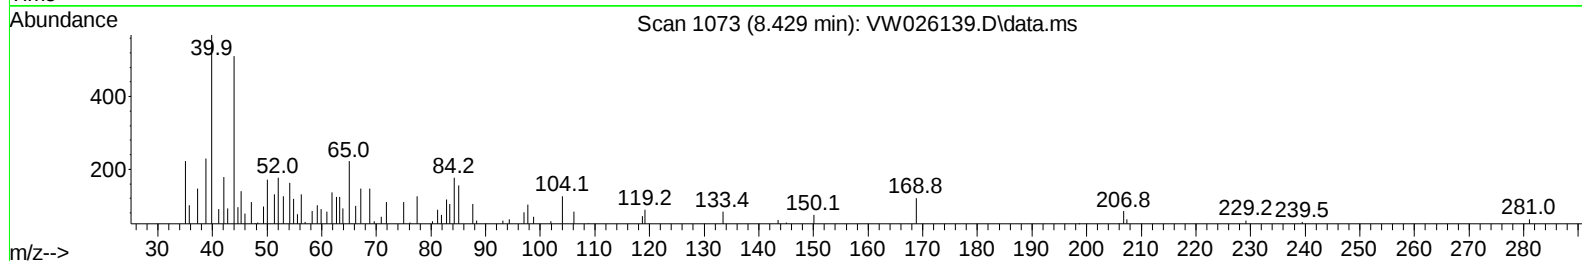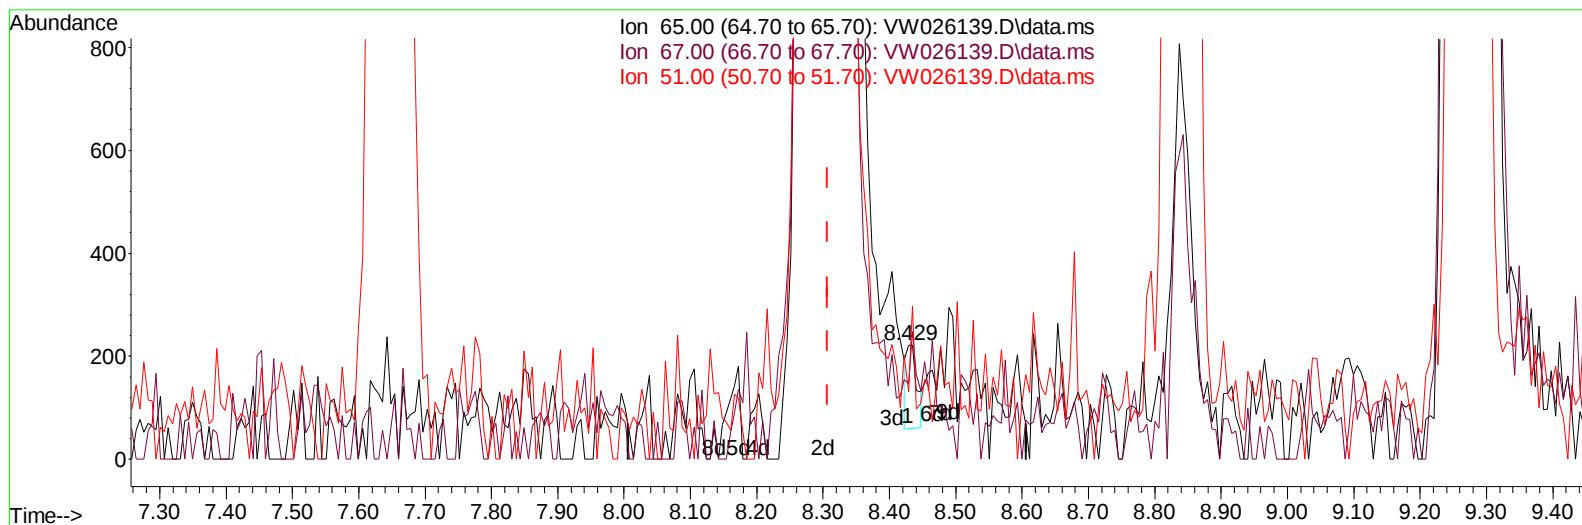

TIC: VW026139.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.429min (+ 0.122) 0.01 ug/L

response 170

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.70	65.29
51.00	106.50	92.35
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060823\
 Data File : VW026139.D
 Acq On : 08 Jun 2023 18:18
 Operator : SY/MD
 Sample : 03078-08
 Misc : 6.03g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 ESQX6

Manual IntegrationsAPPROVED

Quant Time: Jun 09 01:37:09 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 09 01:33:49 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/09/2023
 Supervised By :Mahesh Dadoda 06/09/2023

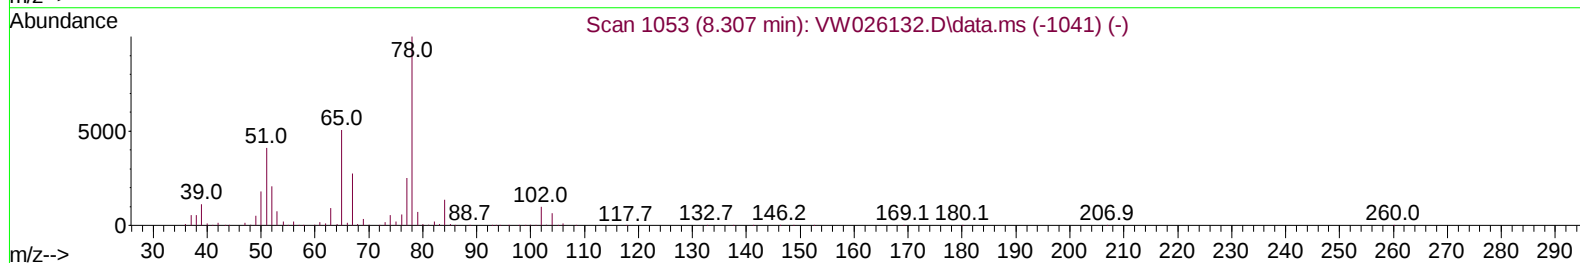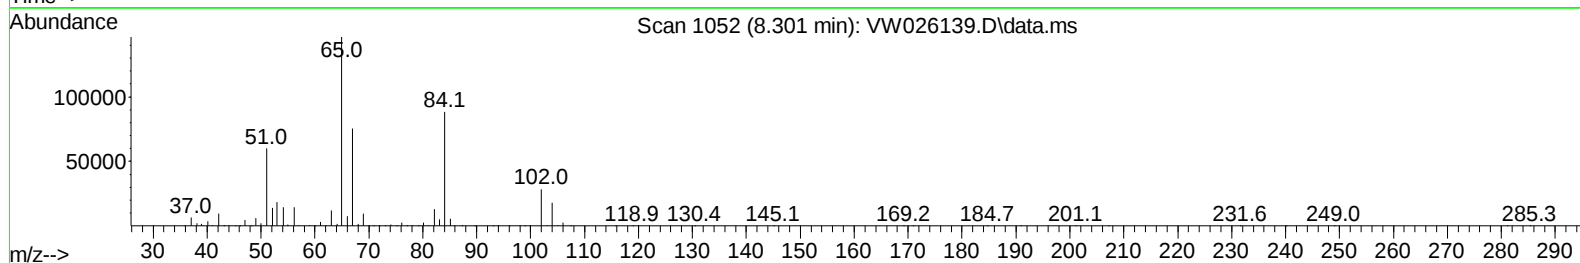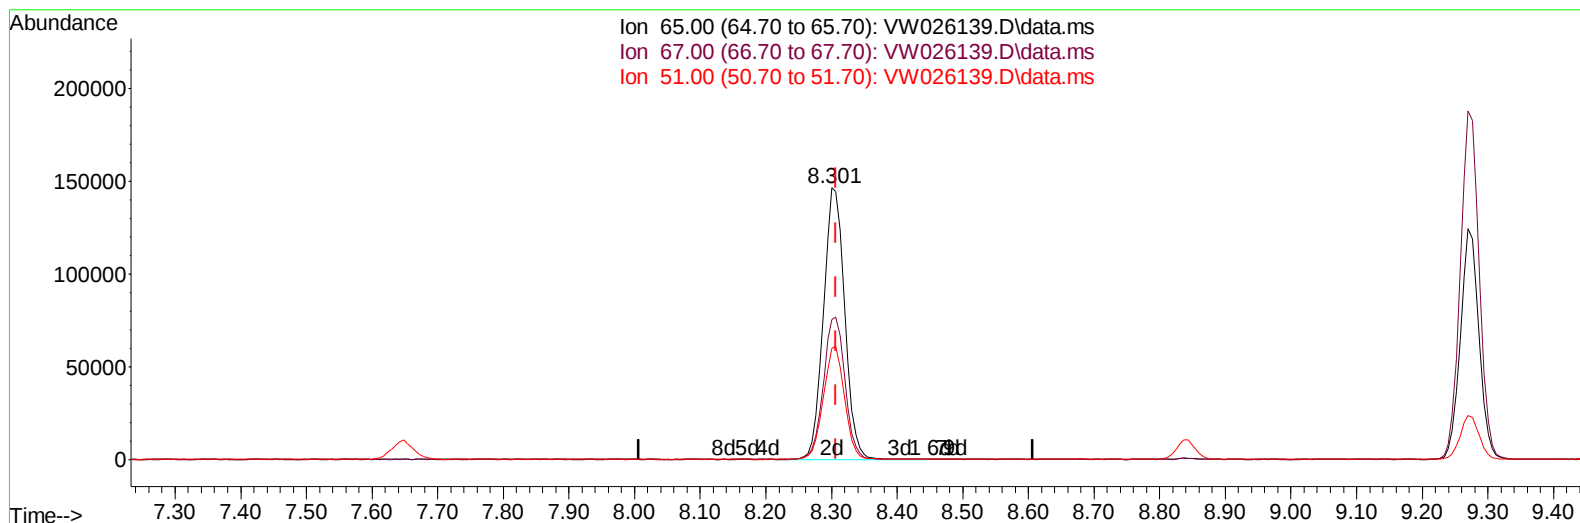

TIC: VW026139.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.301min (-0.006) 21.89 ug/L m

response 329997

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.70	0.03#
51.00	106.50	0.05#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060823\
 Data File : VW026139.D
 Acq On : 08 Jun 2023 18:18
 Operator : SY/MD
 Sample : 03078-08
 Misc : 6.03g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 ESQX6

Manual IntegrationsAPPROVED

Quant Time: Jun 09 01:37:09 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 09 01:33:49 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/09/2023
 Supervised By :Mahesh Dadoda 06/09/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		941271	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		765667	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		256063	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		261569	19.753	ug/L	-0.01
Spiked Amount 25.000	Range 30	- 150		Recovery	=	79.000%	
7) Chloroethane-d5	2.893	69		227056	22.906	ug/L	-0.01
Spiked Amount 25.000	Range 30	- 150		Recovery	=	91.640%	
11) 1,1-Dichloroethene-d2	4.021	65		127516	19.530	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	78.120%	
21) 2-Butanone-d5	7.075	46		184238	47.790	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	95.580%	
24) Chloroform-d	7.648	84		568898	20.639	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	82.560%	
26) 1,2-Dichloroethane-d4	8.301	65		329997m	21.894	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	87.560%	
32) Benzene-d6	8.276	84		1123721	21.811	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	87.240%	
36) 1,2-Dichloropropane-d6	9.270	67		376637	23.075	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	92.320%	
41) Toluene-d8	10.318	98		912141	19.964	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	79.840%	
43) trans-1,3-Dichloroprop...	10.575	79		127341	19.688	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	78.760%	
47) 2-Hexanone-d5	10.922	63		125126	48.618	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	97.240%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		291964	24.581	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	98.320%	
66) 1,2-Dichlorobenzene-d4	13.848	152		212122	21.643	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	86.560%	
Target Compounds							
						Qvalue	
13) Acetone	4.124	43		10961	3.675	ug/L	92
16) Methylene chloride	4.917	84		27876	1.856	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060823\
Data File : VW026139.D
Acq On : 08 Jun 2023 18:18
Operator : SY/MD
Sample : 03078-08
Misc : 6.03g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
ESQX6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/09/2023
Supervised By :Mahesh Dadoda 06/09/2023

Quant Time: Jun 09 01:37:09 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 09 01:33:49 2023
Response via : Initial Calibration

