




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060823\
 Data File : VW026141.D
 Acq On : 08 Jun 2023 19:06
 Operator : SY/MD
 Sample : 03101-01
 Misc : 8.79g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZEL6

Manual IntegrationsAPPROVED

Quant Time: Jun 09 01:37:33 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 09 01:33:49 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/09/2023
 Supervised By :Mahesh Dadoda 06/09/2023

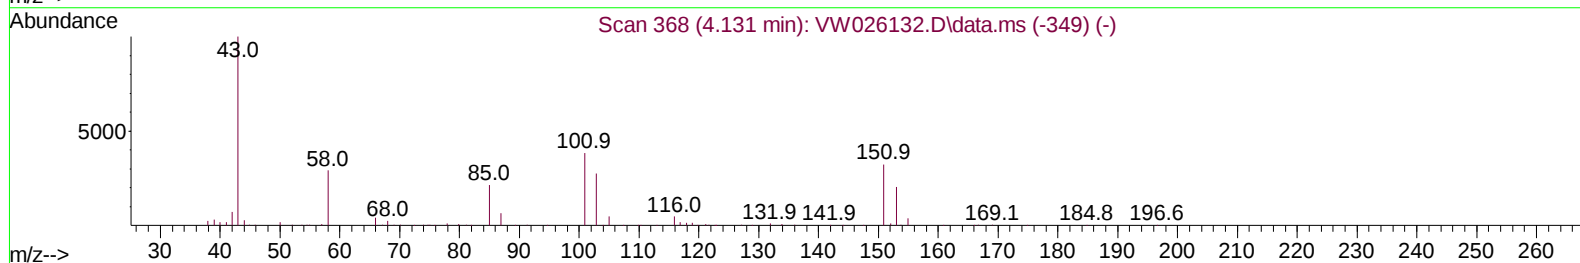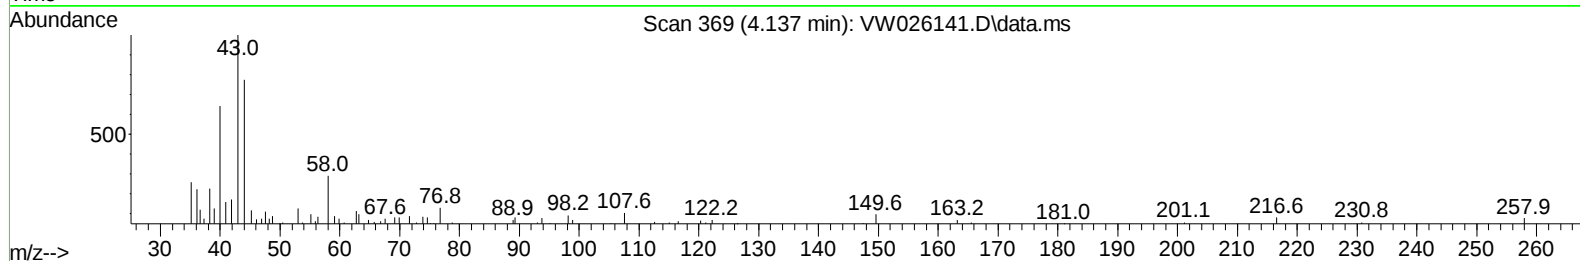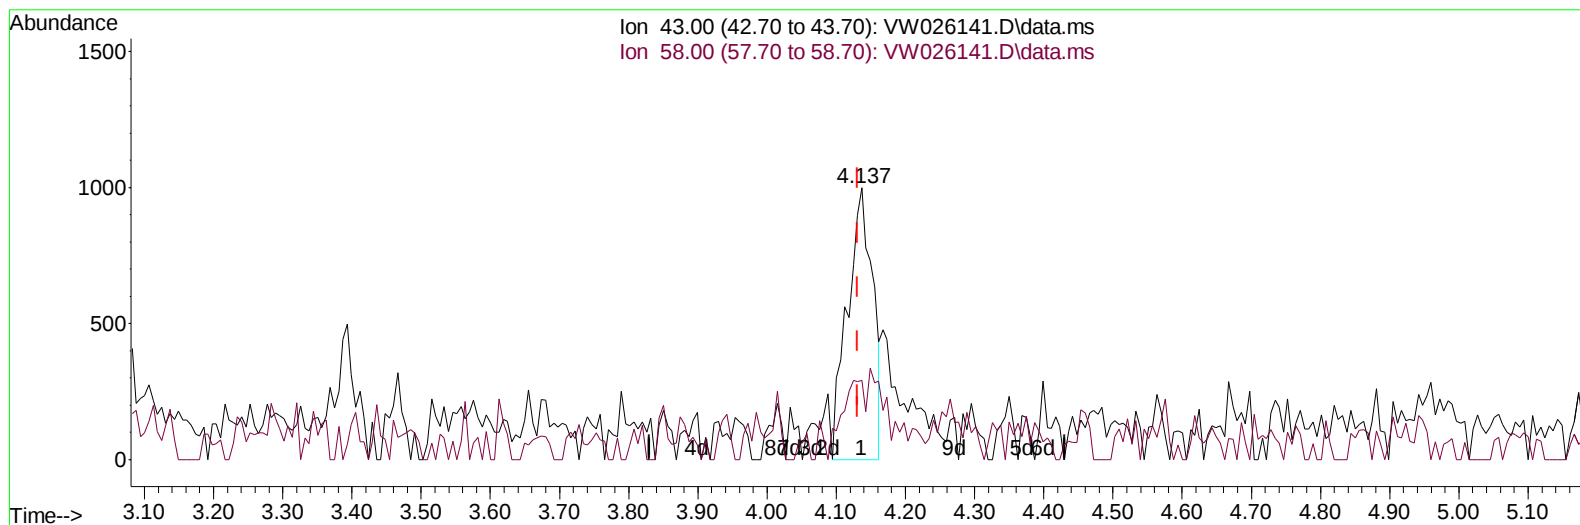

TIC: VW026141.D\data.ms

(13) Acetone (T)

4.137min (+ 0.006) 6.13 ug/L

response 2537

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	29.10	26.76
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060823\
Data File : VW026141.D
Acq On : 08 Jun 2023 19:06
Operator : SY/MD
Sample : 03101-01
Misc : 8.79g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EZEL6

Manual IntegrationsAPPROVED

Quant Time: Jun 09 01:37:33 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 09 01:33:49 2023
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/09/2023
Supervised By :Mahesh Dadoda 06/09/2023

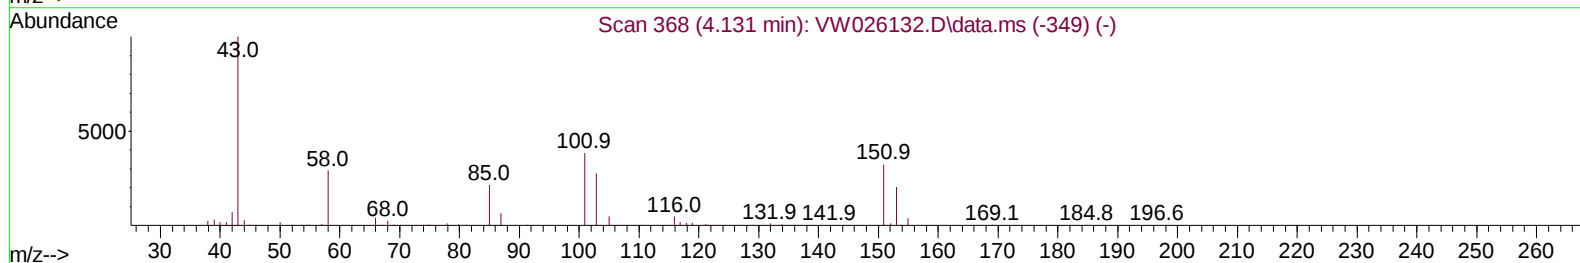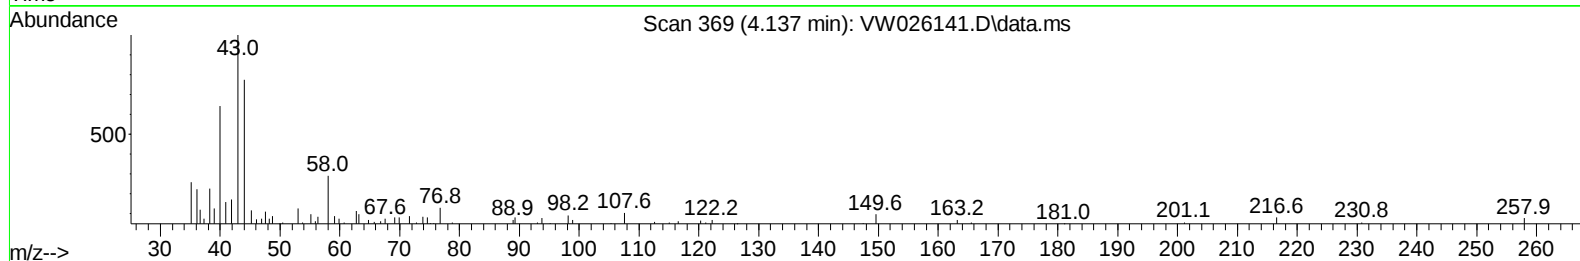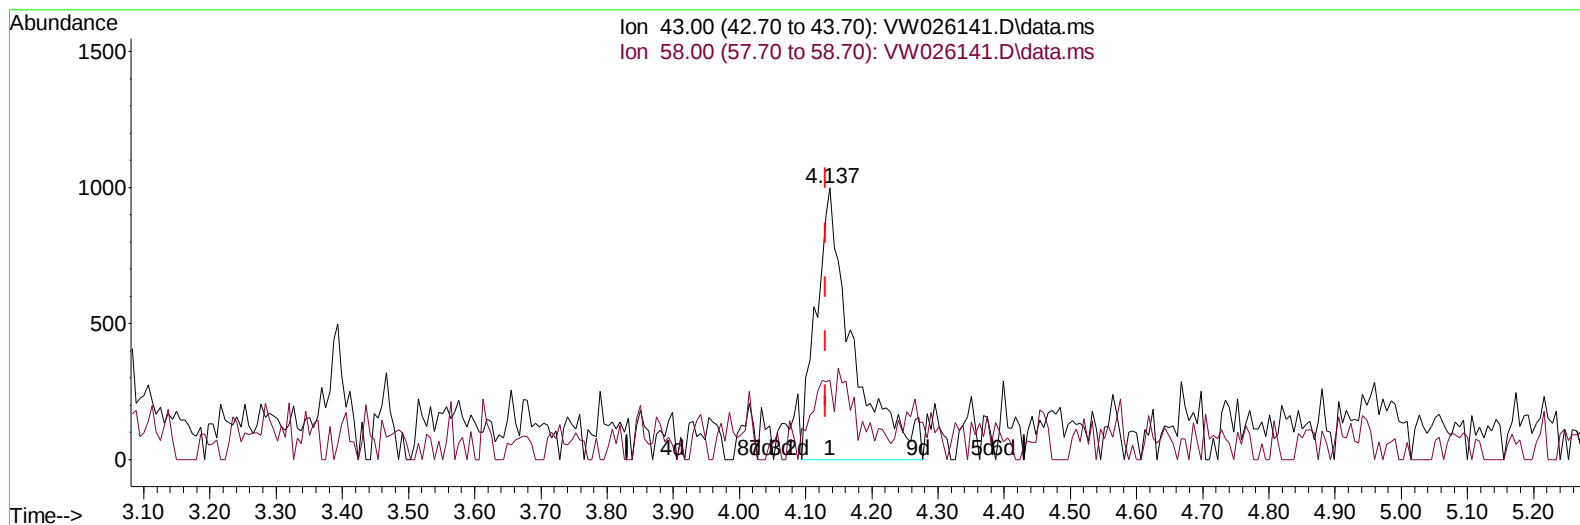

TIC: VW026141.D\data.ms

(13) Acetone (T)

4.137min (+ 0.006) 9.34 ug/L m

response 3864

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	29.10	17.57
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060823\
 Data File : VW026141.D
 Acq On : 08 Jun 2023 19:06
 Operator : SY/MD
 Sample : 03101-01
 Misc : 8.79g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZEL6

Manual IntegrationsAPPROVED

Quant Time: Jun 09 01:37:33 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 09 01:33:49 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/09/2023
 Supervised By :Mahesh Dadoda 06/09/2023

Compound		R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards								
1) 1,4-Difluorobenzene		8.843	114		130531	25.000	ug/L	0.00
28) Chlorobenzene-d5		11.629	117		119058	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		13.556	152		41910	25.000	ug/L	0.00
System Monitoring Compounds								
4) Vinyl Chloride-d3		2.357	65		46992	25.591	ug/L	-0.02
Spiked Amount	25.000	Range	30	- 150	Recovery	=	102.360%	
7) Chloroethane-d5		2.887	69		42055	30.594	ug/L	-0.02
Spiked Amount	25.000	Range	30	- 150	Recovery	=	122.360%	
11) 1,1-Dichloroethene-d2		4.021	65		23076	25.485	ug/L	0.00
Spiked Amount	25.000	Range	45	- 110	Recovery	=	101.960%	
21) 2-Butanone-d5		7.088	46		27372	51.200	ug/L	0.01
Spiked Amount	50.000	Range	20	- 135	Recovery	=	102.400%	
24) Chloroform-d		7.648	84		97477	25.501	ug/L	0.00
Spiked Amount	25.000	Range	40	- 150	Recovery	=	102.000%	
26) 1,2-Dichloroethane-d4		8.307	65		60416	28.905	ug/L	0.00
Spiked Amount	25.000	Range	70	- 130	Recovery	=	115.600%	
32) Benzene-d6		8.276	84		179149	22.362	ug/L	0.00
Spiked Amount	25.000	Range	20	- 135	Recovery	=	89.440%	
36) 1,2-Dichloropropane-d6		9.270	67		63845	25.155	ug/L	0.00
Spiked Amount	25.000	Range	70	- 120	Recovery	=	100.640%	
41) Toluene-d8		10.319	98		135220	19.033	ug/L	0.00
Spiked Amount	25.000	Range	30	- 130	Recovery	=	76.120%	
43) trans-1,3-Dichloroprop...		10.575	79		20505	20.388	ug/L	0.00
Spiked Amount	25.000	Range	30	- 135	Recovery	=	81.560%	
47) 2-Hexanone-d5		10.928	63		9655	24.126	ug/L	0.00
Spiked Amount	50.000	Range	20	- 135	Recovery	=	48.260%	
56) 1,1,2,2-Tetrachloroeth...		12.690	84		56764	30.735	ug/L	0.00
Spiked Amount	25.000	Range	45	- 120	Recovery	=	122.920%#	
66) 1,2-Dichlorobenzene-d4		13.848	152		36406	22.695	ug/L	0.00
Spiked Amount	25.000	Range	75	- 120	Recovery	=	90.800%	
Target Compounds								Qvalue
13) Acetone		4.137	43		3864m	9.341	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060823\
Data File : VW026141.D
Acq On : 08 Jun 2023 19:06
Operator : SY/MD
Sample : 03101-01
Misc : 8.79g/10mL/MSVOA_W/SoIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EZEL6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/09/2023
Supervised By :Mahesh Dadoda 06/09/2023

Quant Time: Jun 09 01:37:33 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 09 01:33:49 2023
Response via : Initial Calibration

