




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060823\
 Data File : VW026145.D
 Acq On : 08 Jun 2023 20:42
 Operator : SY/MD
 Sample : 03101-10
 Misc : 5.81g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZEM6

Manual IntegrationsAPPROVED

Quant Time: Jun 09 01:38:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 09 01:33:49 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/09/2023
 Supervised By :Mahesh Dadoda 06/09/2023

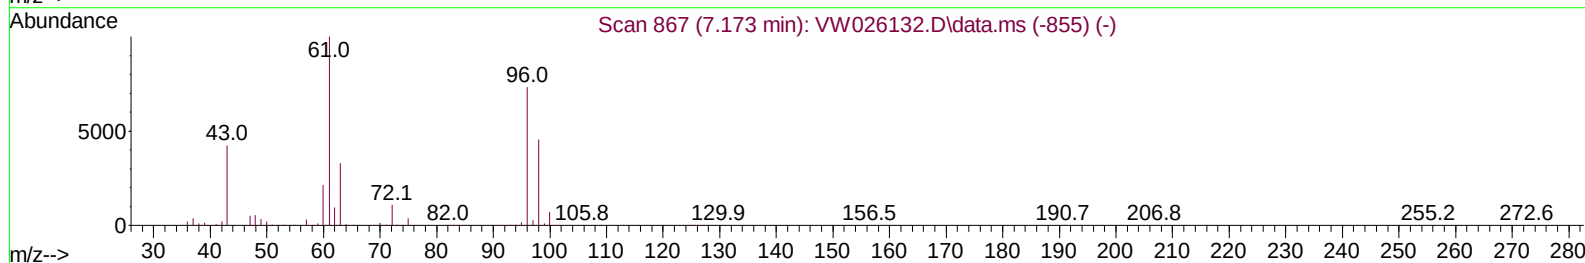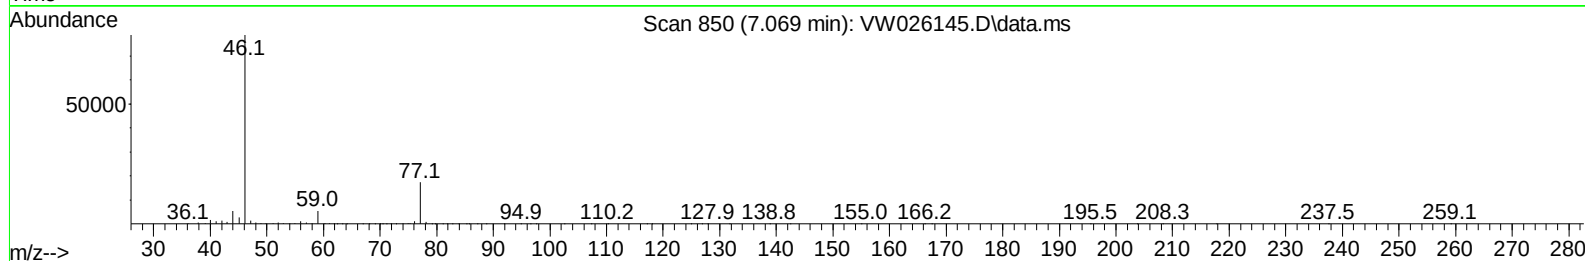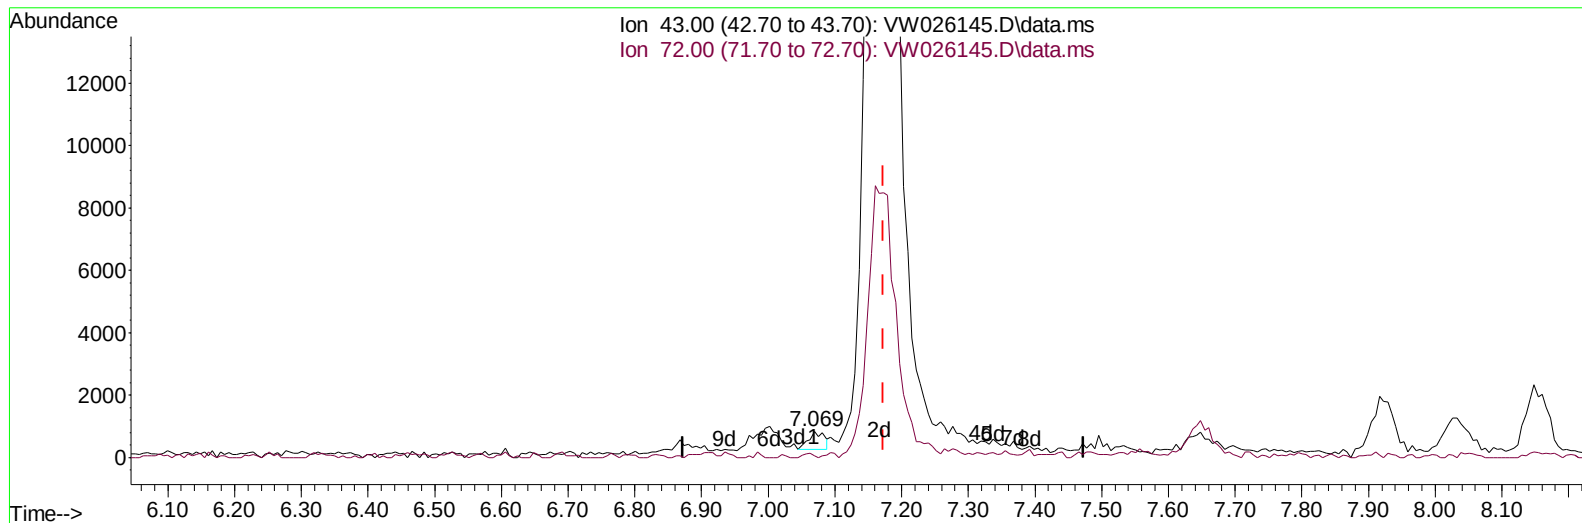

TIC: VW026145.D\data.ms

(22) 2-Butanone (T)

7.069min (-0.104) 0.36 ug/L

response 923

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	24.90	16.36
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060823\
 Data File : VW026145.D
 Acq On : 08 Jun 2023 20:42
 Operator : SY/MD
 Sample : 03101-10
 Misc : 5.81g/10mL/MSVOA_W/SoIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZEM6

Manual IntegrationsAPPROVED

Quant Time: Jun 09 01:38:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 09 01:33:49 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/09/2023
 Supervised By :Mahesh Dadoda 06/09/2023

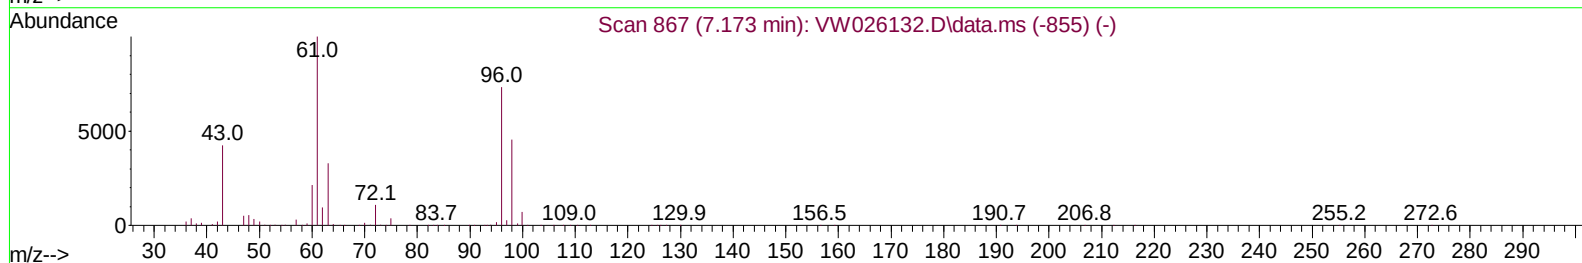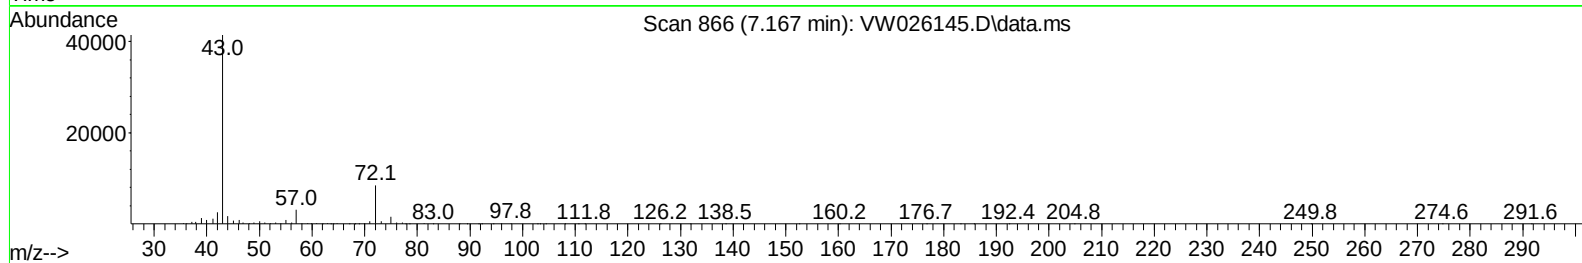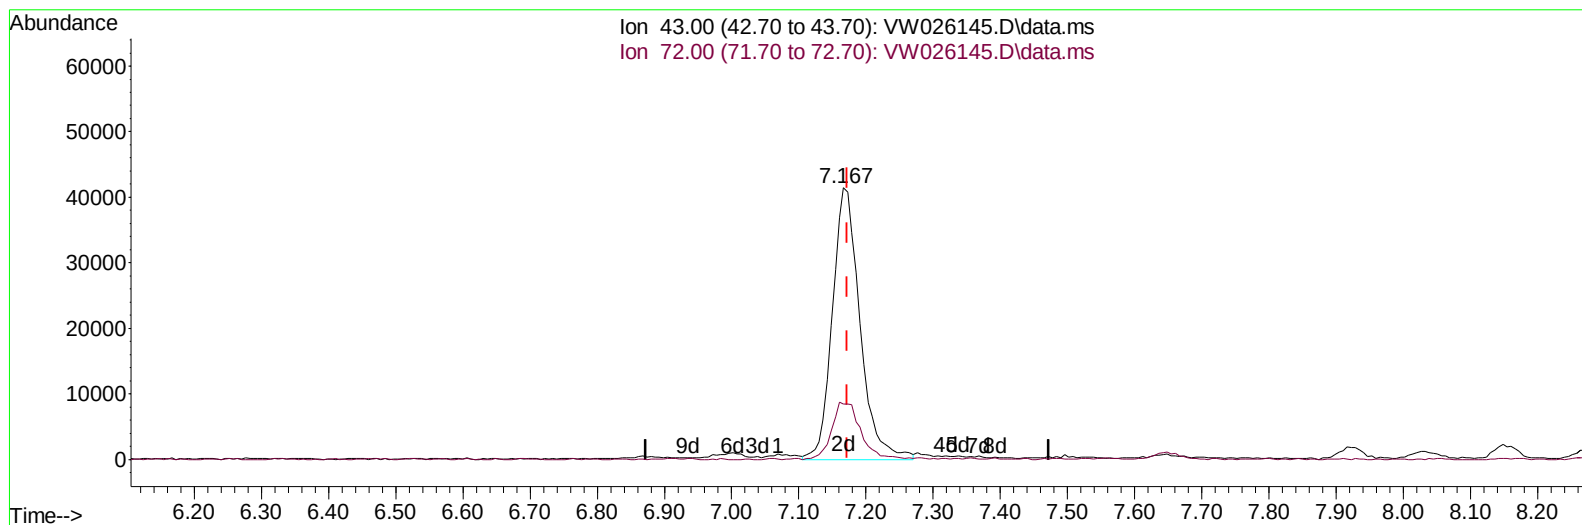

TIC: VW026145.D\data.ms

(22) 2-Butanone (T)

7.167min (-0.006) 46.09 ug/L m

response 118323

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	24.90	0.13#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060823\
 Data File : VW026145.D
 Acq On : 08 Jun 2023 20:42
 Operator : SY/MD
 Sample : 03101-10
 Misc : 5.81g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZEM6

Manual IntegrationsAPPROVED

Quant Time: Jun 09 01:38:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 09 01:33:49 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/09/2023
 Supervised By :Mahesh Dadoda 06/09/2023

Compound			R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards									
1)	1,4-Difluorobenzene		8.843	114		567836	25.000	ug/L	0.00
28)	Chlorobenzene-d5		11.629	117		313354	25.000	ug/L	0.00
58)	1,4-Dichlorobenzene-d4		13.556	152		118109	25.000	ug/L	0.00
System Monitoring Compounds									
4)	Vinyl Chloride-d3		2.363	65		203786	25.511	ug/L	-0.01
	Spiked Amount	25.000	Range	30	- 150	Recovery	= 102.040%		
7)	Chloroethane-d5		2.893	69		186538	31.194	ug/L	-0.01
	Spiked Amount	25.000	Range	30	- 150	Recovery	= 124.760%		
11)	1,1-Dichloroethene-d2		4.015	65		88766	22.536	ug/L	0.00
	Spiked Amount	25.000	Range	45	- 110	Recovery	= 90.160%		
21)	2-Butanone-d5		7.075	46		219423	94.349	ug/L	0.00
	Spiked Amount	50.000	Range	20	- 135	Recovery	= 188.700%#		
24)	Chloroform-d		7.648	84		407342	24.497	ug/L	0.00
	Spiked Amount	25.000	Range	40	- 150	Recovery	= 98.000%		
26)	1,2-Dichloroethane-d4		8.307	65		269139	29.600	ug/L	0.00
	Spiked Amount	25.000	Range	70	- 130	Recovery	= 118.400%		
32)	Benzene-d6		8.270	84		764419	36.254	ug/L	0.00
	Spiked Amount	25.000	Range	20	- 135	Recovery	= 145.000%#		
36)	1,2-Dichloropropane-d6		9.270	67		269350	40.322	ug/L	0.00
	Spiked Amount	25.000	Range	70	- 120	Recovery	= 161.280%#		
41)	Toluene-d8		10.325	98		450454	24.090	ug/L	0.00
	Spiked Amount	25.000	Range	30	- 130	Recovery	= 96.360%		
43)	trans-1,3-Dichloroprop...		10.575	79		71820	27.132	ug/L	0.00
	Spiked Amount	25.000	Range	30	- 135	Recovery	= 108.520%		
47)	2-Hexanone-d5		10.922	63		139687	132.619	ug/L	0.00
	Spiked Amount	50.000	Range	20	- 135	Recovery	= 265.240%#		
56)	1,1,2,2-Tetrachloroeth...		12.690	84		196596	40.444	ug/L	0.00
	Spiked Amount	25.000	Range	45	- 120	Recovery	= 161.760%#		
66)	1,2-Dichlorobenzene-d4		13.861	152		121610	26.901	ug/L	0.00
	Spiked Amount	25.000	Range	75	- 120	Recovery	= 107.600%		
Target Compounds									
13)	Acetone		4.112	43		263007	146.153	ug/L	99
14)	Carbon disulfide		4.387	76		27005	1.058	ug/L	100
22)	2-Butanone		7.167	43		118323m	46.094	ug/L	
35)	Methylcyclohexane		9.331	83		14675	1.509	ug/L #	82

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060823\
Data File : VW026145.D
Acq On : 08 Jun 2023 20:42
Operator : SY/MD
Sample : 03101-10
Misc : 5.81g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EZEM6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/09/2023
Supervised By :Mahesh Dadoda 06/09/2023

Quant Time: Jun 09 01:38:24 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 09 01:33:49 2023
Response via : Initial Calibration

