

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060823\
 Data File : VW026131.D
 Acq On : 08 Jun 2023 11:44
 Operator : SY/MD
 Sample : 03078-06
 Misc : 4.99g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK002

Quant Time: Jun 09 01:24:29 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 09 01:23:25 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	726462	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	655215	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	273093	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	232658	22.765	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	91.080%		
7) Chloroethane-d5	2.899	69	197386	25.801	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	103.200%		
11) 1,1-Dichloroethene-d2	4.021	65	115174	22.855	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	91.440%		
21) 2-Butanone-d5	7.075	46	143194	48.127	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	96.260%		
24) Chloroform-d	7.648	84	463310	21.779	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	87.120%		
26) 1,2-Dichloroethane-d4	8.301	65	263804	22.678	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	90.720%		
32) Benzene-d6	8.276	84	970458	22.012	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	88.040%		
36) 1,2-Dichloropropane-d6	9.276	67	310038	22.197	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	88.800%		
41) Toluene-d8	10.325	98	833017	21.305	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	85.240%		
43) trans-1,3-Dichloroprop...	10.575	79	111989	20.233	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	80.920%		
47) 2-Hexanone-d5	10.922	63	94812	43.049	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	86.100%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	210894	20.749	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	83.000%		
66) 1,2-Dichlorobenzene-d4	13.849	152	253840	24.284	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	97.120%		
Target Compounds						Qvalue
16) Methylene chloride	4.923	84	23616	2.037	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060823\
Data File : VW026131.D
Acq On : 08 Jun 2023 11:44
Operator : SY/MD
Sample : 03078-06
Misc : 4.99g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK002

Quant Time: Jun 09 01:24:29 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 09 01:23:25 2023
Response via : Initial Calibration

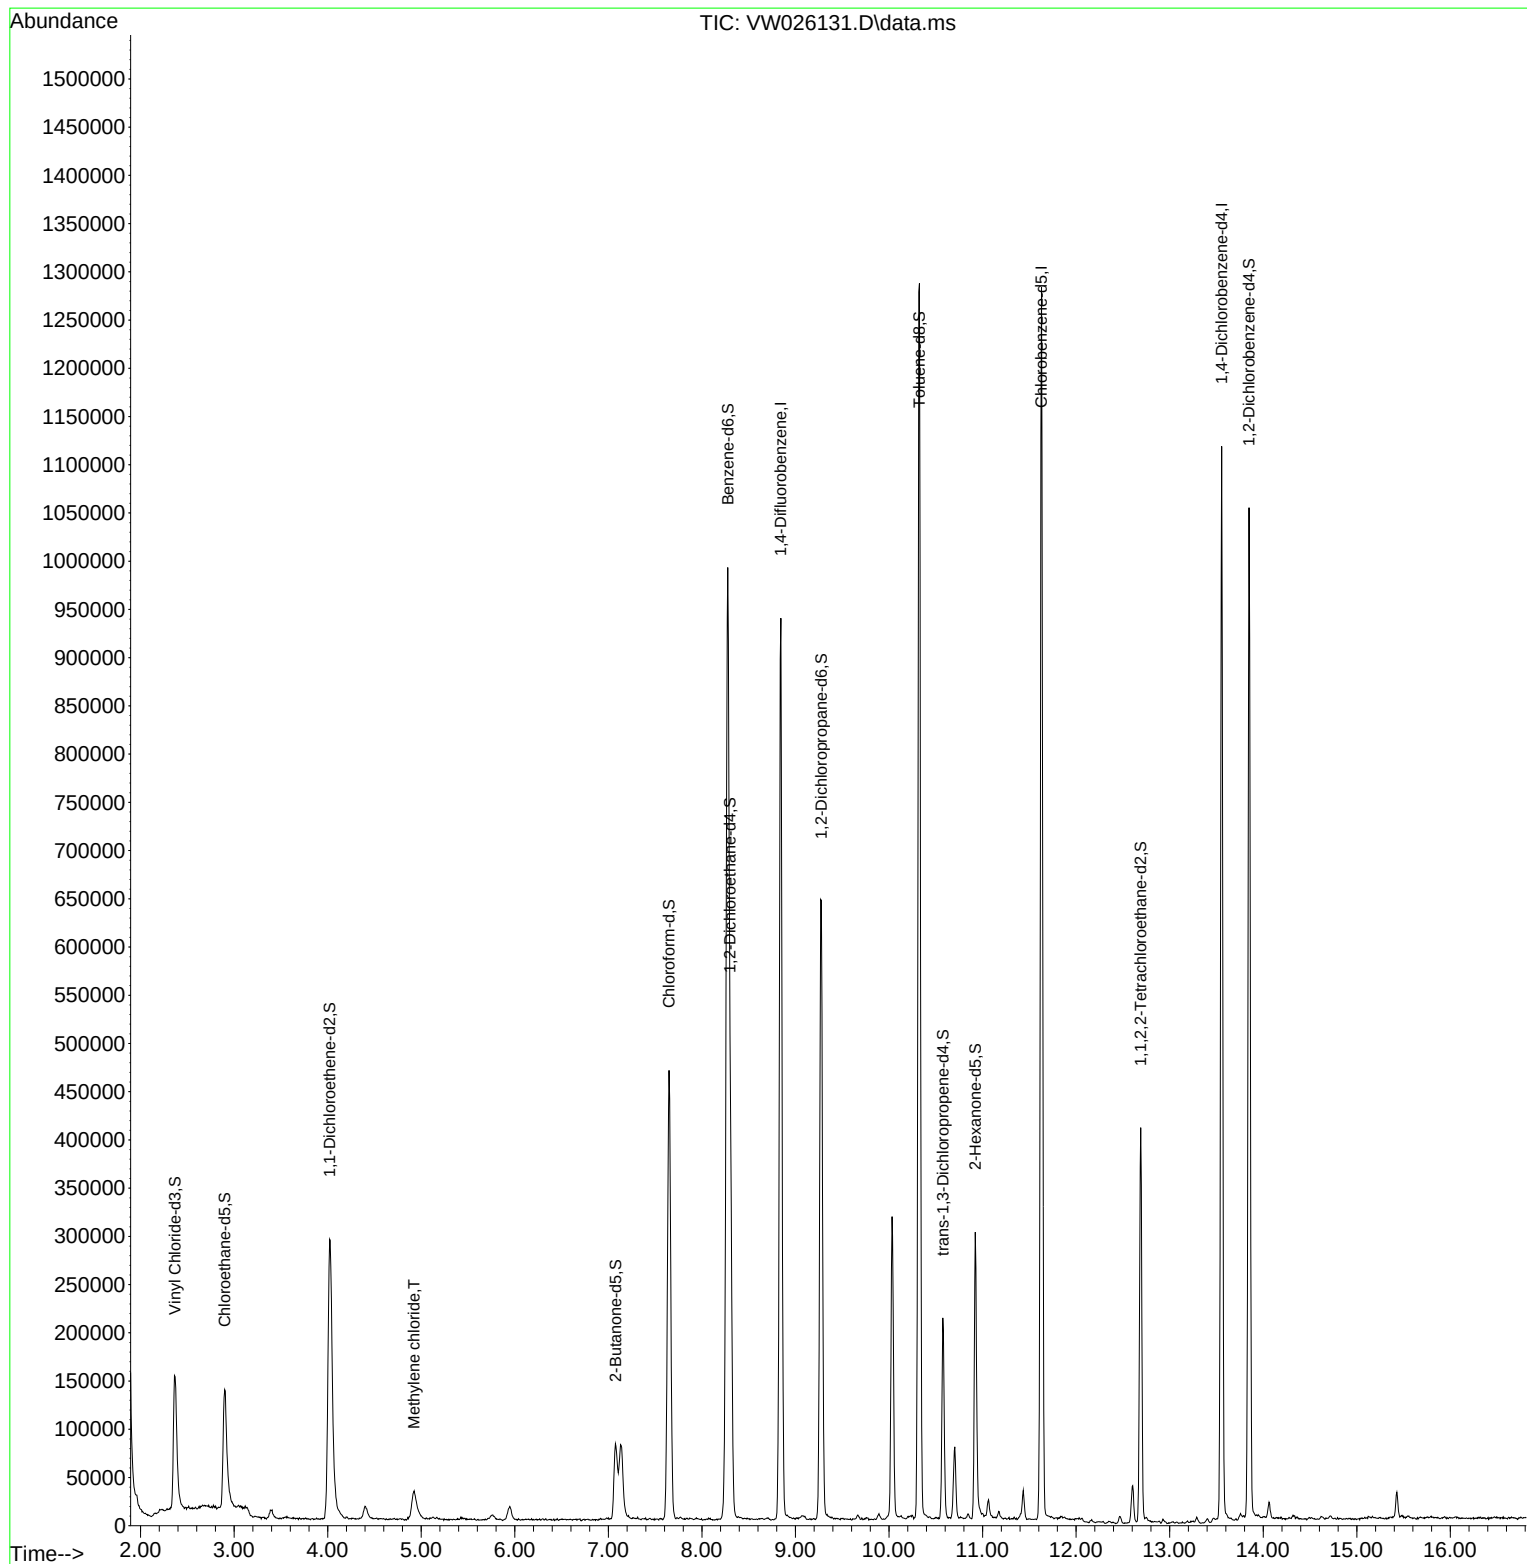

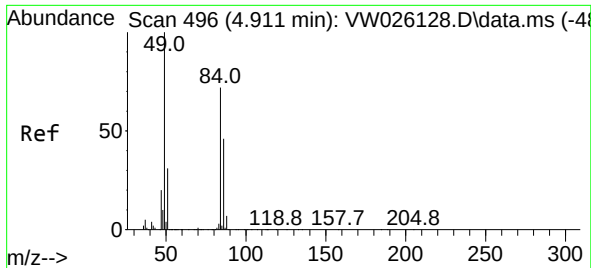

#16
Methylene chloride
Concen: 2.037 ug/L
RT: 4.923 min Scan# 49
Delta R.T. 0.012 min
Lab File: VW026131.D
Acq: 08 Jun 2023 11:44

Instrument :
MSVOA_W
ClientSampleId :
VHBLK002

Tgt Ion: 84	Resp:	23616
Ion Ratio	Lower	Upper
84	100	
86	64.1	44.2 82.0
49	133.8	98.8 183.6

