

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060823\
 Data File : VW026141.D
 Acq On : 08 Jun 2023 19:06
 Operator : SY/MD
 Sample : 03101-01
 Misc : 8.79g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZEL6

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 06/09/2023
 Supervised By :Mahesh Dadoda 06/09/2023

Quant Time: Jun 09 01:37:33 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 09 01:33:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	130531	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	119058	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	41910	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	46992	25.591	ug/L	-0.02
Spiked Amount 25.000	Range 30 - 150		Recovery = 102.360%			
7) Chloroethane-d5	2.887	69	42055	30.594	ug/L	-0.02
Spiked Amount 25.000	Range 30 - 150		Recovery = 122.360%			
11) 1,1-Dichloroethene-d2	4.021	65	23076	25.485	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 101.960%			
21) 2-Butanone-d5	7.088	46	27372	51.200	ug/L	0.01
Spiked Amount 50.000	Range 20 - 135		Recovery = 102.400%			
24) Chloroform-d	7.648	84	97477	25.501	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 102.000%			
26) 1,2-Dichloroethane-d4	8.307	65	60416	28.905	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 115.600%			
32) Benzene-d6	8.276	84	179149	22.362	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 89.440%			
36) 1,2-Dichloropropane-d6	9.270	67	63845	25.155	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 100.640%			
41) Toluene-d8	10.319	98	135220	19.033	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 76.120%			
43) trans-1,3-Dichloroprop...	10.575	79	20505	20.388	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 81.560%			
47) 2-Hexanone-d5	10.928	63	9655	24.126	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 48.260%			
56) 1,1,2,2-Tetrachloroeth...	12.690	84	56764	30.735	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 122.920%#			
66) 1,2-Dichlorobenzene-d4	13.848	152	36406	22.695	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 90.800%			
Target Compounds					Qvalue	
13) Acetone	4.137	43	3864m	9.341	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060823\
Data File : VW026141.D
Acq On : 08 Jun 2023 19:06
Operator : SY/MD
Sample : 03101-01
Misc : 8.79g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EZEL6

Quant Time: Jun 09 01:37:33 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 09 01:33:49 2023
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 06/09/2023
Supervised By : Mahesh Dadoda 06/09/2023

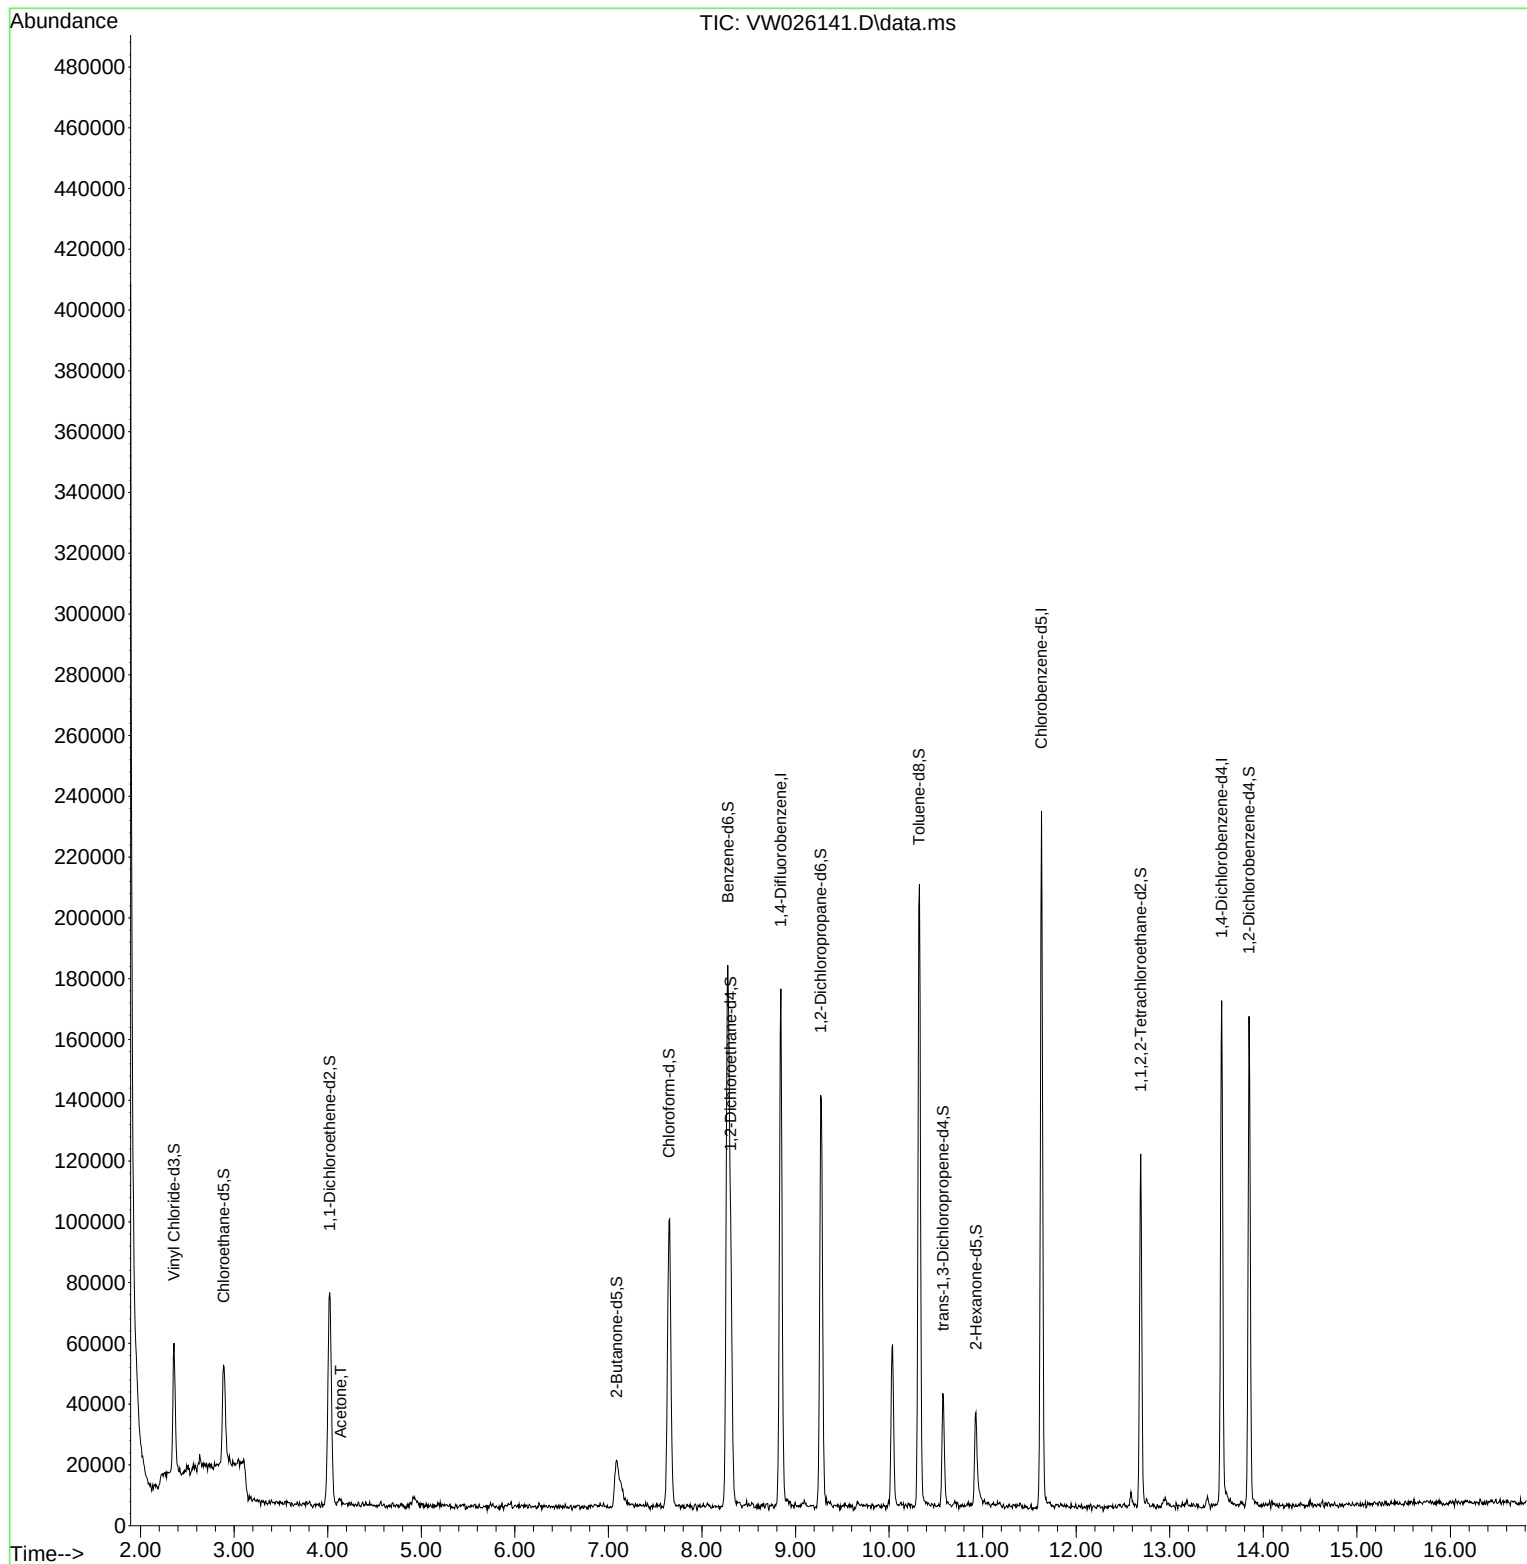

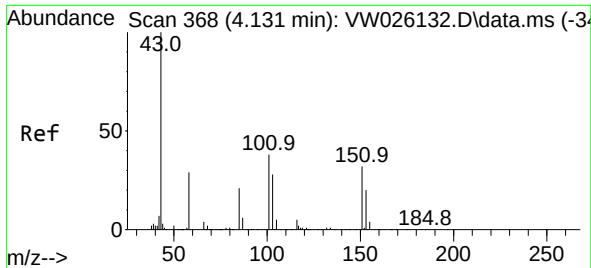

#13

Acetone

Concen: 9.341 ug/L m

RT: 4.137 min Scan# 30

Delta R.T. 0.006 min

Lab File: VW026141.D

Acq: 08 Jun 2023 19:06

Instrument :

MSVOA_W

ClientSampleId :

EZEL6

Tgt Ion: 43 Resp: 386

Ion Ratio Lower Upper

43 100

58 17.6 0.0 58.2

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 06/09/2023

Supervised By :Mahesh Dadoda 06/09/2023

