

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060823\
 Data File : VW026143.D
 Acq On : 08 Jun 2023 19:54
 Operator : SY/MD
 Sample : 03101-07
 Misc : 7.69g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZEM0

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 06/09/2023
 Supervised By :Mahesh Dadoda 06/09/2023

Quant Time: Jun 09 01:37:58 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 09 01:33:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	907029	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	723514	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	224305	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	241588	18.933	ug/L	-0.01
Spiked Amount 25.000	Range 30 - 150		Recovery =	75.720%		
7) Chloroethane-d5	2.893	69	234518	24.552	ug/L	-0.01
Spiked Amount 25.000	Range 30 - 150		Recovery =	98.200%		
11) 1,1-Dichloroethene-d2	4.021	65	129064	20.513	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	82.040%		
21) 2-Butanone-d5	7.075	46	174887	47.077	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	94.160%		
24) Chloroform-d	7.648	84	589160	22.181	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	88.720%		
26) 1,2-Dichloroethane-d4	8.307	65	352045m	24.239	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	96.960%		
32) Benzene-d6	8.276	84	1172426	24.082	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	96.320%		
36) 1,2-Dichloropropane-d6	9.276	67	396887	25.732	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	102.920%		
41) Toluene-d8	10.325	98	956577	22.156	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	88.640%		
43) trans-1,3-Dichloroprop...	10.575	79	114412	18.719	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	74.880%		
47) 2-Hexanone-d5	10.922	63	113122	46.514	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	93.020%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	281252	25.059	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	100.240%		
66) 1,2-Dichlorobenzene-d4	13.848	152	195041	22.718	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	90.880%		
Target Compounds					Qvalue	
13) Acetone	4.118	43	15960	5.552	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060823\
Data File : VW026143.D
Acq On : 08 Jun 2023 19:54
Operator : SY/MD
Sample : 03101-07
Misc : 7.69g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EZEM0

Quant Time: Jun 09 01:37:58 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 09 01:33:49 2023
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 06/09/2023
Supervised By : Mahesh Dadoda 06/09/2023

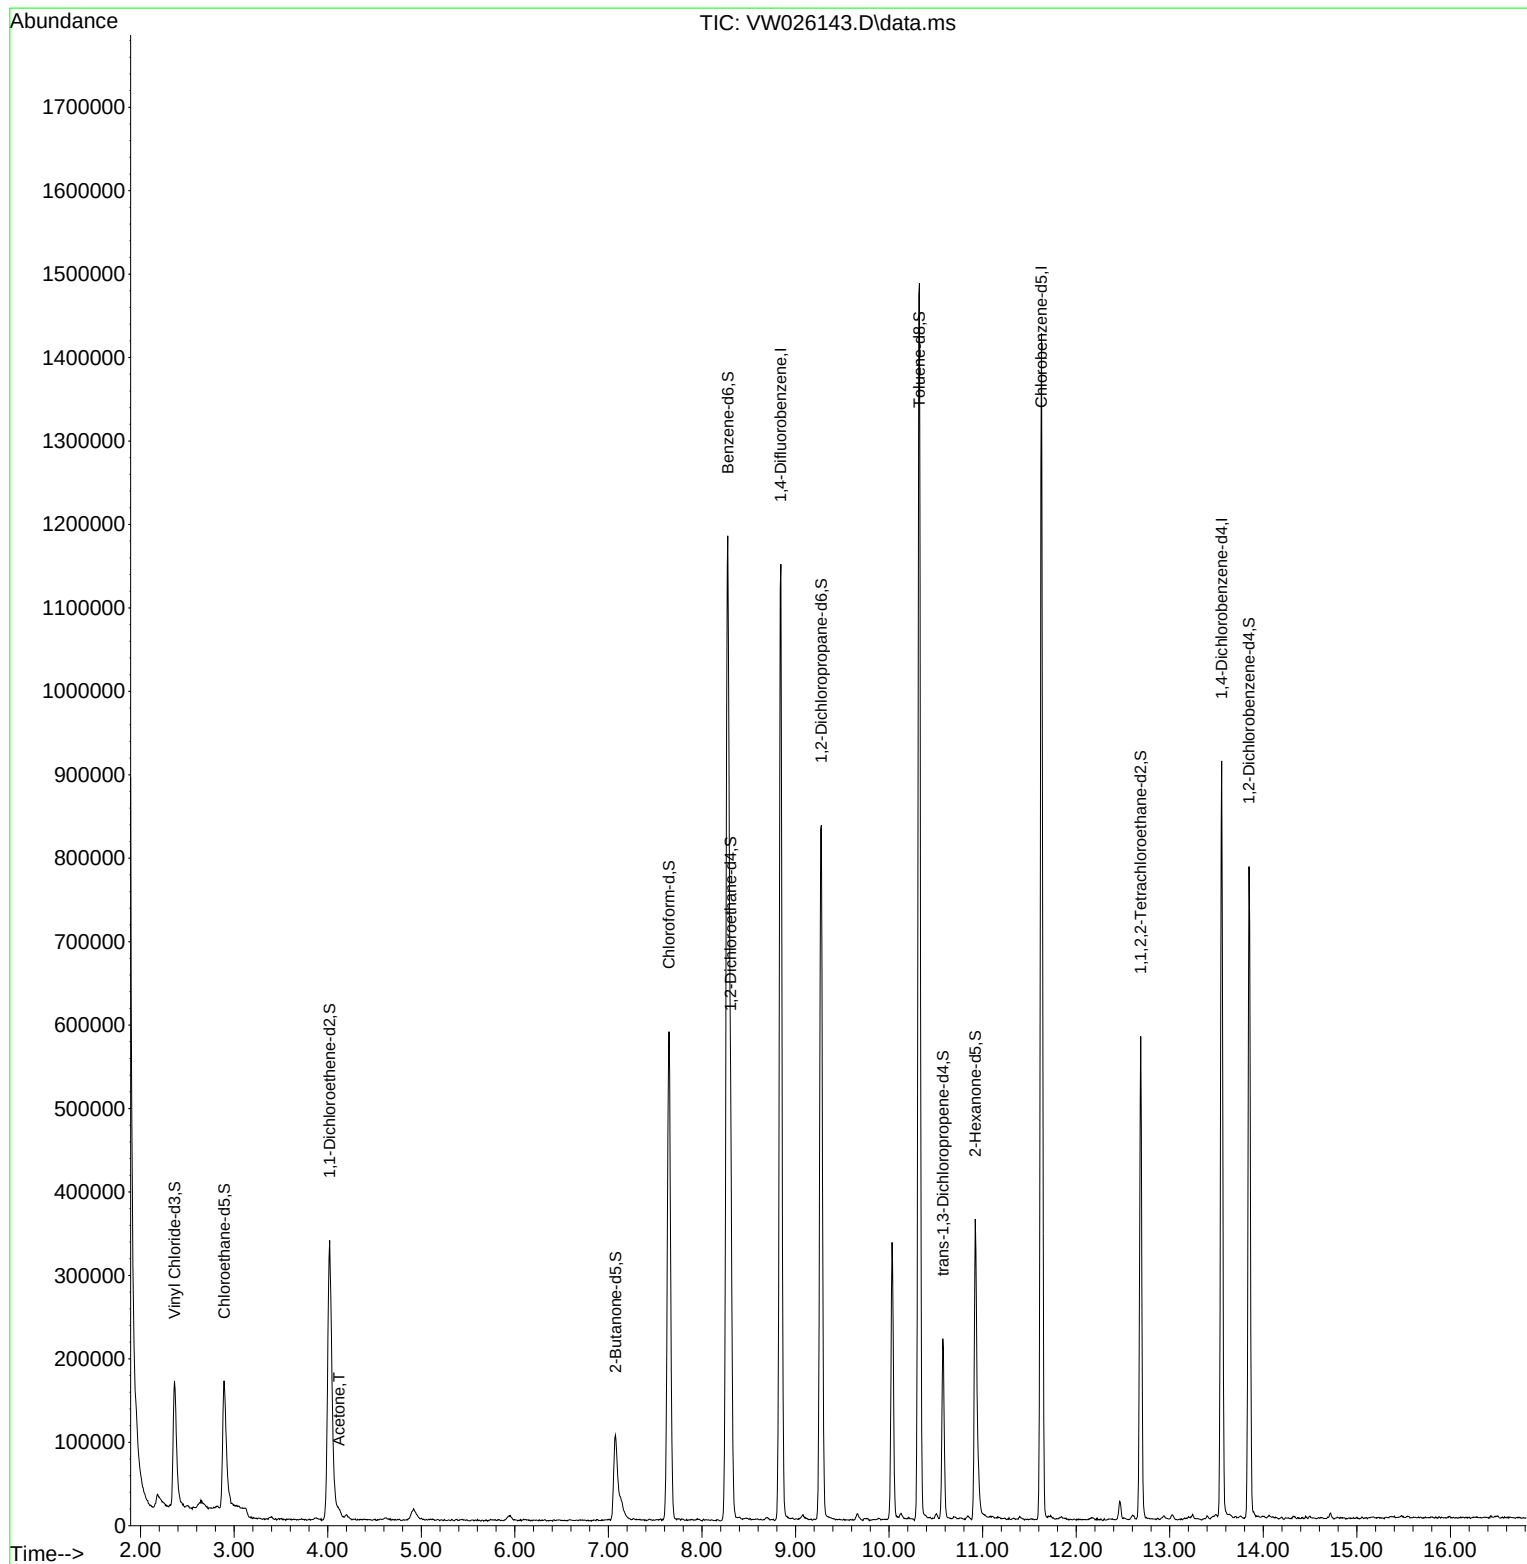

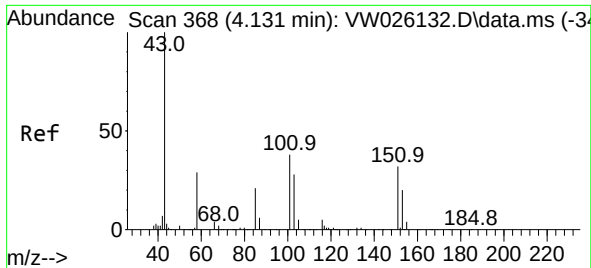

#13

Acetone

Concen: 5.552 ug/L

RT: 4.118 min Scan# 30

Delta R.T. -0.012 min

Lab File: VW026143.D

Acq: 08 Jun 2023 19:54

Instrument :

MSVOA_W

ClientSampleId :

EZEM0

Tgt Ion: 43 Resp: 1596

Ion Ratio Lower Upper

43 100

58 28.7 0.0 58.2

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 06/09/2023

Supervised By :Mahesh Dadoda 06/09/2023

