
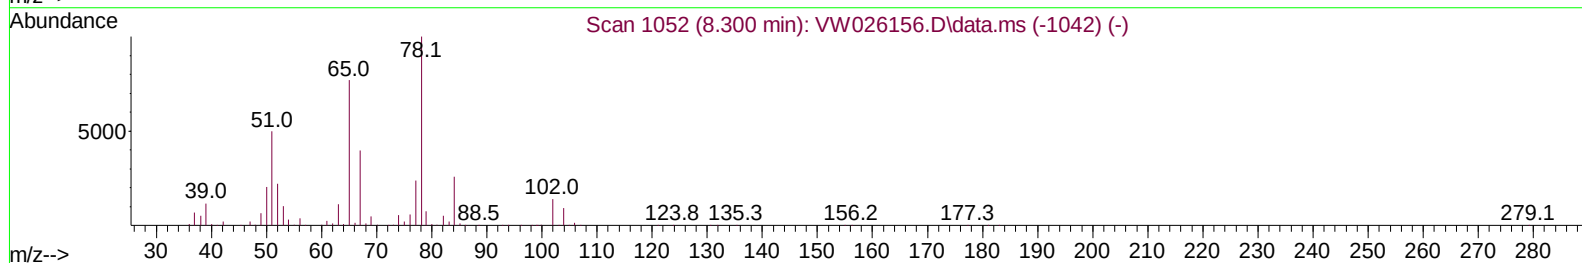
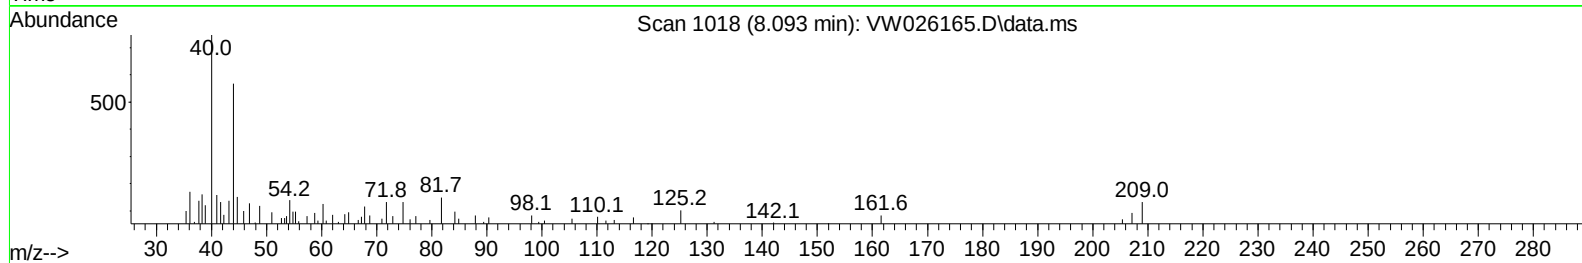


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060923\
 Data File : VW026165.D
 Acq On : 09 Jun 2023 13:01
 Operator : SY/MD
 Sample : VIBLK472
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 22:55:10 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 09 22:52:55 2023
 Response via : Initial Calibration

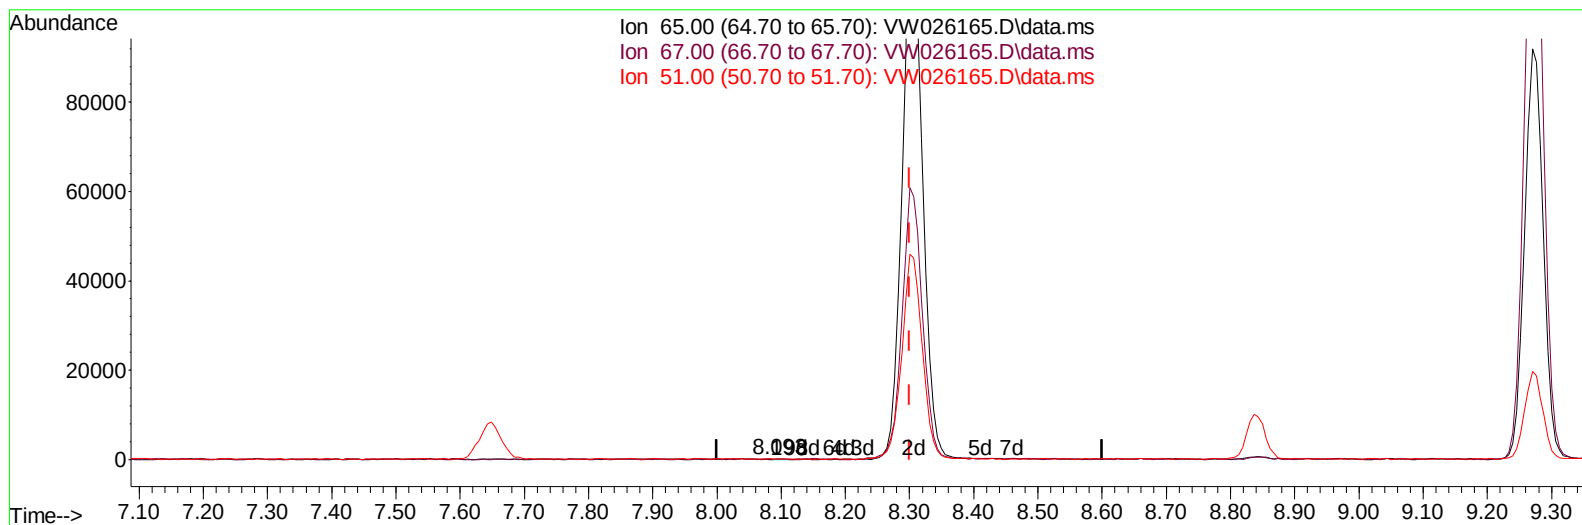




TIC: VW026165.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)**8.093min (-0.207) 0.01 ug/L****response 77**

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.70	46.75
51.00	106.50	105.19
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060923\
 Data File : VW026165.D
 Acq On : 09 Jun 2023 13:01
 Operator : SY/MD
 Sample : VIBLK472
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 22:55:10 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 09 22:52:55 2023
 Response via : Initial Calibration

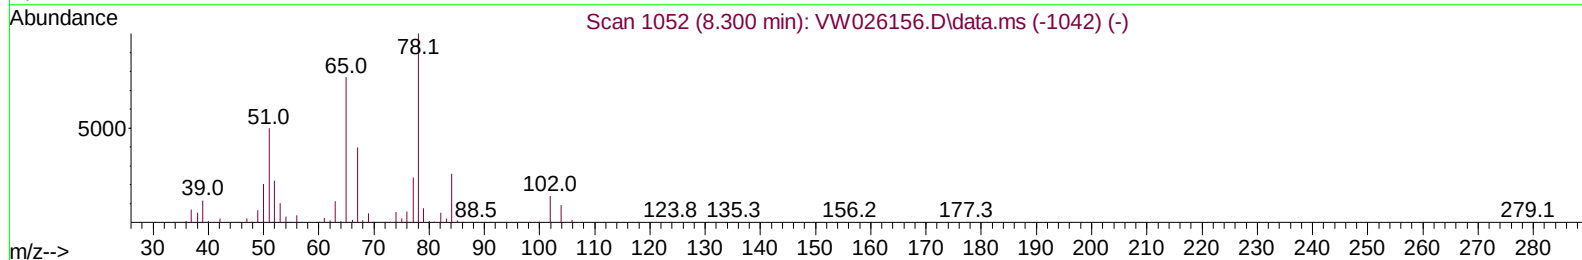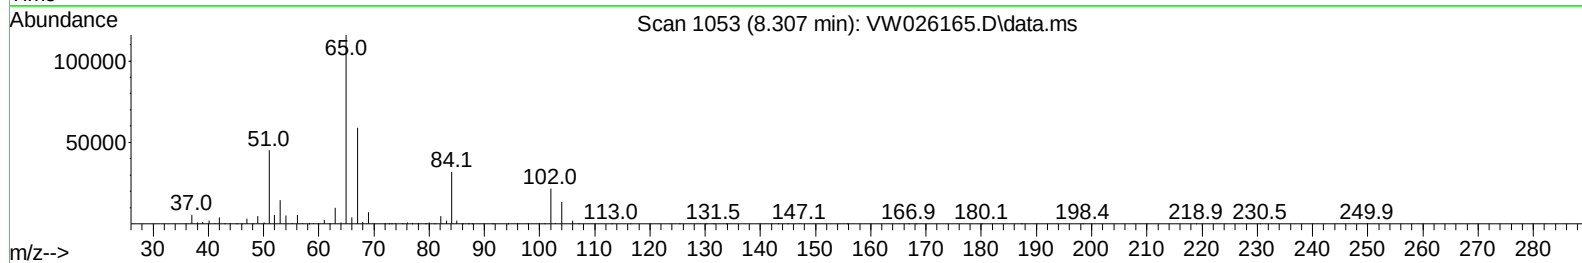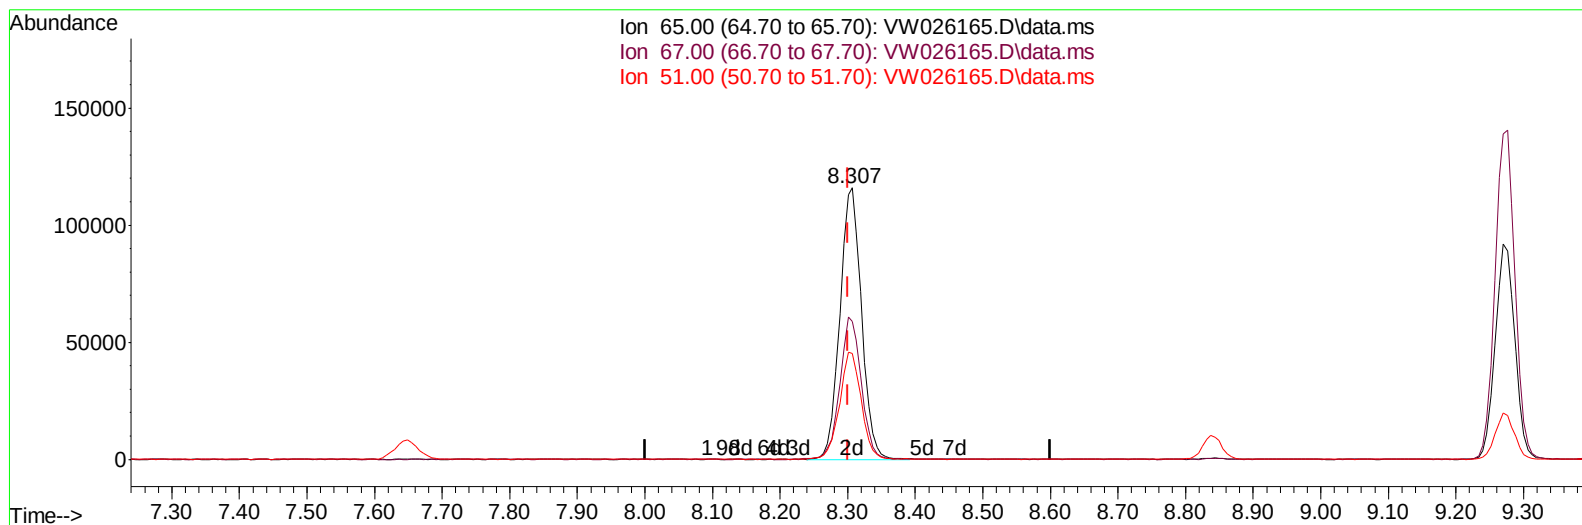

TIC: VW026165.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)**8.307min (+ 0.006) 19.21 ug/L m****response 257885**

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.70	0.01#
51.00	106.50	0.03#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060923\
 Data File : VW026165.D
 Acq On : 09 Jun 2023 13:01
 Operator : SY/MD
 Sample : VIBLK472
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 22:55:10 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 09 22:52:55 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	838344	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	748099	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	366432	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	209175	17.736	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	70.960%	
7) Chloroethane-d5	2.899	69	179203	20.298	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	81.200%	
11) 1,1-Dichloroethene-d2	4.021	65	104538	17.976	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	71.920%	
21) 2-Butanone-d5	7.075	46	143391	41.761	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	83.520%	
24) Chloroform-d	7.648	84	447499	18.228	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	72.920%	
26) 1,2-Dichloroethane-d4	8.307	65	257885m	19.210	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	76.840%	
32) Benzene-d6	8.270	84	890183	17.684	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	70.720%	
36) 1,2-Dichloropropane-d6	9.276	67	286112	17.941	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	71.760%	
41) Toluene-d8	10.319	98	772996	17.315	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	69.280%	
43) trans-1,3-Dichloroprop...	10.575	79	101441	16.052	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	64.200%	
47) 2-Hexanone-d5	10.922	63	90507	35.992	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	71.980%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	216968	18.696	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	74.800%	
66) 1,2-Dichlorobenzene-d4	13.848	152	248812	17.740	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	70.960%#	
Target Compounds						
16) Methylene chloride	4.923	84	28559	2.134	ug/L	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060923\
Data File : VW026165.D
Acq On : 09 Jun 2023 13:01
Operator : SY/MD
Sample : VIBLK472
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 22:55:10 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 09 22:52:55 2023
Response via : Initial Calibration

