

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060923\
 Data File : VW026159.D
 Acq On : 09 Jun 2023 10:33
 Operator : SY/MD
 Sample : VIBLK469
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK469

Quant Time: Jun 09 22:53:59 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 09 22:52:55 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	863245	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	760830	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	362626	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	258767	21.308	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	85.240%
7) Chloroethane-d5	2.893	69	223195	24.552	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	98.200%
11) 1,1-Dichloroethene-d2	4.021	65	133567	22.305	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	89.240%
21) 2-Butanone-d5	7.075	46	176659	49.966	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	99.940%
24) Chloroform-d	7.642	84	549461	21.736	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	86.960%
26) 1,2-Dichloroethane-d4	8.307	65	322241	23.312	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	93.240%
32) Benzene-d6	8.270	84	1115874	21.796	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	87.200%
36) 1,2-Dichloropropane-d6	9.270	67	356503	21.980	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	87.920%
41) Toluene-d8	10.319	98	971571	21.399	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	85.600%
43) trans-1,3-Dichloroprop...	10.575	79	133867	20.828	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.320%
47) 2-Hexanone-d5	10.922	63	115021	44.975	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.960%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	261709	22.174	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	88.680%
66) 1,2-Dichlorobenzene-d4	13.849	152	295979	21.324	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	85.280%
Target Compounds					Qvalue	
13) Acetone	4.125	43	8804	3.218	ug/L	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060923\
Data File : VW026159.D
Acq On : 09 Jun 2023 10:33
Operator : SY/MD
Sample : VIBLK469
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK469

Quant Time: Jun 09 22:53:59 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 09 22:52:55 2023
Response via : Initial Calibration

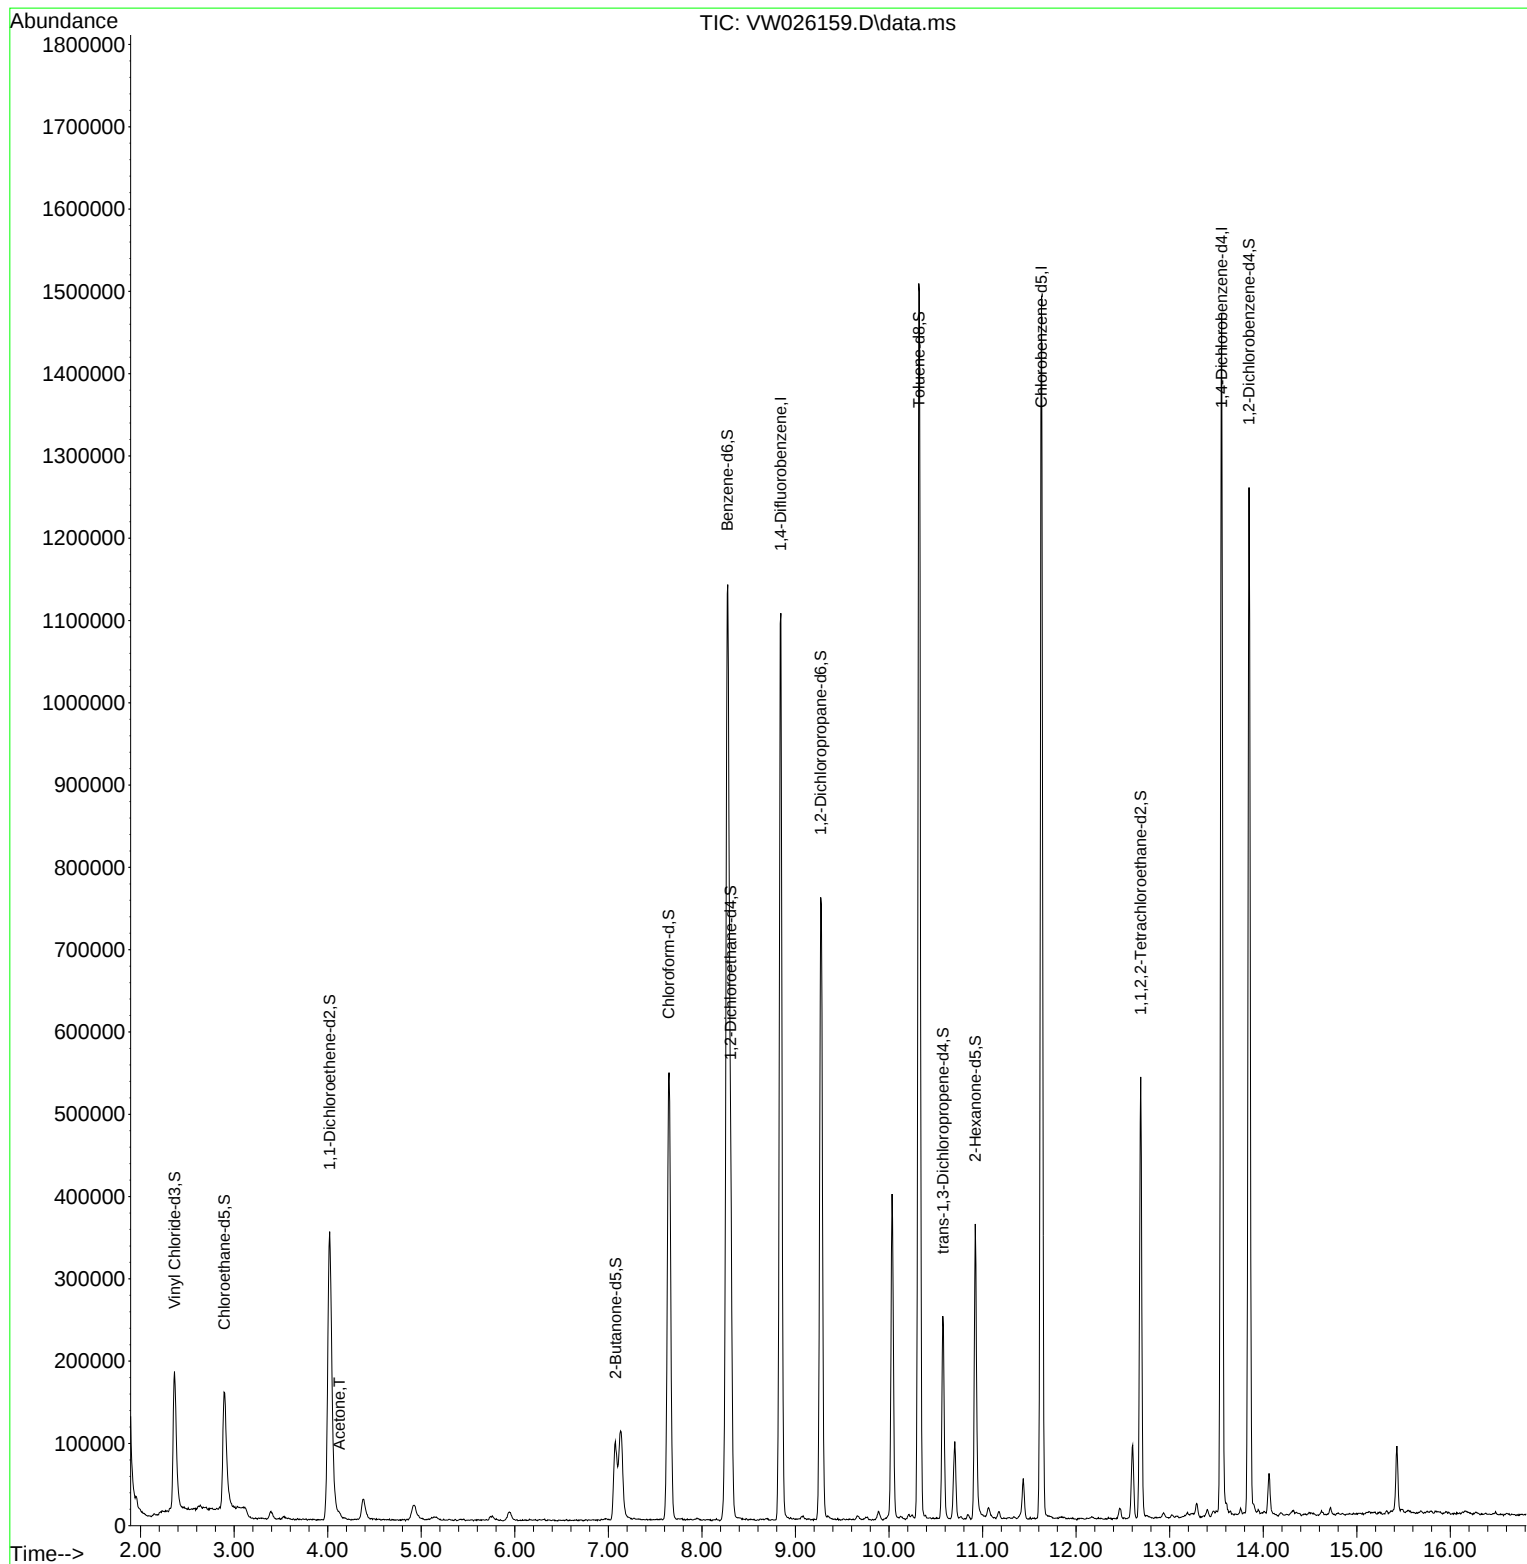

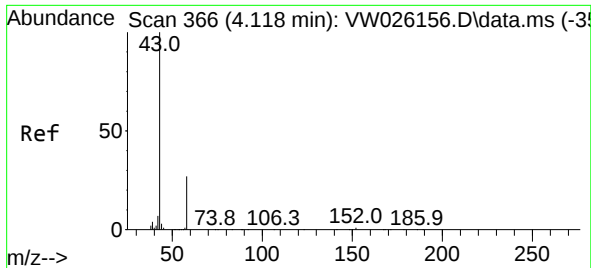

#13
 Acetone
 Concen: 3.218 ug/L
 RT: 4.125 min Scan# 30
 Delta R.T. 0.007 min
 Lab File: VW026159.D
 Acq: 09 Jun 2023 10:33

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK469

Tgt Ion: 43 Resp: 8804
 Ion Ratio Lower Upper
 43 100
 58 9.5 0.0 58.2

