

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060923\
 Data File : VW026161.D
 Acq On : 09 Jun 2023 11:21
 Operator : SY/MD
 Sample : 03101-02RE
 Misc : 18.18g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZEL7RE

Quant Time: Jun 09 22:54:22 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 09 22:52:55 2023
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		8.843	114	68085	25.000	ug/L	0.00
28) Chlorobenzene-d5		11.629	117	57895	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		13.556	152	17289	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		2.357	65	24907	26.004	ug/L	-0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	= 104.000%		
7) Chloroethane-d5		2.893	69	23468	32.731	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	= 130.920%		
11) 1,1-Dichloroethene-d2		4.021	65	12584	26.645	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	= 106.560%		
21) 2-Butanone-d5		7.087	46	10211	36.618	ug/L	0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	= 73.240%		
24) Chloroform-d		7.654	84	47937	24.043	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	= 96.160%		
26) 1,2-Dichloroethane-d4		8.307	65	31868m	29.231	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	= 116.920%		
32) Benzene-d6		8.276	84	90698	23.282	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	= 93.120%		
36) 1,2-Dichloropropane-d6		9.276	67	31287	25.350	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	= 101.400%		
41) Toluene-d8		10.325	98	68236	19.751	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	= 79.000%		
43) trans-1,3-Dichloroprop...		10.581	79	8845	18.085	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	= 72.360%		
47) 2-Hexanone-d5		10.928	63	3968m	20.390	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	= 40.780%		
56) 1,1,2,2-Tetrachloroeth...		12.690	84	22548	25.106	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	= 100.440%		
66) 1,2-Dichlorobenzene-d4		13.848	152	16244	24.547	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	= 98.200%		
Target Compounds							Qvalue
13) Acetone		4.125	43	3517m	16.300	ug/L	


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060923\
Data File : VW026161.D
Acq On : 09 Jun 2023 11:21
Operator : SY/MD
Sample : 03101-02RE
Misc : 18.18g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EZEL7RE

Quant Time: Jun 09 22:54:22 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 09 22:52:55 2023
Response via : Initial Calibration

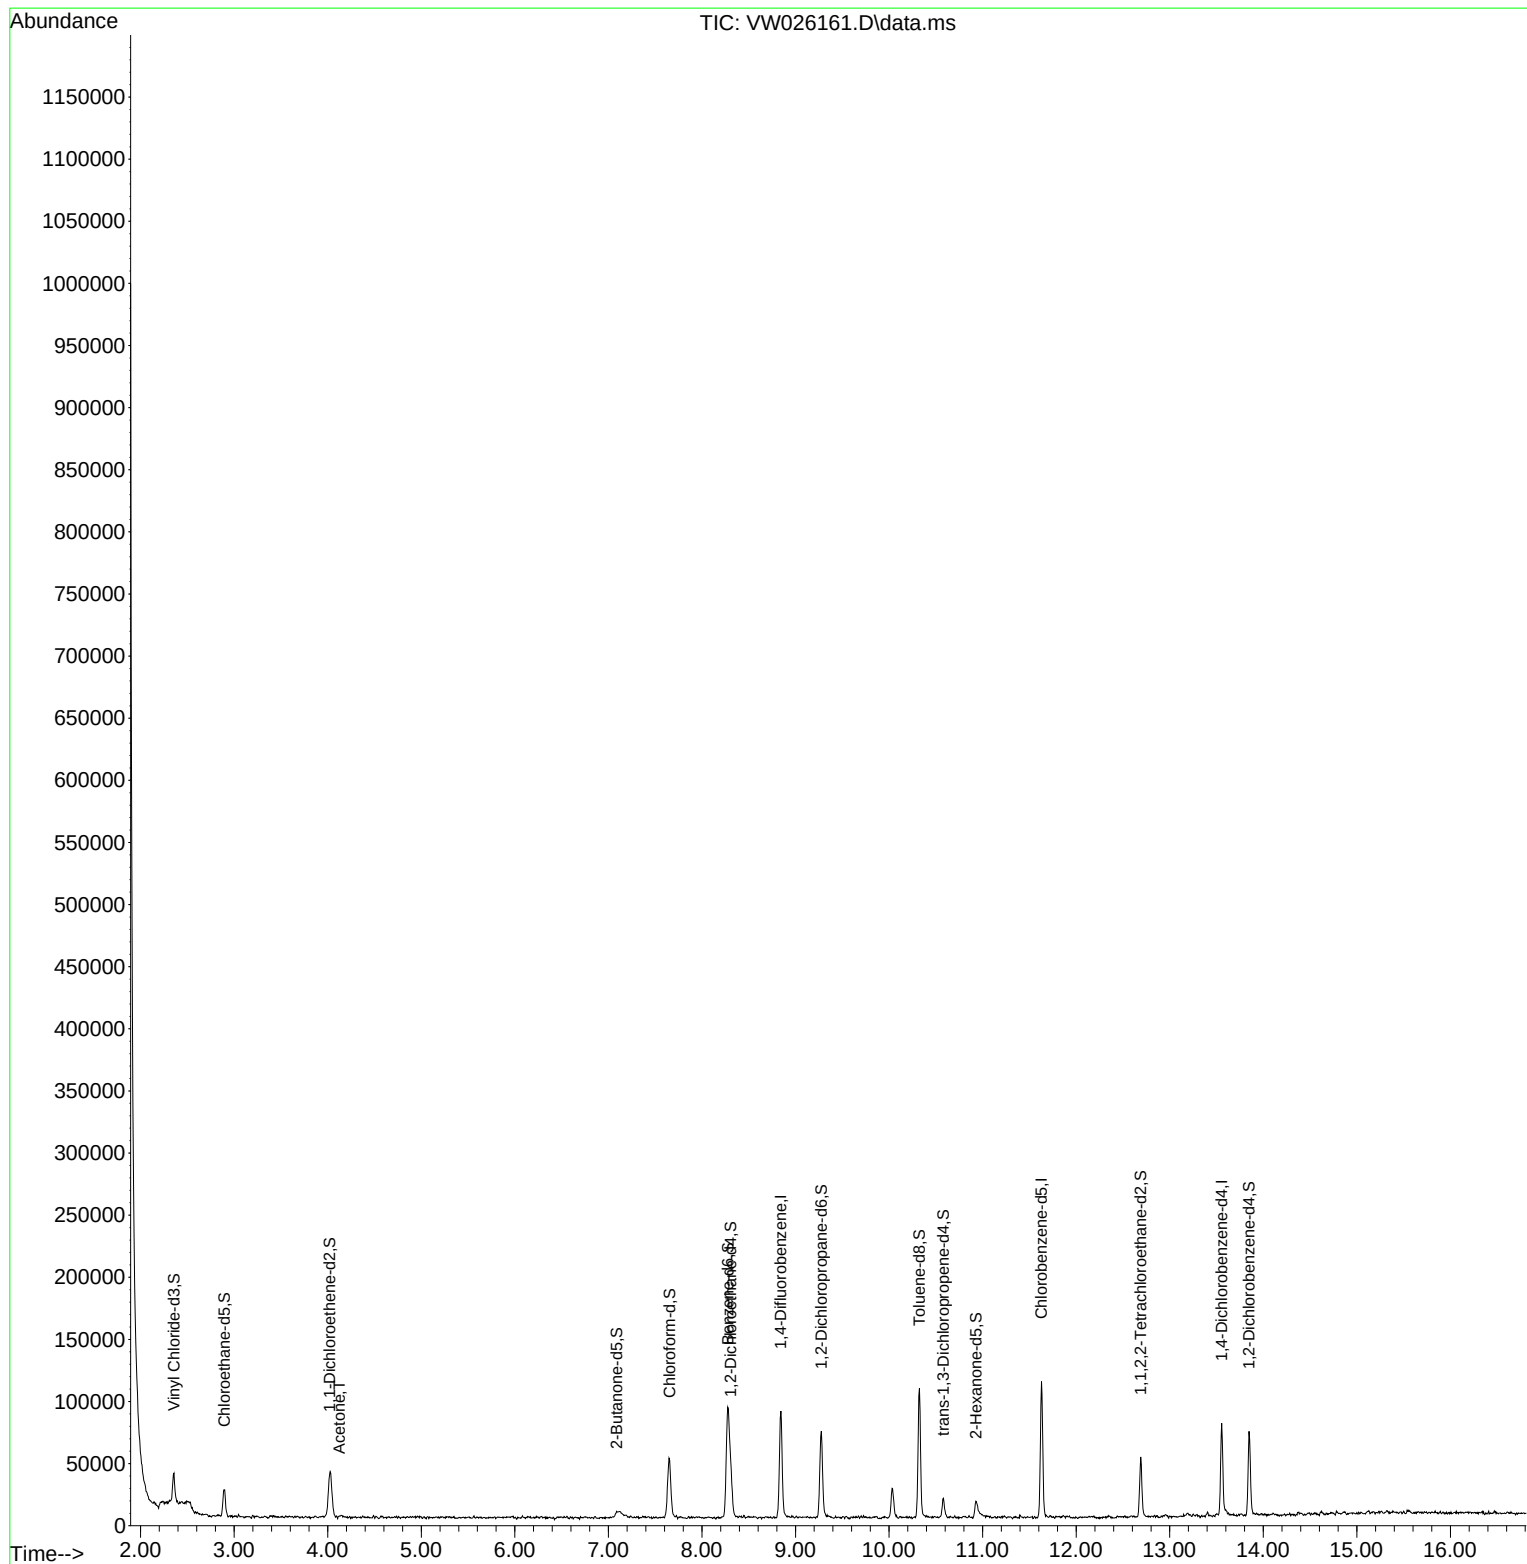

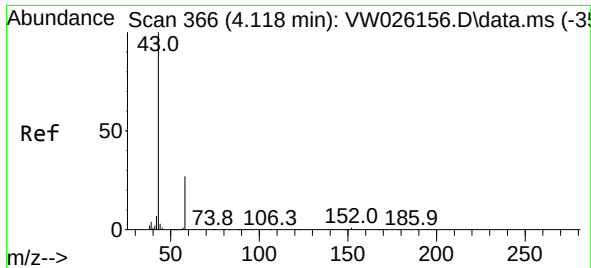

#13
 Acetone
 Concen: 16.300 ug/L m
 RT: 4.125 min Scan# 3
 Delta R.T. 0.006 min
 Lab File: VW026161.D
 Acq: 09 Jun 2023 11:21

Instrument :
 MSVOA_W
 ClientSampleId :
 EZEL7RE

Tgt Ion: 43 Resp: 3517
 Ion Ratio Lower Upper
 43 100
 58 7.3 0.0 58.2

