

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060923\
 Data File : VW026166.D
 Acq On : 09 Jun 2023 13:25
 Operator : SY/MD
 Sample : 03078-07
 Misc : 5.85g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 ESQX4

Quant Time: Jun 09 22:55:21 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 09 22:52:55 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	736046	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	615516	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	245388	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	224756	21.706	ug/L	-0.01
Spiked Amount	25.000	Range 30 - 150	Recovery	=	86.840%	
7) Chloroethane-d5	2.893	69	192178	24.793	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	99.160%	
11) 1,1-Dichloroethene-d2	4.015	65	112953	22.123	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery	=	88.480%	
21) 2-Butanone-d5	7.075	46	124691	41.362	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	82.720%	
24) Chloroform-d	7.648	84	471846	21.891	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	=	87.560%	
26) 1,2-Dichloroethane-d4	8.307	65	264844	22.471	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	=	89.880%	
32) Benzene-d6	8.276	84	922803	22.281	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	=	89.120%	
36) 1,2-Dichloropropane-d6	9.276	67	297619	22.682	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	=	90.720%	
41) Toluene-d8	10.325	98	769697	20.955	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	=	83.840%	
43) trans-1,3-Dichloroprop...	10.575	79	98708	18.984	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	=	75.920%	
47) 2-Hexanone-d5	10.922	63	74124	35.827	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	71.660%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	198086	20.746	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	=	83.000%	
66) 1,2-Dichlorobenzene-d4	13.848	152	189293	20.154	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	=	80.600%	
Target Compounds						
13) Acetone	4.125	43	21132	9.059	ug/L	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060923\
Data File : VW026166.D
Acq On : 09 Jun 2023 13:25
Operator : SY/MD
Sample : 03078-07
Misc : 5.85g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
ESQX4

Quant Time: Jun 09 22:55:21 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 09 22:52:55 2023
Response via : Initial Calibration

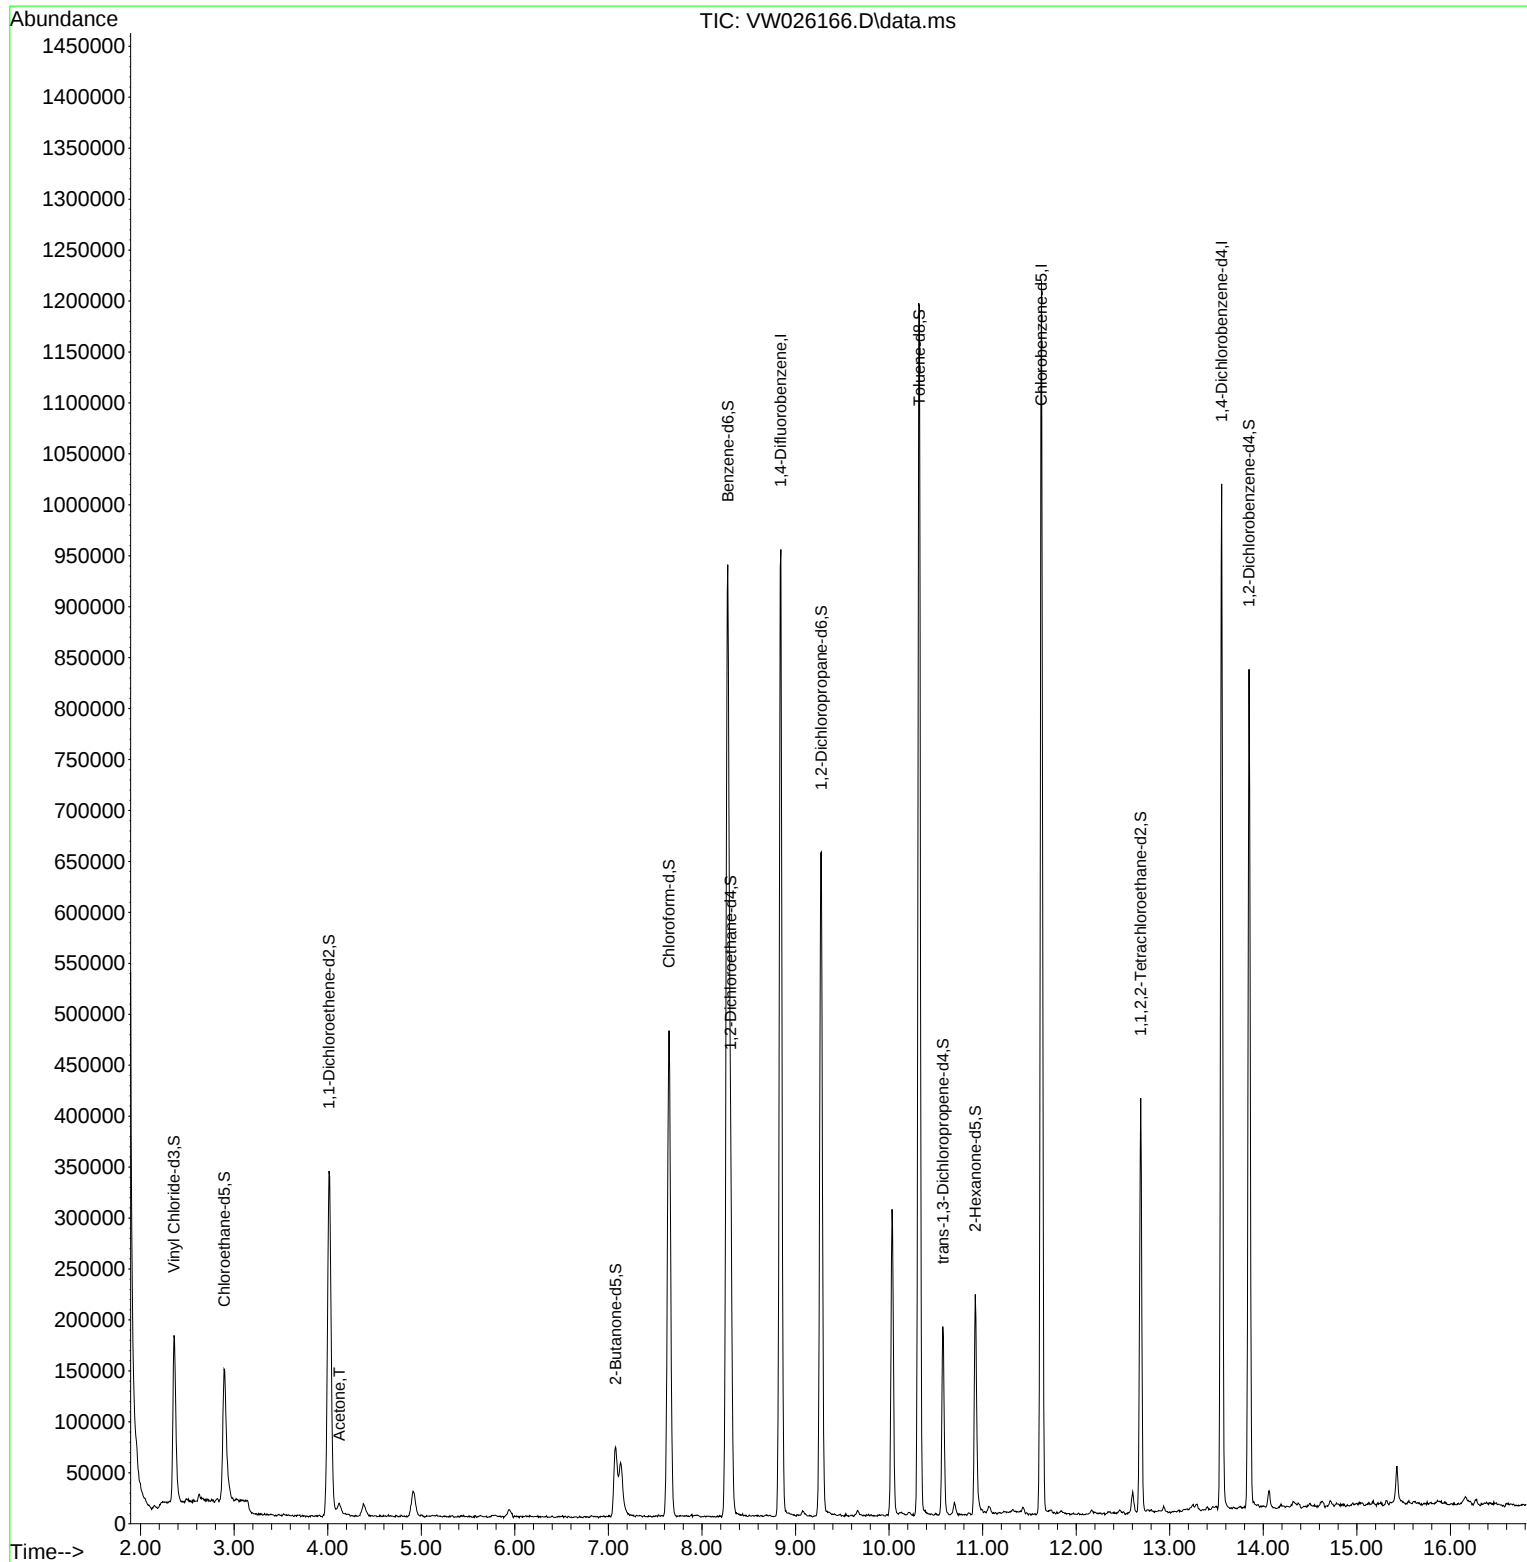

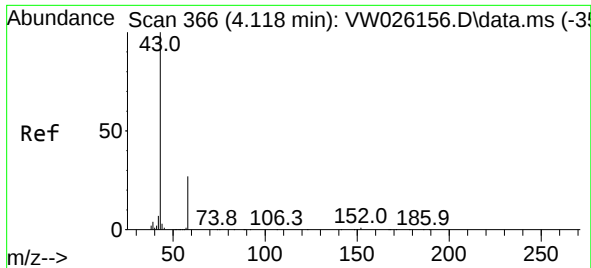

#13

Acetone

Concen: 9.059 ug/L

RT: 4.125 min Scan# 3

Delta R.T. 0.006 min

Lab File: VW026166.D


Acq: 09 Jun 2023 13:25

Instrument :

MSVOA_W

ClientSampleId :

ESQX4

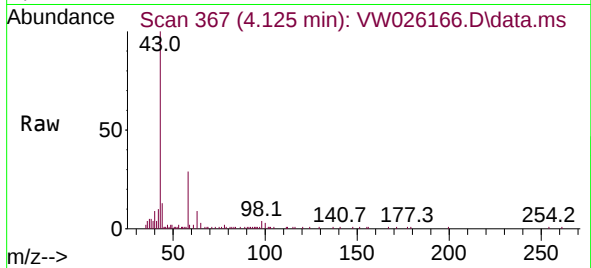

Tgt Ion: 43 Resp: 21132

Ion Ratio Lower Upper

43 100

58 25.1 0.0 58.2

