

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061022\
 Data File : VW023446.D
 Acq On : 10 Jun 2022 15:04
 Operator : SY/VA
 Sample : N3226-20
 Misc : 6.24g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Jun 11 00:08:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jun 11 00:06:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	407682	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	336377	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	122561	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	151506	23.392	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.560%
7) Chloroethane-d5	2.879	69	123583	25.957	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	103.840%
11) 1,1-Dichloroethene-d2	4.019	63	136917	15.145	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	60.560%
21) 2-Butanone-d5	7.080	46	31129	23.540	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	47.080%
24) Chloroform-d	7.647	84	268162	23.895	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.560%
26) 1,2-Dichloroethane-d4	8.305	65	157421	26.045	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	104.200%
32) Benzene-d6	8.275	84	491898	27.579	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	110.320%
36) 1,2-Dichloropropane-d6	9.274	67	154488	29.400	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	117.600%
41) Toluene-d8	10.323	98	429639	24.662	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	98.640%
43) trans-1,3-Dichloroprop...	10.579	79	43120	17.979	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	71.920%
47) 2-Hexanone-d5	10.926	63	22213	26.455	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	52.900%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	126557	25.787	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	103.160%
66) 1,2-Dichlorobenzene-d4	13.853	152	109259	24.695	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.760%
Target Compounds						
39) cis-1,3-Dichloropropene	10.036	75	3860	0.530	ug/L	Qvalue # 69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061022\
Data File : VW023446.D
Acq On : 10 Jun 2022 15:04
Operator : SY/VA
Sample : N3226-20
Misc : 6.24g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Jun 11 00:08:10 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jun 11 00:06:08 2022
Response via : Initial Calibration

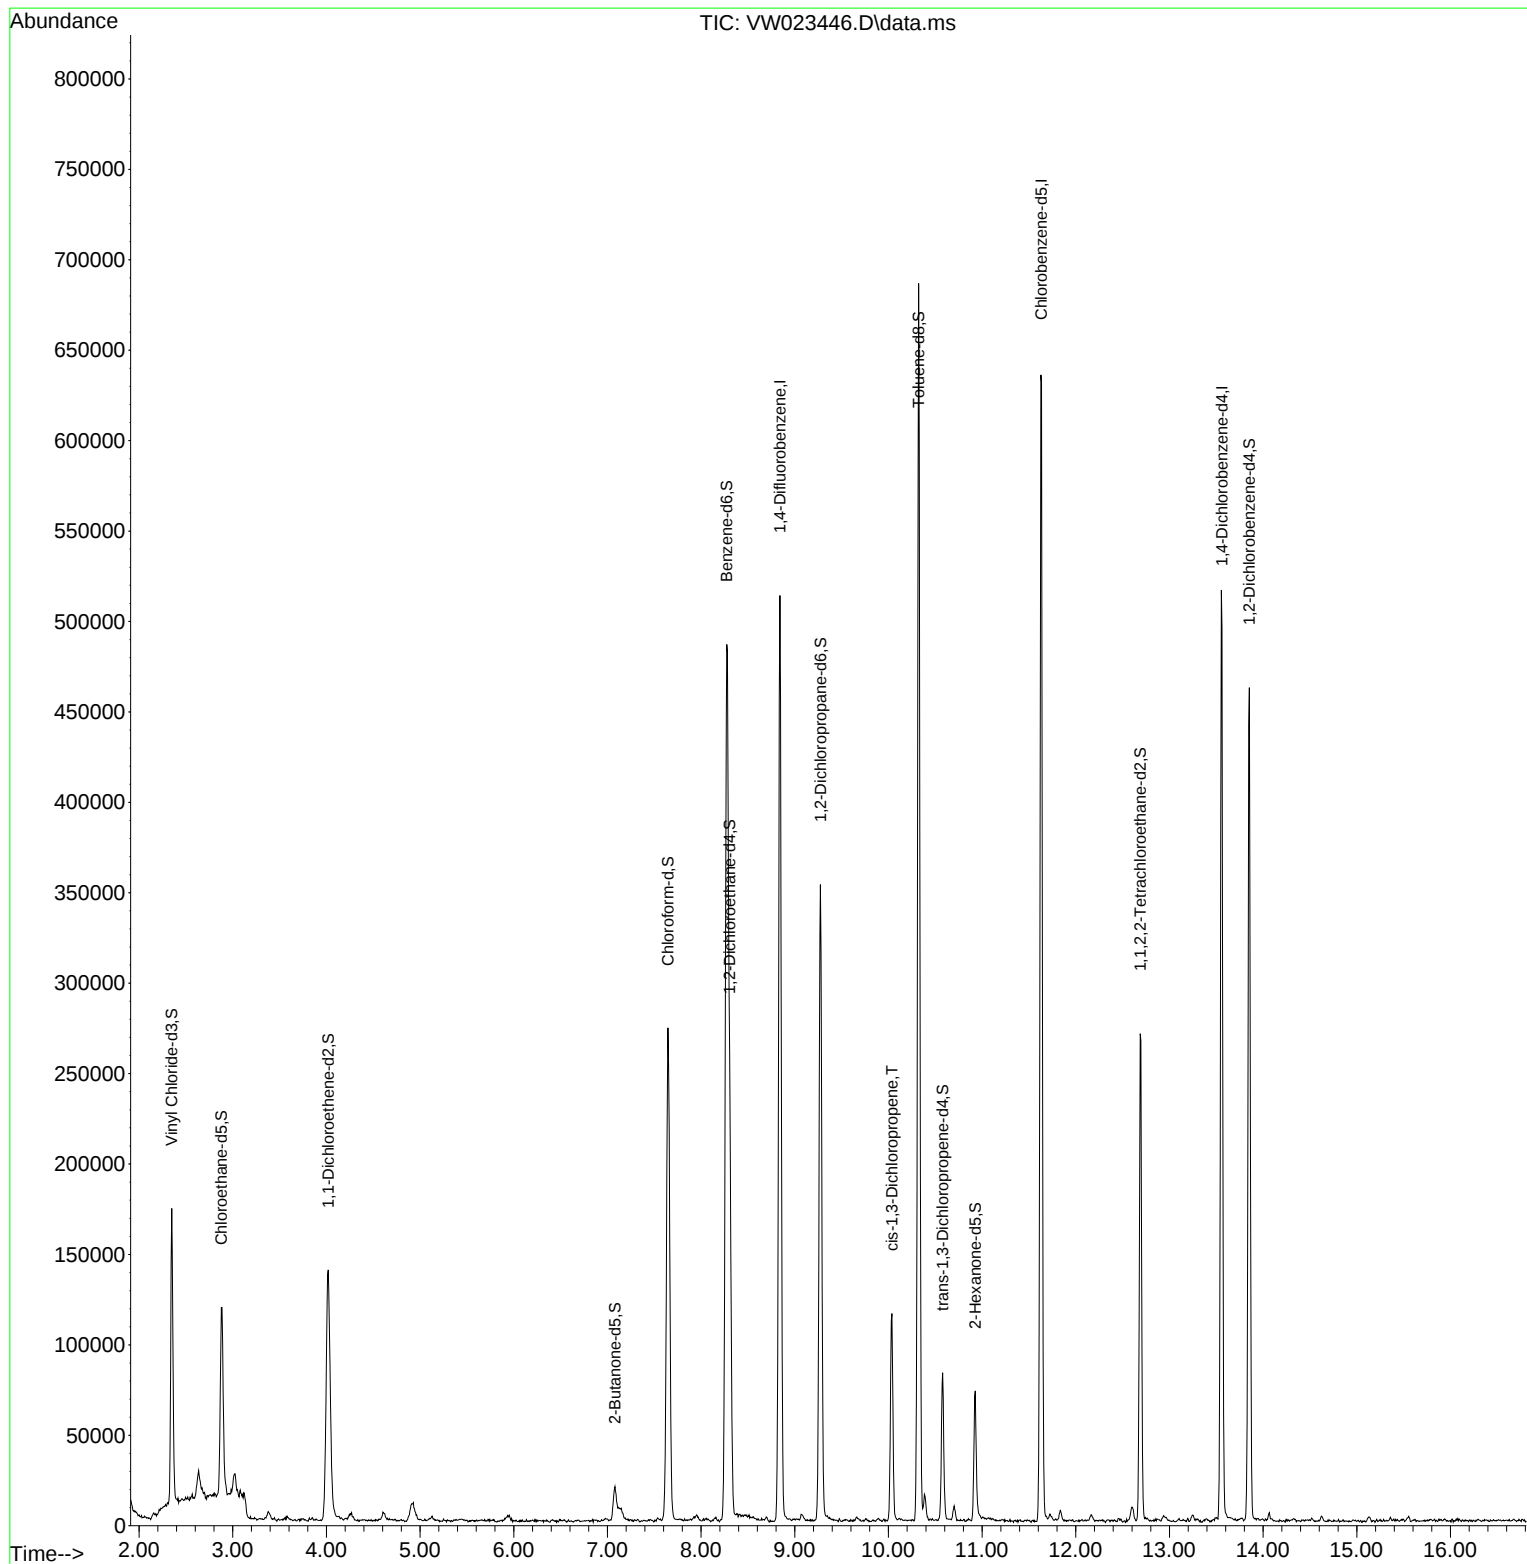

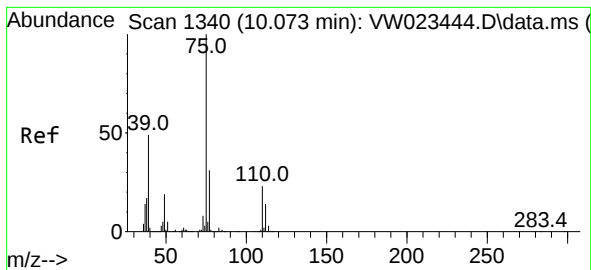

#39
 cis-1,3-Dichloropropene
 Concen: 0.530 ug/L
 RT: 10.036 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW023446.D
 Acq: 10 Jun 2022 15:04

Instrument :
 MSVOA_W
 ClientSampleId :

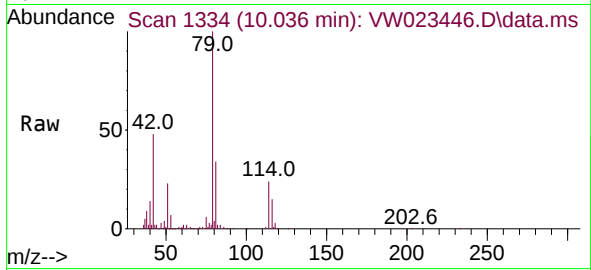

Tgt Ion: 75 Resp: 3860
 Ion Ratio Lower Upper
 75 100
 77 48.7 22.1 41.1#

