
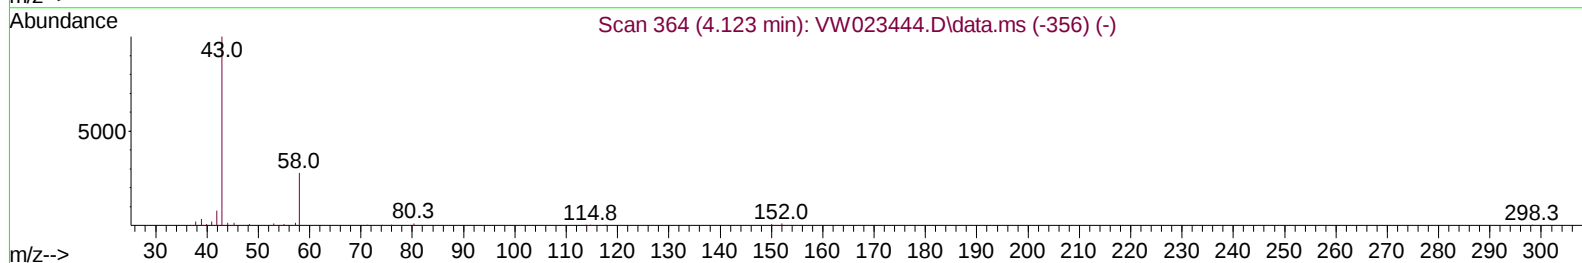
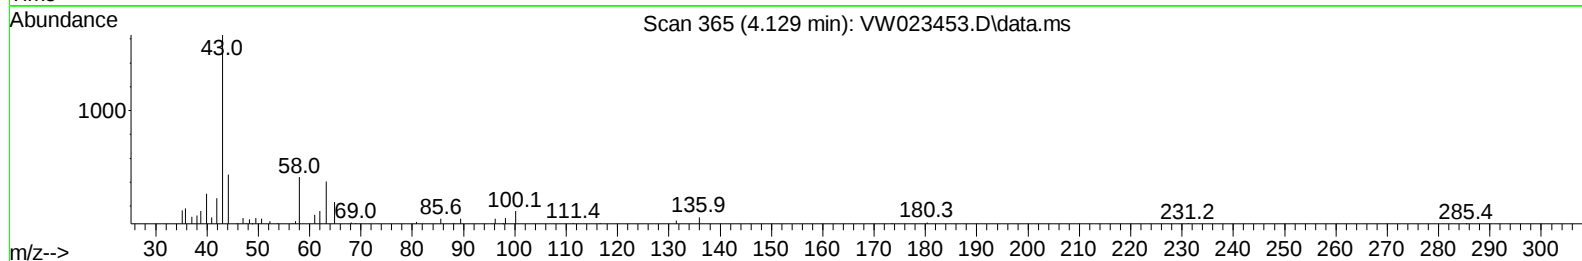


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061022\
Data File : VW023453.D
Acq On : 10 Jun 2022 17:53
Operator : SY/VA
Sample : N3226-15
Misc : 5.34g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 00:10:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jun 11 00:06:08 2022
Response via : Initial Calibration

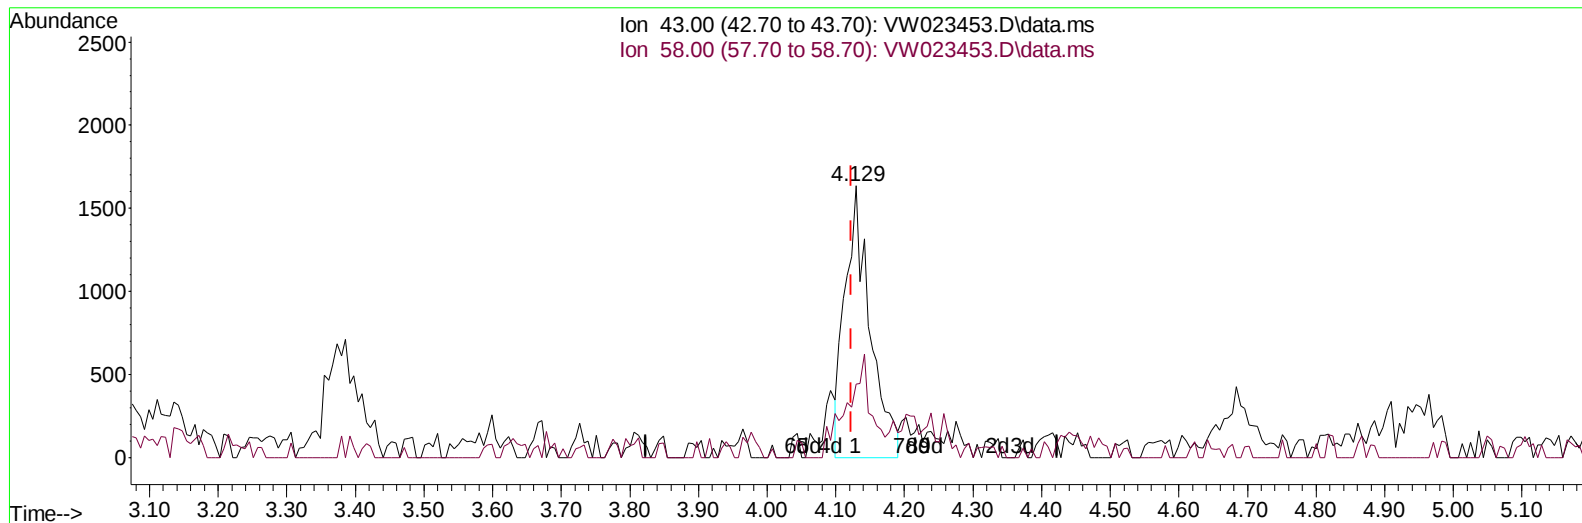

TIC: VW023453.D\data.ms

(13) Acetone (T)




4.129min (+ 0.006) 7.01 ug/L

response 4121

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	30.16
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061022\
Data File : VW023453.D
Acq On : 10 Jun 2022 17:53
Operator : SY/VA
Sample : N3226-15
Misc : 5.34g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 00:10:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jun 11 00:06:08 2022
Response via : Initial Calibration

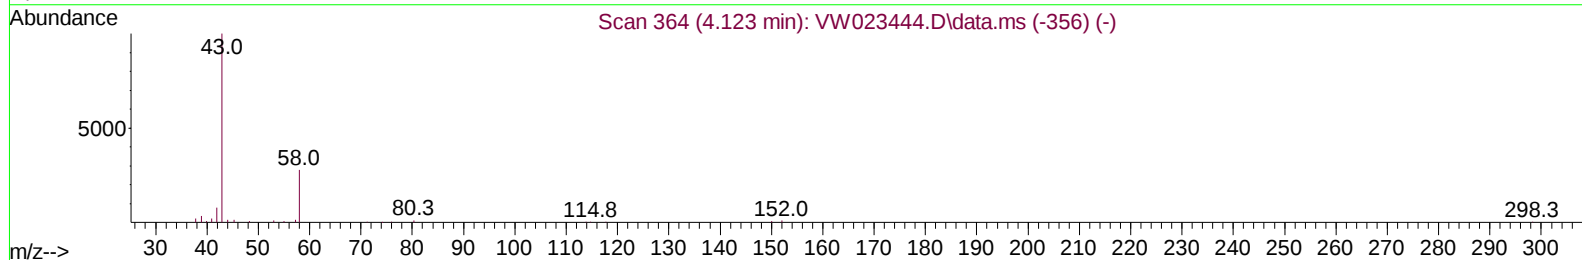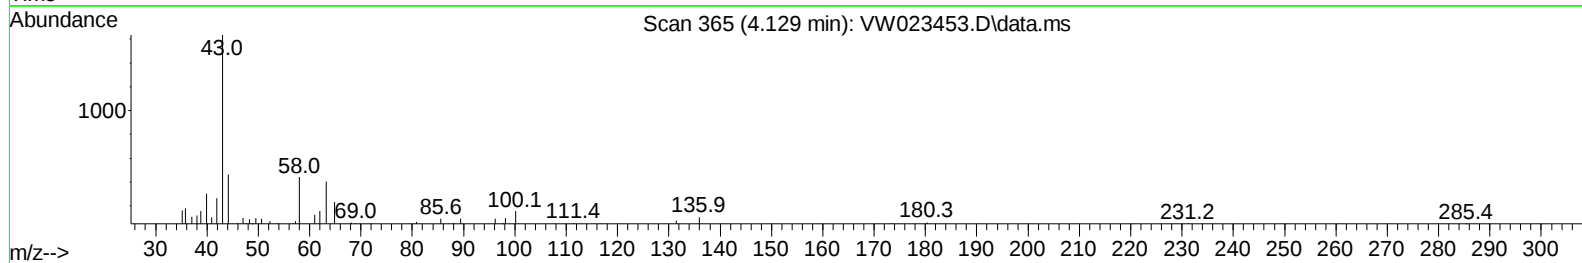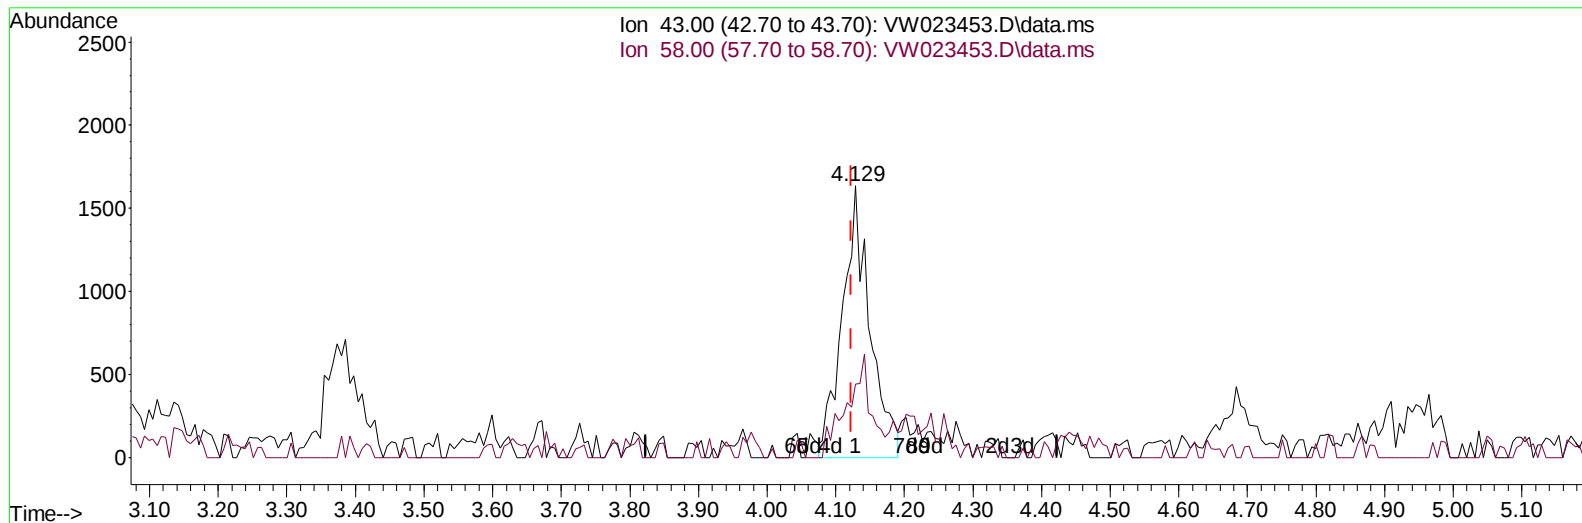

TIC: VW023453.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 7.73 ug/L m

response 4548

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	27.33
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061022\
 Data File : VW023453.D
 Acq On : 10 Jun 2022 17:53
 Operator : SY/VA
 Sample : N3226-15
 Misc : 5.34g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 00:10:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jun 11 00:06:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	251598	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	189805	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	51003	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	116646	29.183	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 116.720%			
7) Chloroethane-d5	2.886	69	89261	30.379	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 121.520%			
11) 1,1-Dichloroethene-d2	4.019	63	97165	17.415	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 69.680%			
21) 2-Butanone-d5	7.080	46	32761	40.143	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 80.280%			
24) Chloroform-d	7.647	84	190700	27.534	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 110.120%			
26) 1,2-Dichloroethane-d4	8.305	65	113426	30.408	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 121.640%			
32) Benzene-d6	8.275	84	310372	30.840	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 123.360%			
36) 1,2-Dichloropropane-d6	9.275	67	106938	36.067	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 144.280%#			
41) Toluene-d8	10.323	98	247553	25.184	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 100.720%			
43) trans-1,3-Dichloroprop...	10.579	79	26441	19.538	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 78.160%			
47) 2-Hexanone-d5	10.921	63	16704	35.256	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 70.520%			
56) 1,1,2,2-Tetrachloroeth...	12.689	84	92035	33.234	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 132.920%#			
66) 1,2-Dichlorobenzene-d4	13.853	152	51522	27.983	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 111.920%			
Target Compounds						
13) Acetone	4.129	43	4548m	7.735	ug/L	
29) Cyclohexane	7.952	56	3599	0.941	ug/L #	79

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061022\
Data File : VW023453.D
Acq On : 10 Jun 2022 17:53
Operator : SY/VA
Sample : N3226-15
Misc : 5.34g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 00:10:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jun 11 00:06:08 2022
Response via : Initial Calibration

