
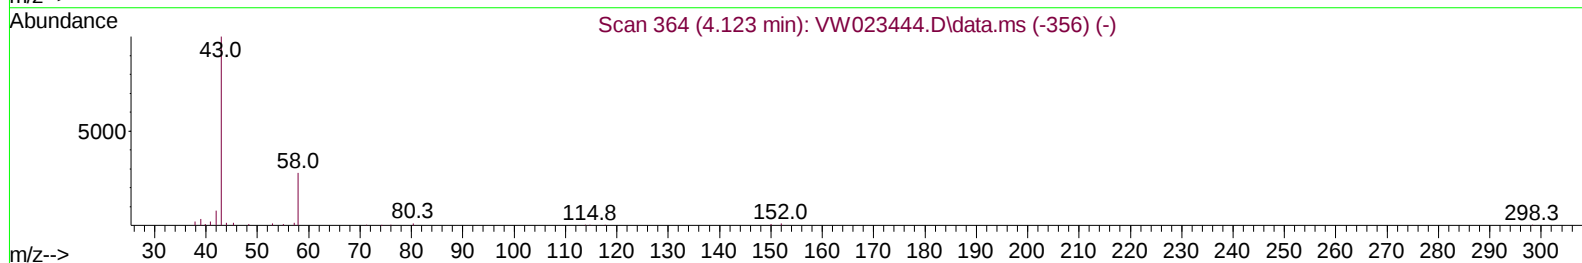
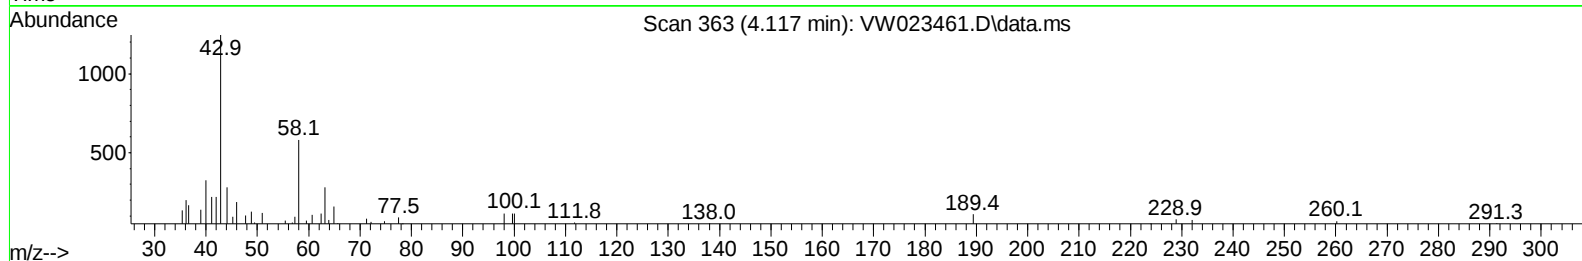


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061022\
 Data File : VW023461.D
 Acq On : 10 Jun 2022 21:06
 Operator : SY/VA
 Sample : N3292-03
 Misc : 7.17g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 00:12:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jun 11 00:06:08 2022
 Response via : Initial Calibration

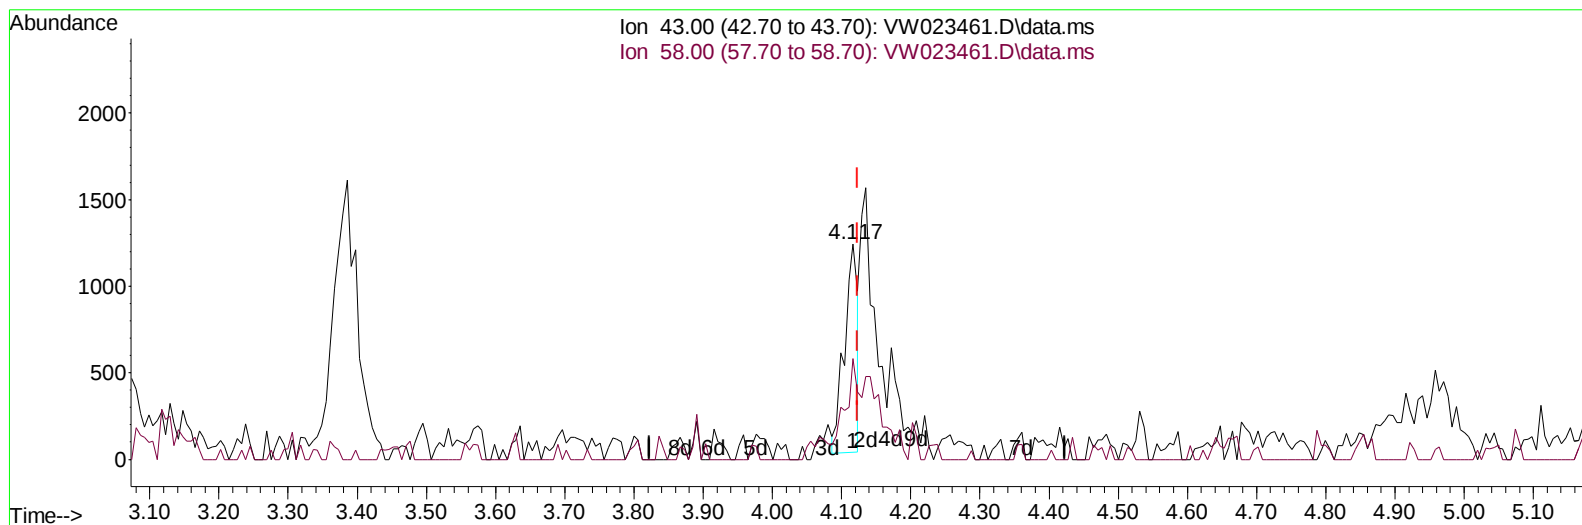




TIC: VW023461.D\data.ms

(13) Acetone (T)**4.117min (-0.006) 3.69 ug/L****response 1603**

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	37.12
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061022\
Data File : VW023461.D
Acq On : 10 Jun 2022 21:06
Operator : SY/VA
Sample : N3292-03
Misc : 7.17g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 00:12:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jun 11 00:06:08 2022
Response via : Initial Calibration

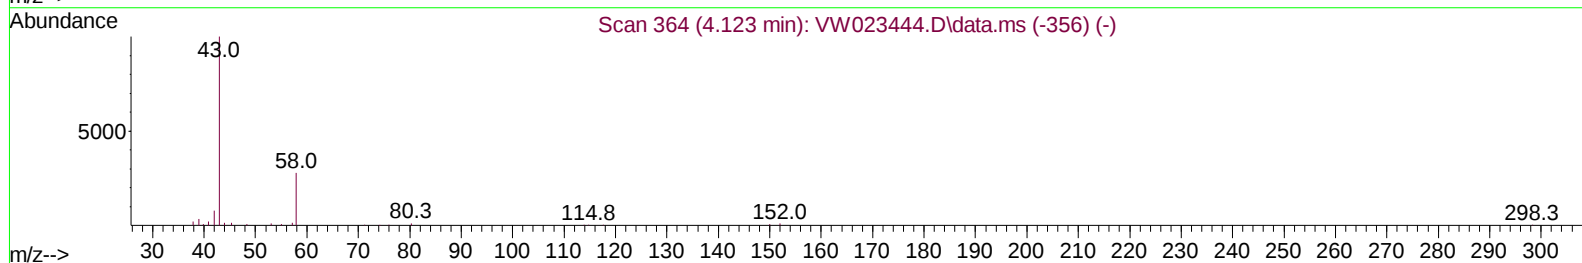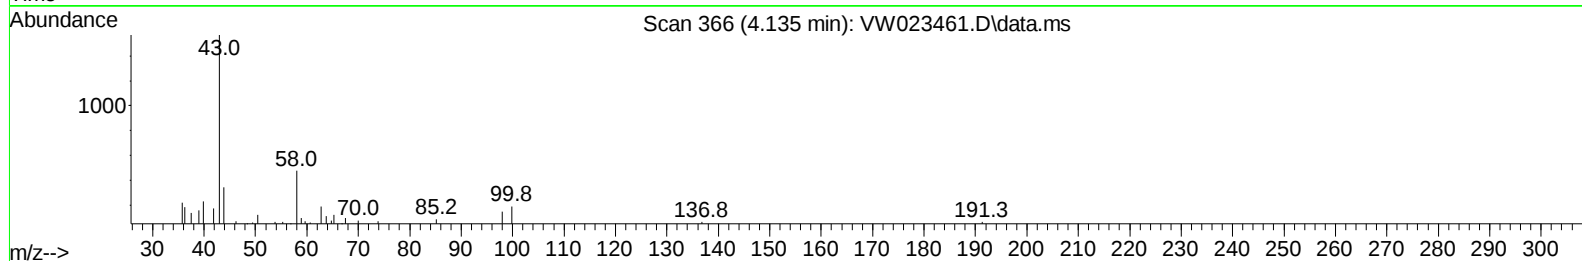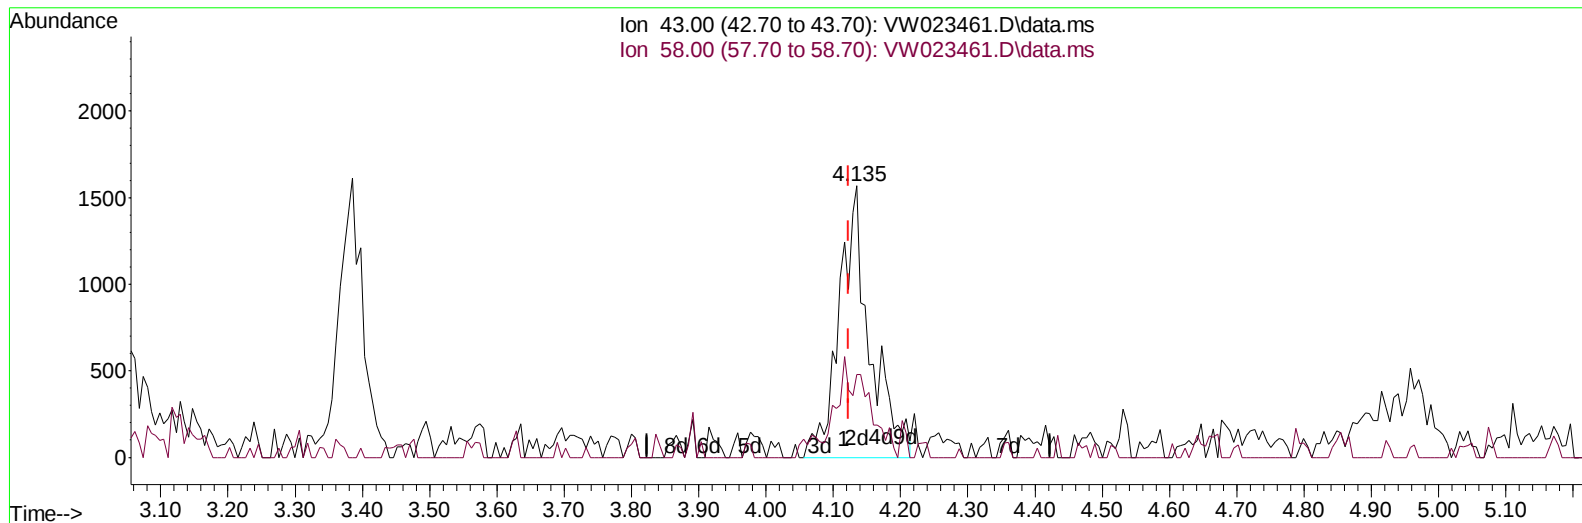

TIC: VW023461.D\data.ms

(13) Acetone (T)

4.135min (+ 0.012) 11.51 ug/L m

response 4996

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	11.91
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061022\
 Data File : VW023461.D
 Acq On : 10 Jun 2022 21:06
 Operator : SY/VA
 Sample : N3292-03
 Misc : 7.17g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 00:12:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jun 11 00:06:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	185663	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	113773	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	19979	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	99733	33.812	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	135.240%	
7) Chloroethane-d5	2.885	69	75852	34.983	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	139.920%	
11) 1,1-Dichloroethene-d2	4.013	63	78609	19.093	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110	Recovery	=	76.360%	
21) 2-Butanone-d5	7.074	46	50973	84.639	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	169.280%#	
24) Chloroform-d	7.647	84	161776	31.653	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	126.600%	
26) 1,2-Dichloroethane-d4	8.305	65	93875	34.104	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	136.400%#	
32) Benzene-d6	8.275	84	266146	44.118	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	176.480%#	
36) 1,2-Dichloropropane-d6	9.274	67	85650	48.191	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	192.760%#	
41) Toluene-d8	10.323	98	168394	28.579	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	114.320%	
43) trans-1,3-Dichloroprop...	10.579	79	22063	27.198	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	108.800%	
47) 2-Hexanone-d5	10.926	63	25040	88.170	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	176.340%#	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	60354	36.359	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	145.440%#	
66) 1,2-Dichlorobenzene-d4	13.847	152	23182	32.142	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	128.560%#	
Target Compounds						
					Qvalue	
13) Acetone	4.135	43	4996m	11.514	ug/L	
16) Methylene chloride	4.921	84	9638	3.836	ug/L	90
29) Cyclohexane	7.951	56	3574	1.560	ug/L #	50
42) Toluene	10.390	91	7761	1.057	ug/L	98
53) m,p-Xylene	11.829	106	2018	0.621	ug/L	89
63) 1,2,4-Trimethylbenzene	13.255	105	1097	0.469	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061022\
Data File : VW023461.D
Acq On : 10 Jun 2022 21:06
Operator : SY/VA
Sample : N3292-03
Misc : 7.17g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 00:12:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jun 11 00:06:08 2022
Response via : Initial Calibration

