
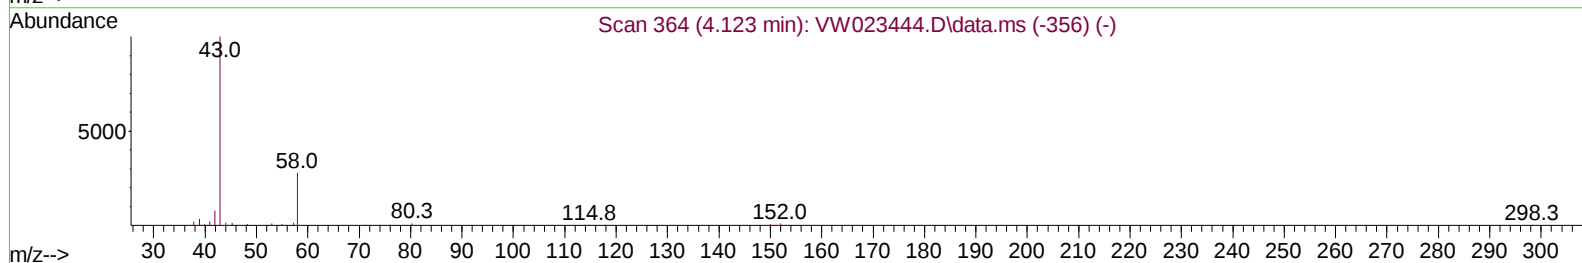
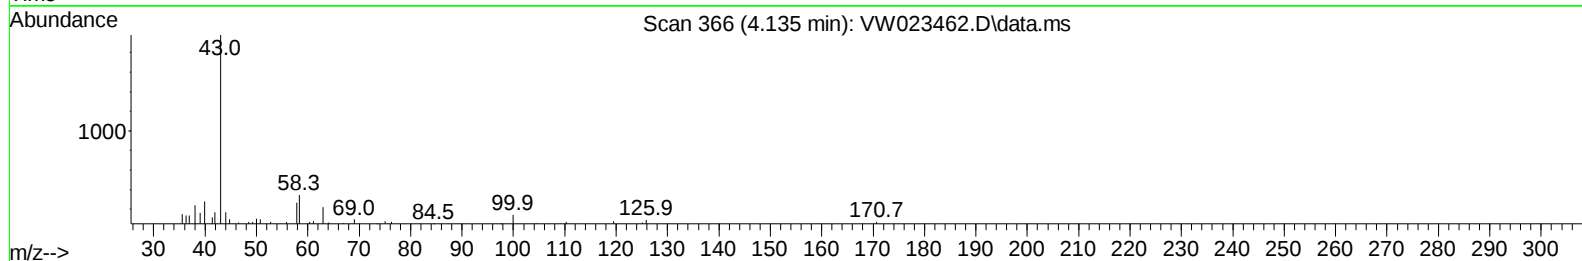


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061022\
Data File : VW023462.D
Acq On : 10 Jun 2022 21:30
Operator : SY/VA
Sample : N3256-07
Misc : 7.37g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 00:12:14 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jun 11 00:06:08 2022
Response via : Initial Calibration

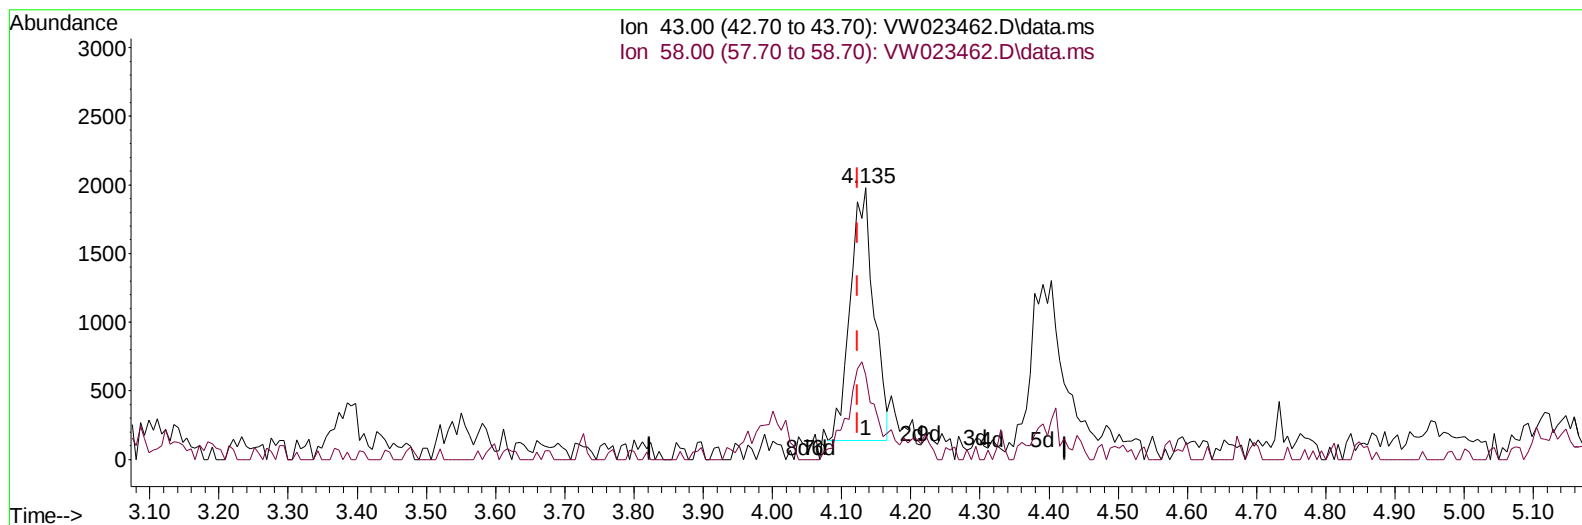

TIC: VW023462.D\data.ms

(13) Acetone (T)




4.135min (+ 0.012) 5.91 ug/L

response 4336

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	42.16
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061022\
 Data File : VW023462.D
 Acq On : 10 Jun 2022 21:30
 Operator : SY/VA
 Sample : N3256-07
 Misc : 7.37g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 00:12:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jun 11 00:06:08 2022
 Response via : Initial Calibration

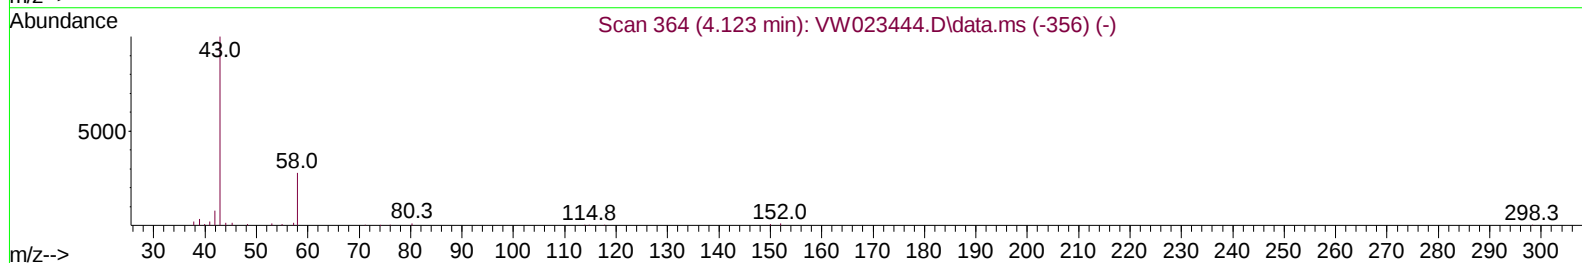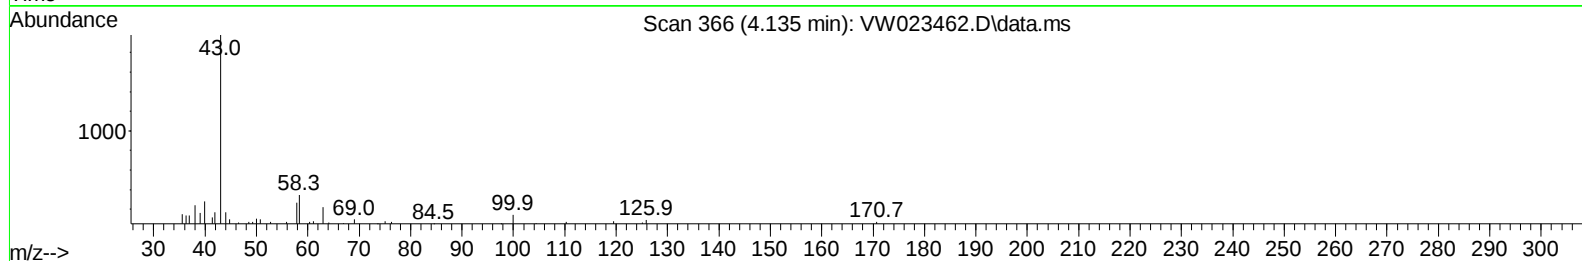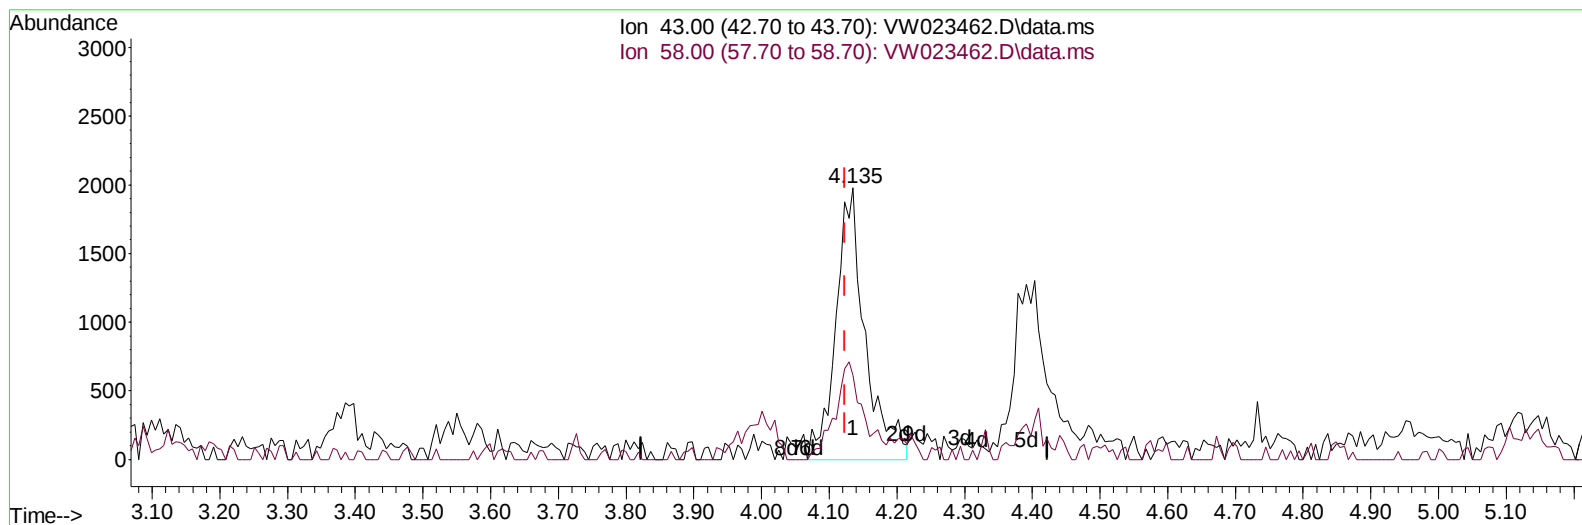

TIC: VW023462.D\data.ms

(13) Acetone (T)

4.135min (+ 0.012) 8.04 ug/L m

response 5900

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	30.98
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061022\
 Data File : VW023462.D
 Acq On : 10 Jun 2022 21:30
 Operator : SY/VA
 Sample : N3256-07
 Misc : 7.37g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 00:12:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jun 11 00:06:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	313852	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	307334	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	133872	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	96745	19.403	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	77.600%	
7) Chloroethane-d5	2.879	69	65209	17.791	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	71.160%	
11) 1,1-Dichloroethene-d2	4.019	63	90854	13.054	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	52.200%	
21) 2-Butanone-d5	7.080	46	45348	44.544	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	89.080%	
24) Chloroform-d	7.647	84	171229	19.819	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	79.280%	
26) 1,2-Dichloroethane-d4	8.305	65	97657	20.988	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	83.960%	
32) Benzene-d6	8.275	84	309685	19.004	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	76.000%	
36) 1,2-Dichloropropane-d6	9.274	67	99649	20.756	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	83.040%	
41) Toluene-d8	10.323	98	281148	17.664	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	70.640%	
43) trans-1,3-Dichloroprop...	10.579	79	37337	17.039	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	68.160%	
47) 2-Hexanone-d5	10.927	63	31113	40.556	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	81.120%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	86071	19.195	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	76.800%	
66) 1,2-Dichlorobenzene-d4	13.853	152	97632	20.202	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	80.800%	
Target Compounds						
13) Acetone	4.135	43	5900m	8.044	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061022\
Data File : VW023462.D
Acq On : 10 Jun 2022 21:30
Operator : SY/VA
Sample : N3256-07
Misc : 7.37g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 00:12:14 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jun 11 00:06:08 2022
Response via : Initial Calibration

