

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061022\
 Data File : VW023457.D
 Acq On : 10 Jun 2022 19:30
 Operator : SY/VA
 Sample : N3226-19
 Misc : 5.78g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4N9

Quant Time: Jun 11 00:11:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jun 11 00:06:08 2022
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		8.842	114	282777	25.000	ug/L	0.00
28) Chlorobenzene-d5		11.628	117	207537	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		13.554	152	49890	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		2.349	65	134140	29.859	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	119.440%	
7) Chloroethane-d5		2.879	69	98601	29.858	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	119.440%	
11) 1,1-Dichloroethene-d2		4.013	63	109614	17.480	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	69.920%	
21) 2-Butanone-d5		7.080	46	29958	32.661	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	65.320%	
24) Chloroform-d		7.647	84	224502	28.841	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	115.360%	
26) 1,2-Dichloroethane-d4		8.305	65	131601	31.391	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	125.560%	
32) Benzene-d6		8.275	84	364786	33.150	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	132.600%	
36) 1,2-Dichloropropane-d6		9.275	67	129484	39.939	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	159.760%#	
41) Toluene-d8		10.323	98	286984	26.700	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	106.800%	
43) trans-1,3-Dichloroprop...		10.579	79	26263	17.748	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	71.000%	
47) 2-Hexanone-d5		10.921	63	15033	29.019	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	58.040%	
56) 1,1,2,2-Tetrachloroeth...		12.689	84	97772	32.289	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	129.160%#	
66) 1,2-Dichlorobenzene-d4		13.853	152	54383	30.196	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	120.800%#	
Target Compounds							
13) Acetone		4.123	43	3461	5.237	ug/L	Qvalue 67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061022\
Data File : VW023457.D
Acq On : 10 Jun 2022 19:30
Operator : SY/VA
Sample : N3226-19
Misc : 5.78g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW4N9

Quant Time: Jun 11 00:11:14 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jun 11 00:06:08 2022
Response via : Initial Calibration

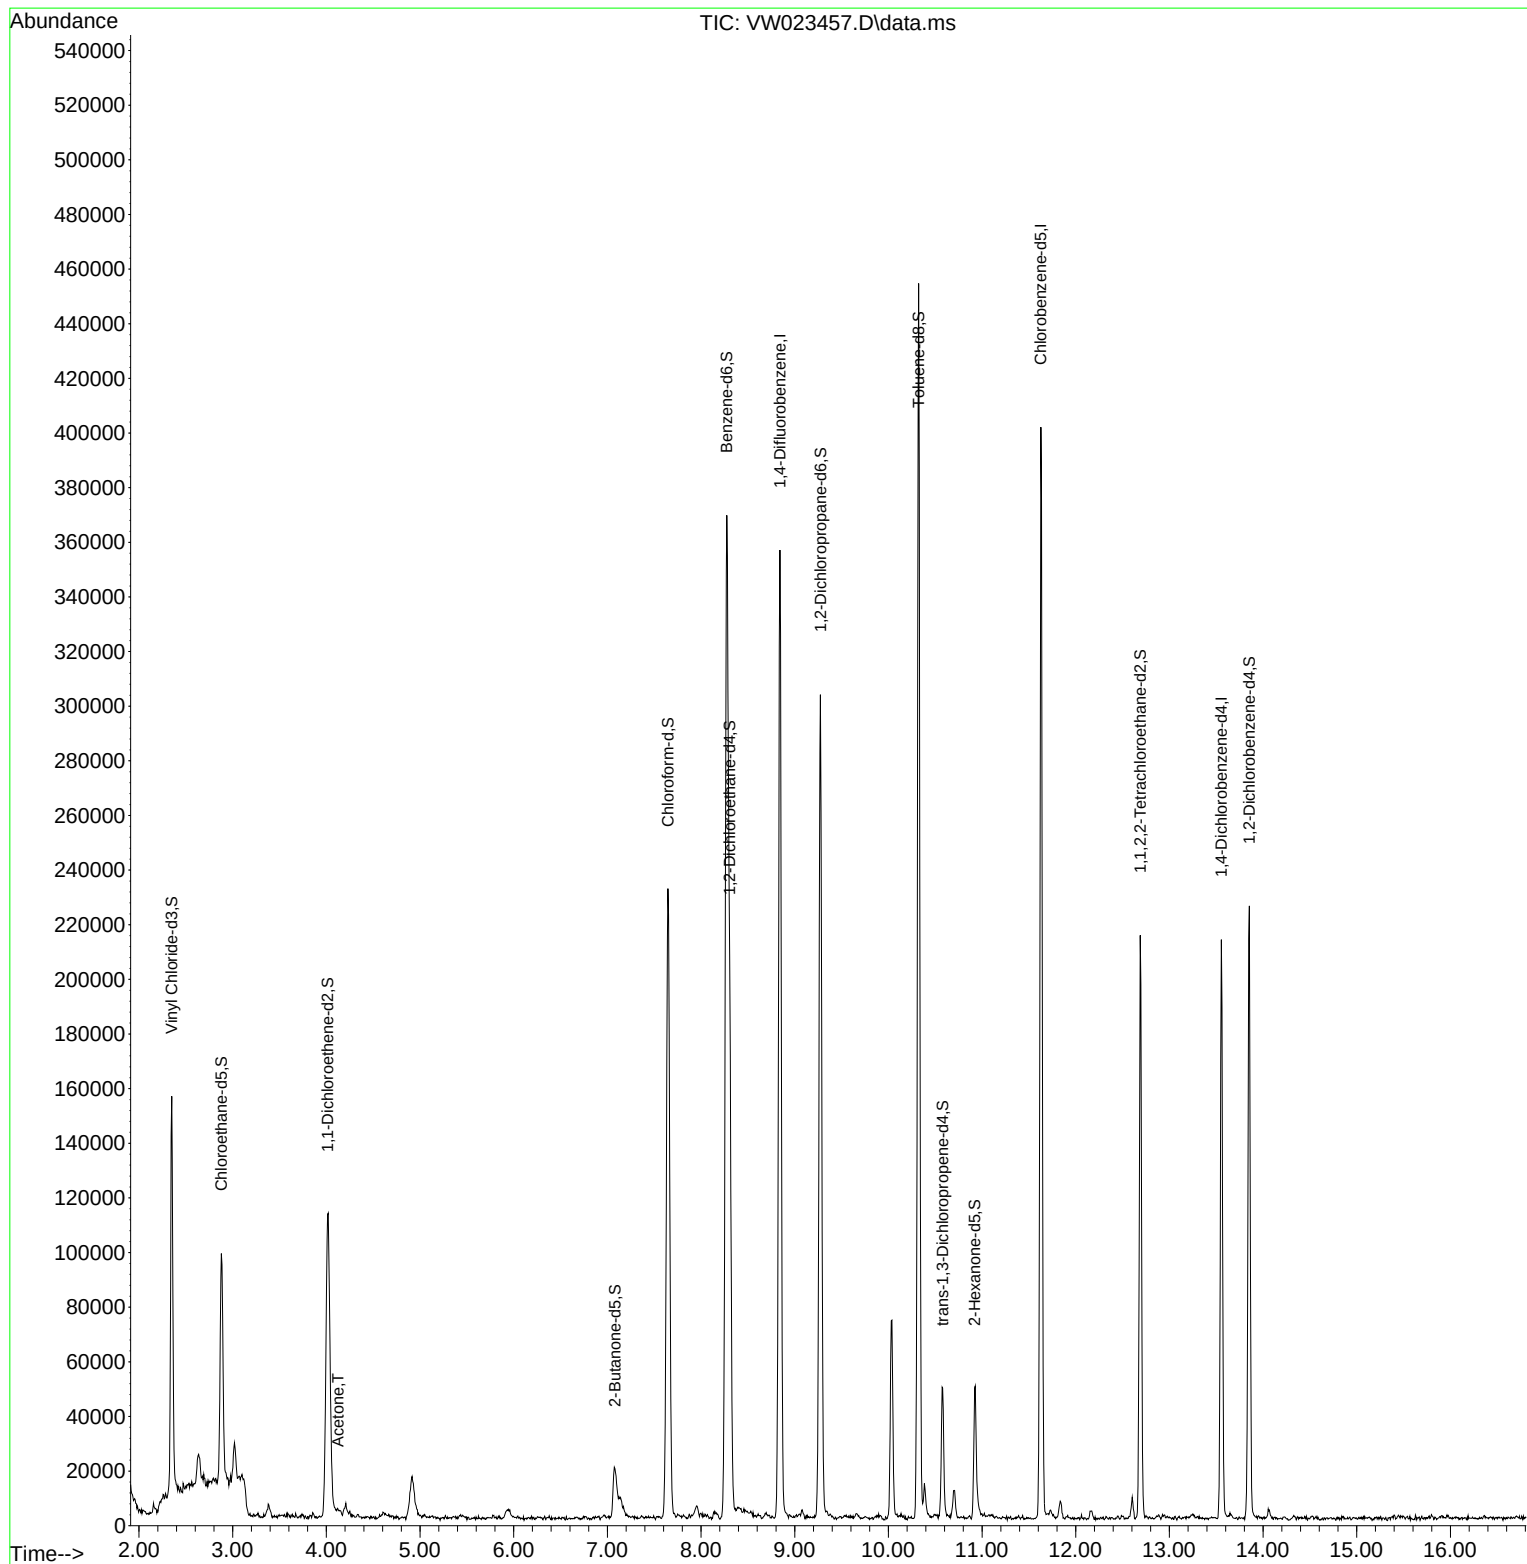

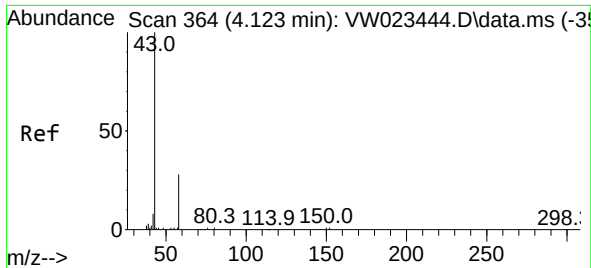

#13
 Acetone
 Concen: 5.237 ug/L
 RT: 4.123 min Scan# 30
 Delta R.T. 0.000 min
 Lab File: VW023457.D
 Acq: 10 Jun 2022 19:30

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4N9

Tgt Ion: 43 Resp: 3461
 Ion Ratio Lower Upper
 43 100
 58 13.4 0.0 64.0

