

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061022\
 Data File : VW023459.D
 Acq On : 10 Jun 2022 20:18
 Operator : SY/VA
 Sample : N3292-01
 Misc : 6.47g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4P2

Quant Time: Jun 11 00:11:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jun 11 00:06:08 2022
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		8.842	114	250112	25.000	ug/L	0.00
28) Chlorobenzene-d5		11.634	117	177009	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		13.560	152	45853	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		2.349	65	120583	30.347	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	121.400%	
7) Chloroethane-d5		2.885	69	85885	29.404	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	117.600%	
11) 1,1-Dichloroethene-d2		4.019	63	98188	17.703	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	70.800%	
21) 2-Butanone-d5		7.086	46	13105	16.153	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	32.300%	
24) Chloroform-d		7.653	84	190976	27.738	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	110.960%	
26) 1,2-Dichloroethane-d4		8.305	65	113698	30.662	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	122.640%	
32) Benzene-d6		8.275	84	324143	34.537	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	138.160%#	
36) 1,2-Dichloropropane-d6		9.274	67	107185	38.763	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	155.040%#	
41) Toluene-d8		10.323	98	237096	25.863	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	103.440%	
43) trans-1,3-Dichloroprop...		10.579	79	24595	19.488	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	77.960%	
47) 2-Hexanone-d5		10.927	63	2203	4.986	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	9.980%#	
56) 1,1,2,2-Tetrachloroeth...		12.688	84	85096	32.950	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	131.800%#	
66) 1,2-Dichlorobenzene-d4		13.853	152	47233	28.535	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	114.120%	
Target Compounds							
29) Cyclohexane		7.964	56	2121	0.595	ug/L	Qvalue # 38


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061022\
Data File : VW023459.D
Acq On : 10 Jun 2022 20:18
Operator : SY/VA
Sample : N3292-01
Misc : 6.47g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW4P2


Quant Time: Jun 11 00:11:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jun 11 00:06:08 2022
Response via : Initial Calibration

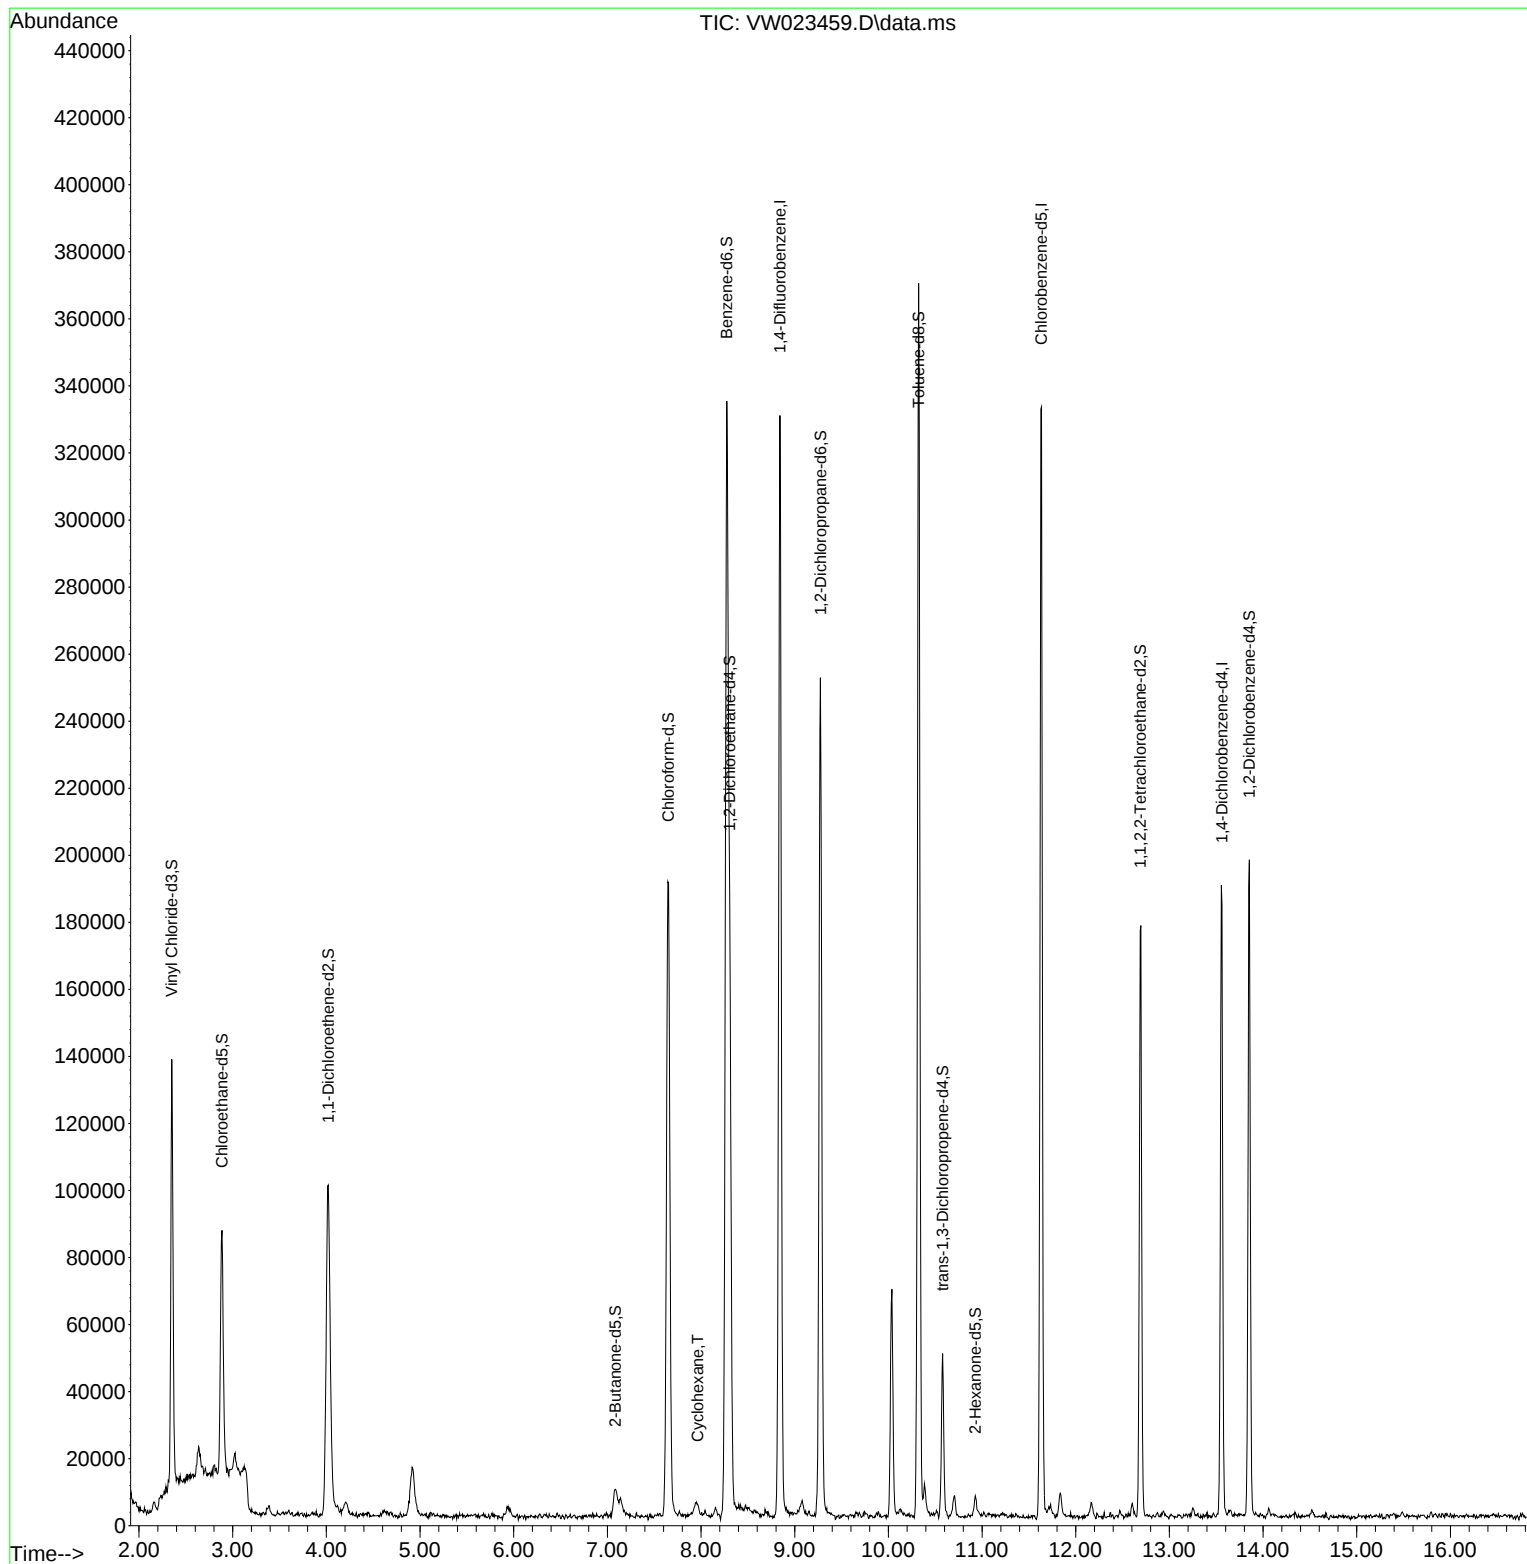

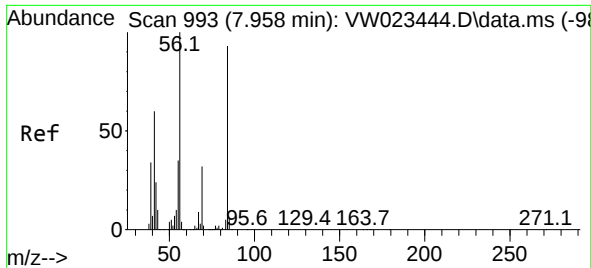

#29
Cyclohexane
Concen: 0.595 ug/L
RT: 7.964 min Scan# 994
Delta R.T. 0.006 min
Lab File: VW023459.D
Acq: 10 Jun 2022 20:18

Instrument :
MSVOA_W
ClientSampleId :
EW4P2

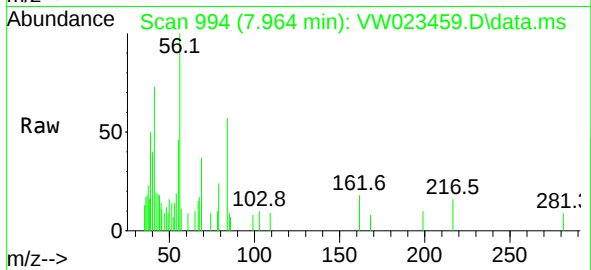

Tgt Ion:	56	Resp:	2121
Ion	Ratio	Lower	Upper
56	100		
69	20.7	25.6	38.4#
84	22.4	78.2	117.4#

