

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061124\
 Data File : VW029092.D
 Acq On : 11 Jun 2024 11:18
 Operator : SY/MD
 Sample : VW0611SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Jun 12 00:21:07 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 12 00:20:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	296641	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	286318	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	133395	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	98451	20.891	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	83.560%		
7) Chloroethane-d5	2.899	69	79354	21.928	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	87.720%		
11) 1,1-Dichloroethene-d2	4.021	65	44545	21.506	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	86.040%		
21) 2-Butanone-d5	7.081	46	52818	54.856	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	109.720%		
24) Chloroform-d	7.648	84	195372	23.086	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	92.360%		
26) 1,2-Dichloroethane-d4	8.307	65	110385	24.775	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	99.120%		
32) Benzene-d6	8.276	84	390644	22.229	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	88.920%		
36) 1,2-Dichloropropane-d6	9.270	67	124703	23.404	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	93.600%		
41) Toluene-d8	10.325	98	340073	21.685	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	86.760%		
43) trans-1,3-Dichloroprop...	10.575	79	44994	21.976	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	87.920%		
47) 2-Hexanone-d5	10.922	63	35586	50.611	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	101.220%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	91697	24.773	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	99.080%		
66) 1,2-Dichlorobenzene-d4	13.848	152	114431	24.174	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	96.680%		
Target Compounds				Qvalue		
39) cis-1,3-Dichloropropene	10.032	75	3630	0.536	ug/L #	61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061124\
Data File : VW029092.D
Acq On : 11 Jun 2024 11:18
Operator : SY/MD
Sample : VW0611SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Jun 12 00:21:07 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 12 00:20:38 2024
Response via : Initial Calibration

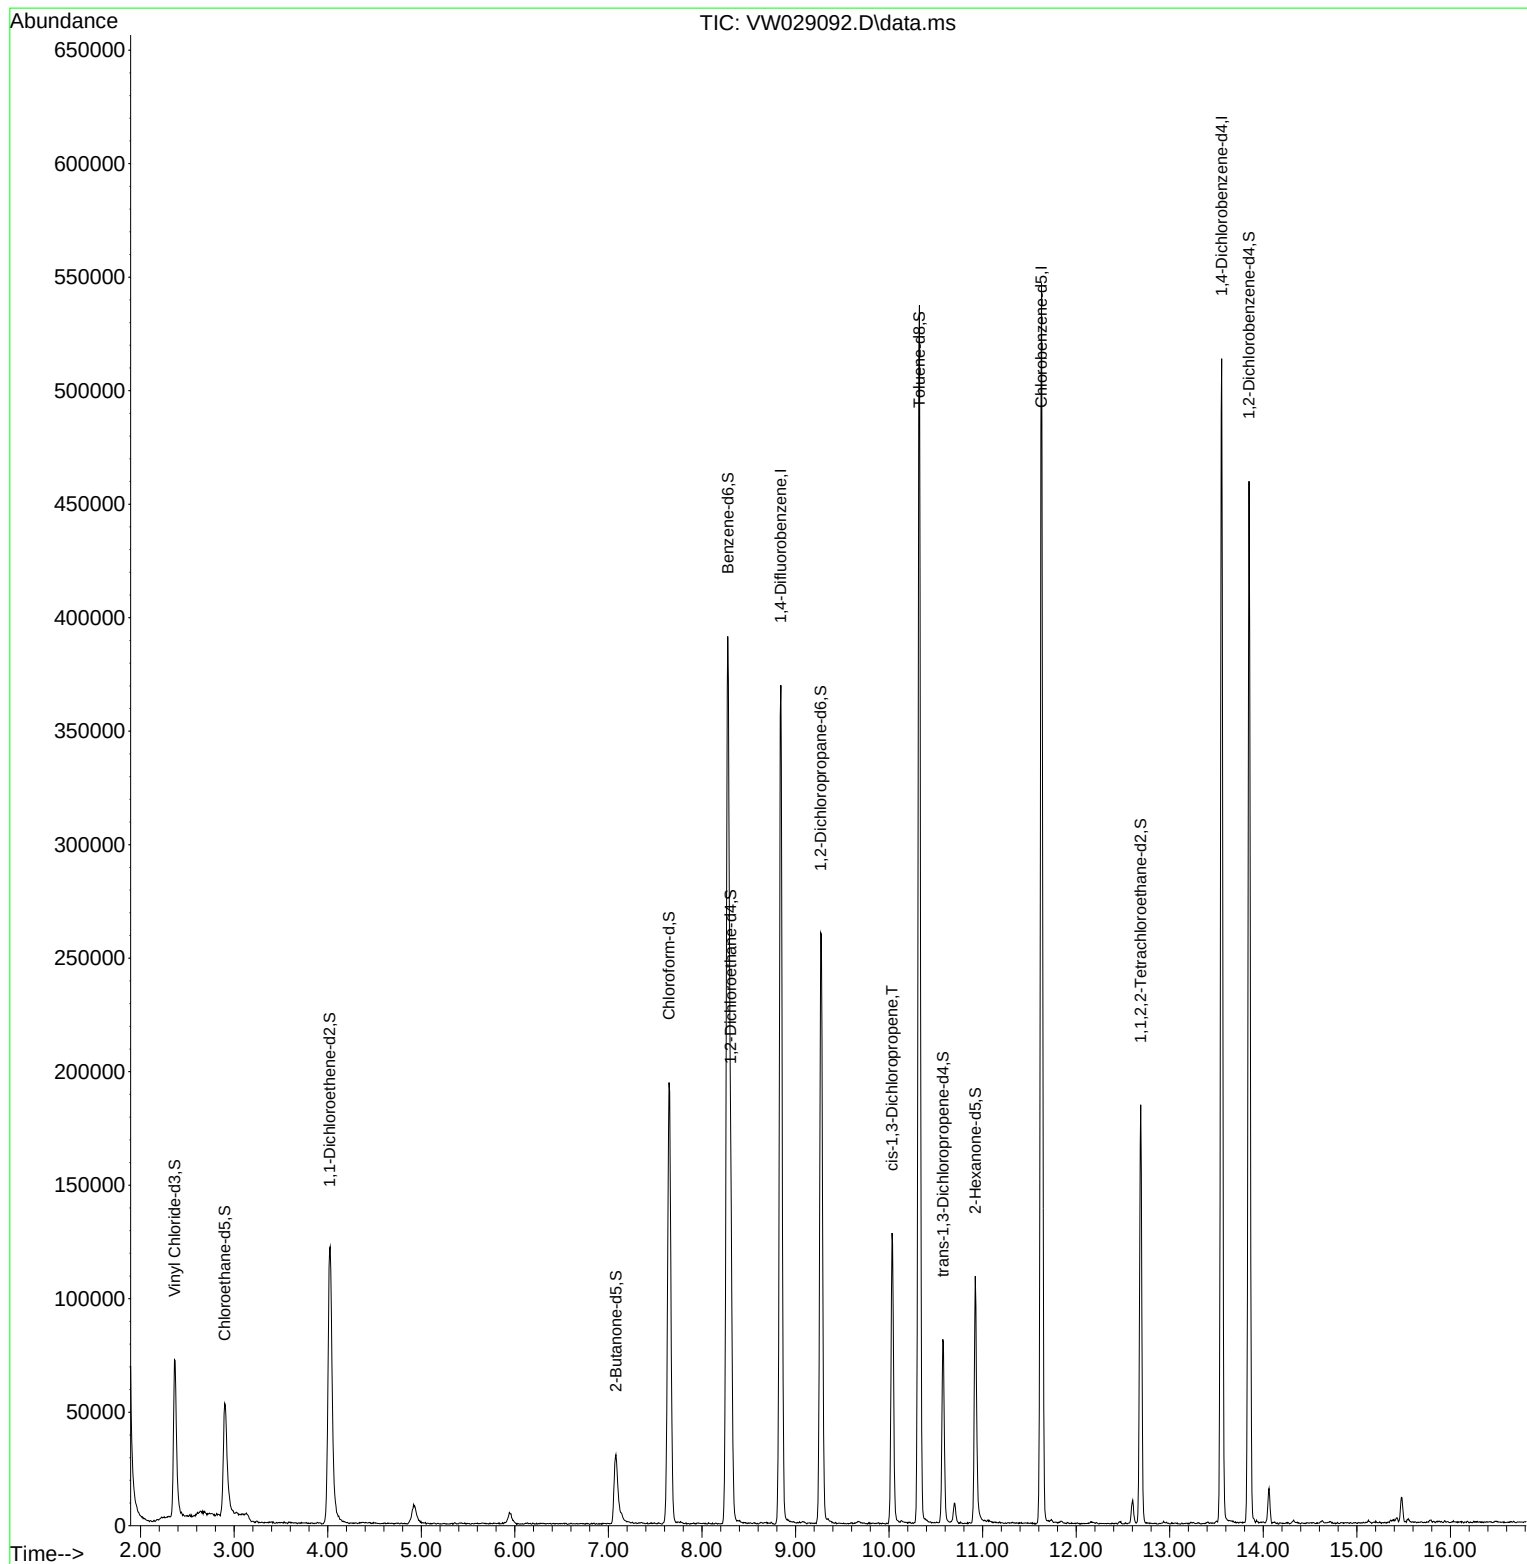

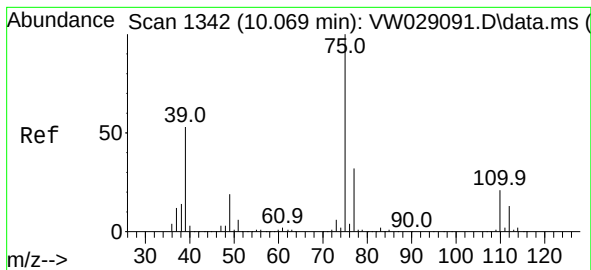

#39
cis-1,3-Dichloropropene
Concen: 0.536 ug/L
RT: 10.032 min Scan# 14
Delta R.T. -0.037 min
Lab File: VW029092.D
Acq: 11 Jun 2024 11:18

Instrument :
MSVOA_W
ClientSampleId :

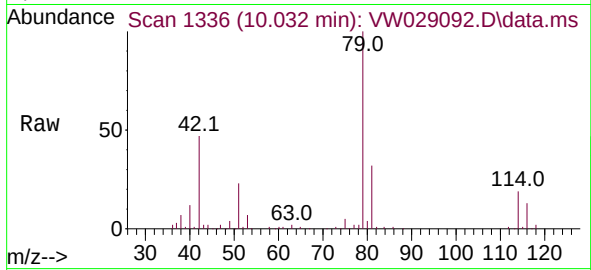

Tgt Ion: 75 Resp: 3630
Ion Ratio Lower Upper
75 100
77 51.2 21.0 39.0#

