

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061124\
 Data File : VW029093.D
 Acq On : 11 Jun 2024 11:42
 Operator : SY/MD
 Sample : P2696-18
 Misc : 5.01g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Jun 12 00:21:22 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 12 00:20:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	310157	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	295348	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	129010	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	98669	20.025	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.120%
7) Chloroethane-d5	2.899	69	80203	21.197	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.800%
11) 1,1-Dichloroethene-d2	4.021	65	45546	21.031	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	84.120%
21) 2-Butanone-d5	7.075	46	57892	57.506	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	115.020%
24) Chloroform-d	7.648	84	204211	23.079	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.320%
26) 1,2-Dichloroethane-d4	8.301	65	115368	24.765	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	99.080%
32) Benzene-d6	8.276	84	404896	22.336	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	89.360%
36) 1,2-Dichloropropane-d6	9.270	67	131330	23.894	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.560%
41) Toluene-d8	10.325	98	355576	21.981	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	87.920%
43) trans-1,3-Dichloroprop...	10.575	79	47706	22.588	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	90.360%
47) 2-Hexanone-d5	10.922	63	38848	53.561	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	107.120%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	100552	26.334	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	105.320%
66) 1,2-Dichlorobenzene-d4	13.849	152	116679	25.487	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	101.960%
Target Compounds				Qvalue		
39) cis-1,3-Dichloropropene	10.032	75	3528	0.505	ug/L #	67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061124\
Data File : VW029093.D
Acq On : 11 Jun 2024 11:42
Operator : SY/MD
Sample : P2696-18
Misc : 5.01g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Jun 12 00:21:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 12 00:20:38 2024
Response via : Initial Calibration

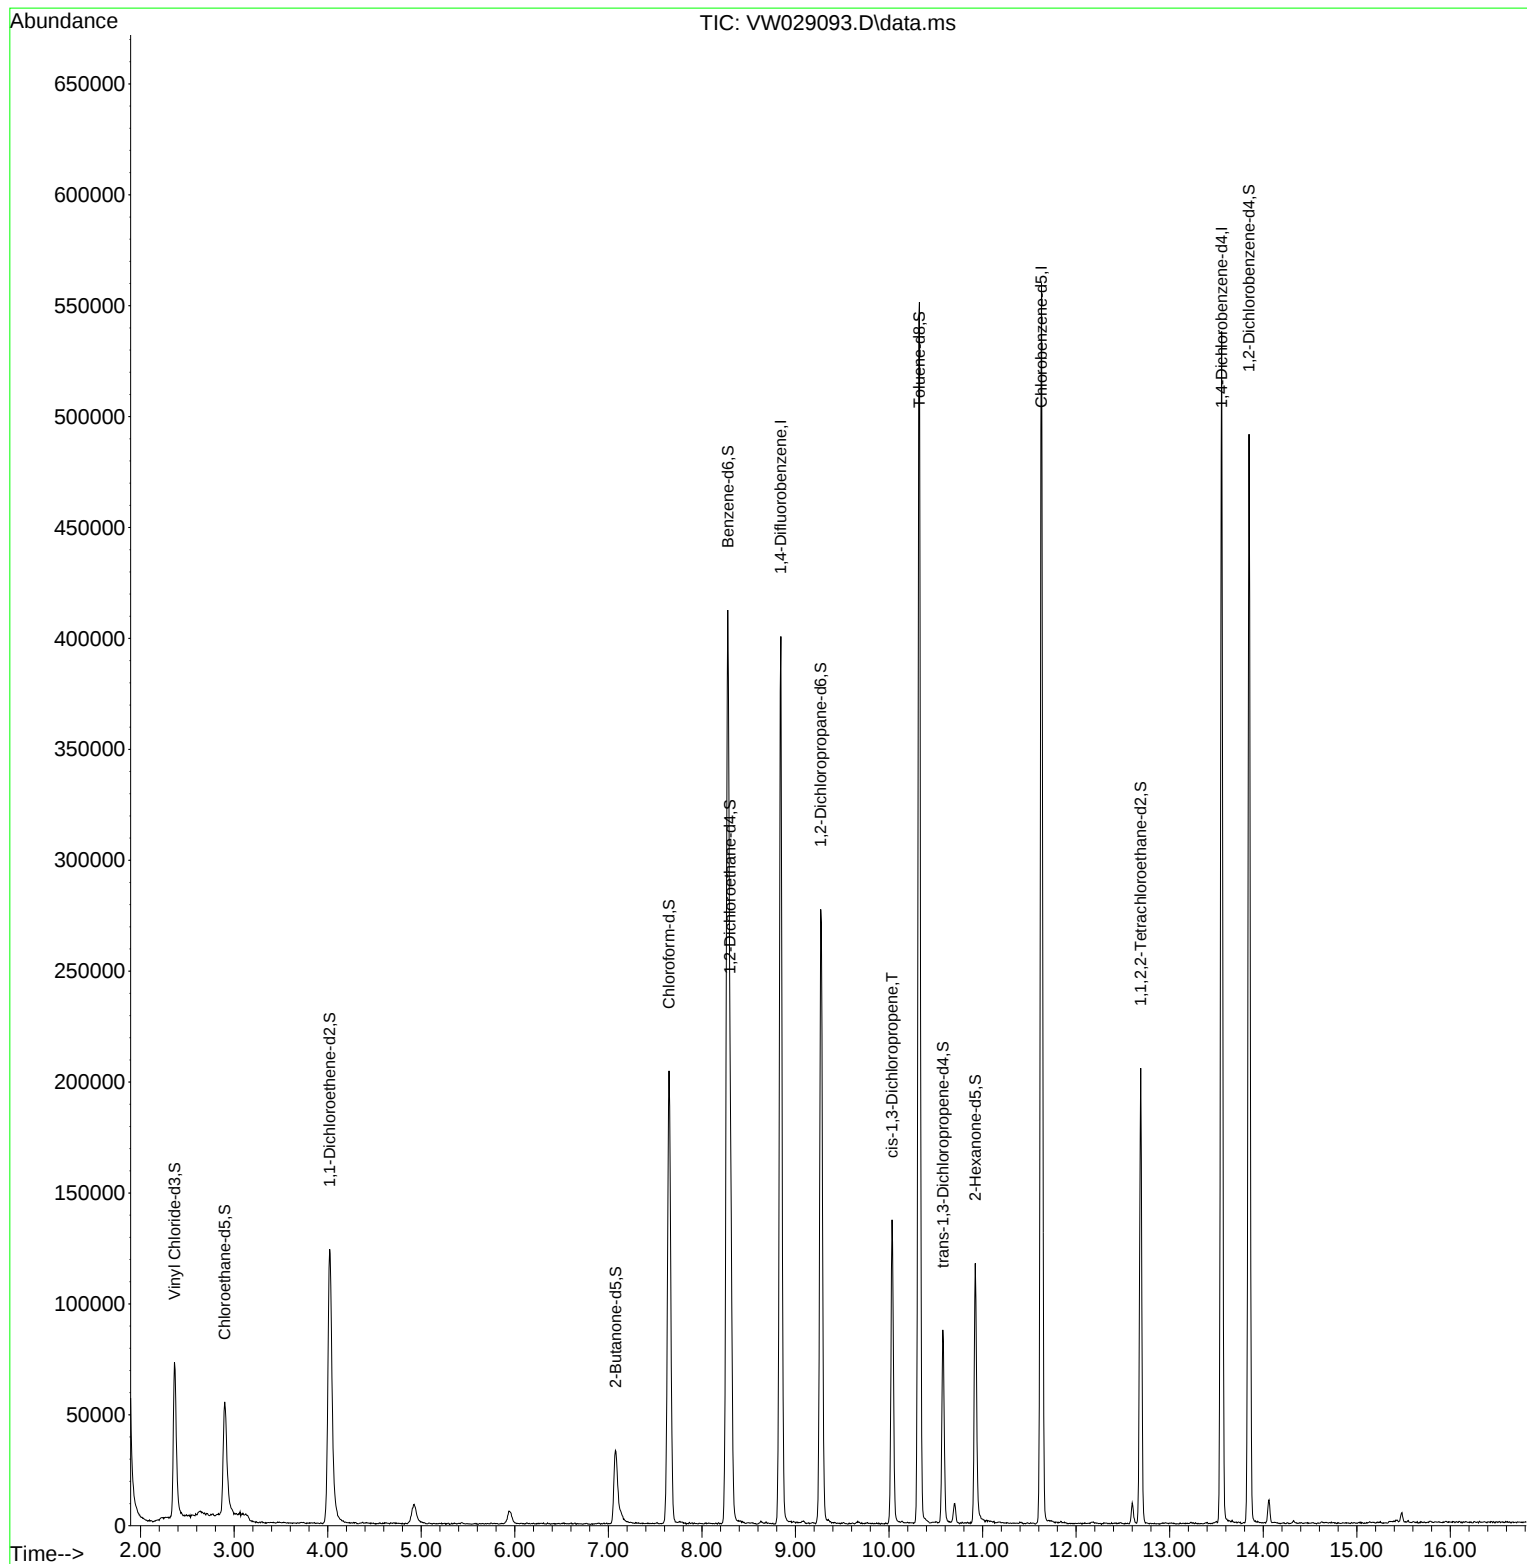

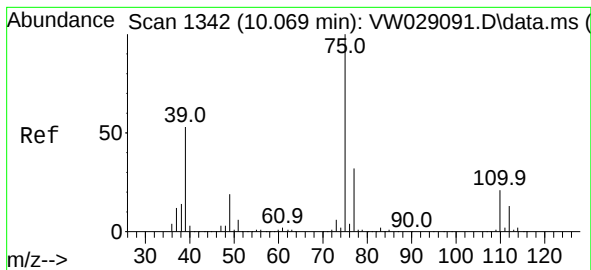

#39
 cis-1,3-Dichloropropene
 Concen: 0.505 ug/L
 RT: 10.032 min Scan# 14
 Delta R.T. -0.036 min
 Lab File: VW029093.D
 Acq: 11 Jun 2024 11:42

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 3528
 Ion Ratio Lower Upper
 75 100
 77 47.8 21.0 39.0#

