

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061124\
 Data File : VW029095.D
 Acq On : 11 Jun 2024 12:48
 Operator : SY/MD
 Sample : P2776-04
 Misc : 5.03g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Jun 12 00:21:50 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 12 00:20:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	294684	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	275395	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	120191	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	103590	22.128	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.520%
7) Chloroethane-d5	2.905	69	83557	23.243	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	92.960%
11) 1,1-Dichloroethene-d2	4.021	65	46329	22.516	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	90.080%
21) 2-Butanone-d5	7.075	46	41620	43.513	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.020%
24) Chloroform-d	7.648	84	199973	23.786	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.160%
26) 1,2-Dichloroethane-d4	8.307	65	104550	23.622	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	94.480%
32) Benzene-d6	8.276	84	404765	23.946	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	95.800%
36) 1,2-Dichloropropane-d6	9.270	67	123278	24.054	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	96.200%
41) Toluene-d8	10.325	98	349062	23.141	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	92.560%
43) trans-1,3-Dichloroprop...	10.575	79	41632	21.140	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	84.560%
47) 2-Hexanone-d5	10.922	63	27747	41.027	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	82.060%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	78407	22.022	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	88.080%
66) 1,2-Dichlorobenzene-d4	13.849	152	108783	25.505	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	102.040%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	3322	0.510	ug/L	# 69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061124\
Data File : VW029095.D
Acq On : 11 Jun 2024 12:48
Operator : SY/MD
Sample : P2776-04
Misc : 5.03g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Jun 12 00:21:50 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 12 00:20:38 2024
Response via : Initial Calibration

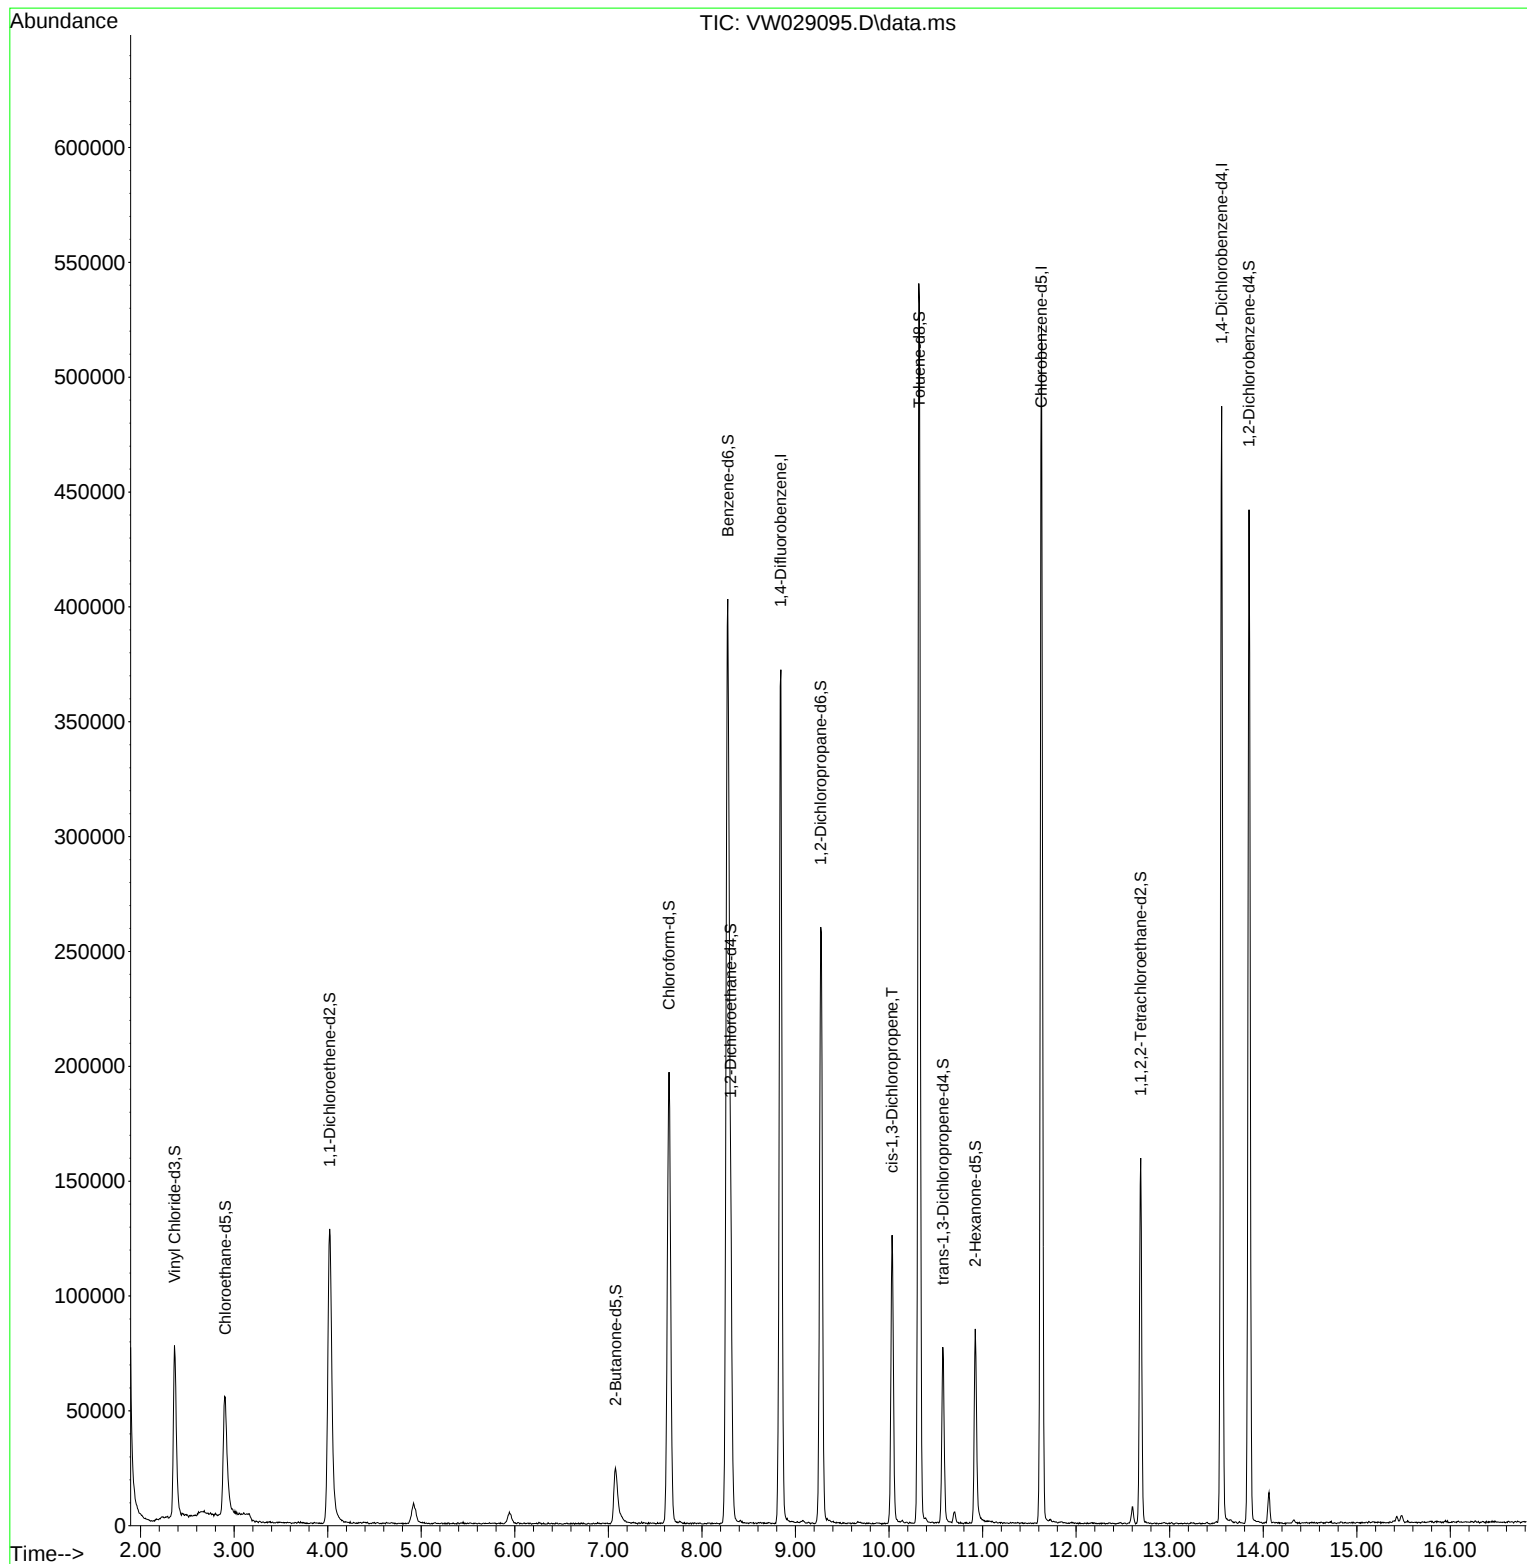

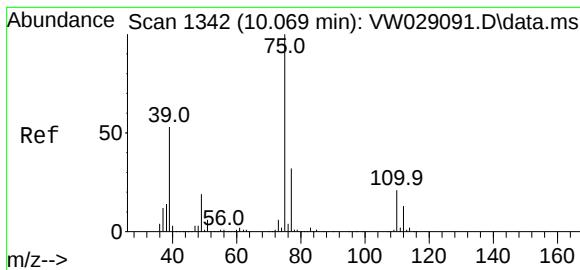

#39
 cis-1,3-Dichloropropene
 Concen: 0.510 ug/L
 RT: 10.032 min Scan# 14
 Delta R.T. -0.036 min
 Lab File: VW029095.D
 Acq: 11 Jun 2024 12:48

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 3322
 Ion Ratio Lower Upper
 75 100
 77 46.8 21.0 39.0#

