
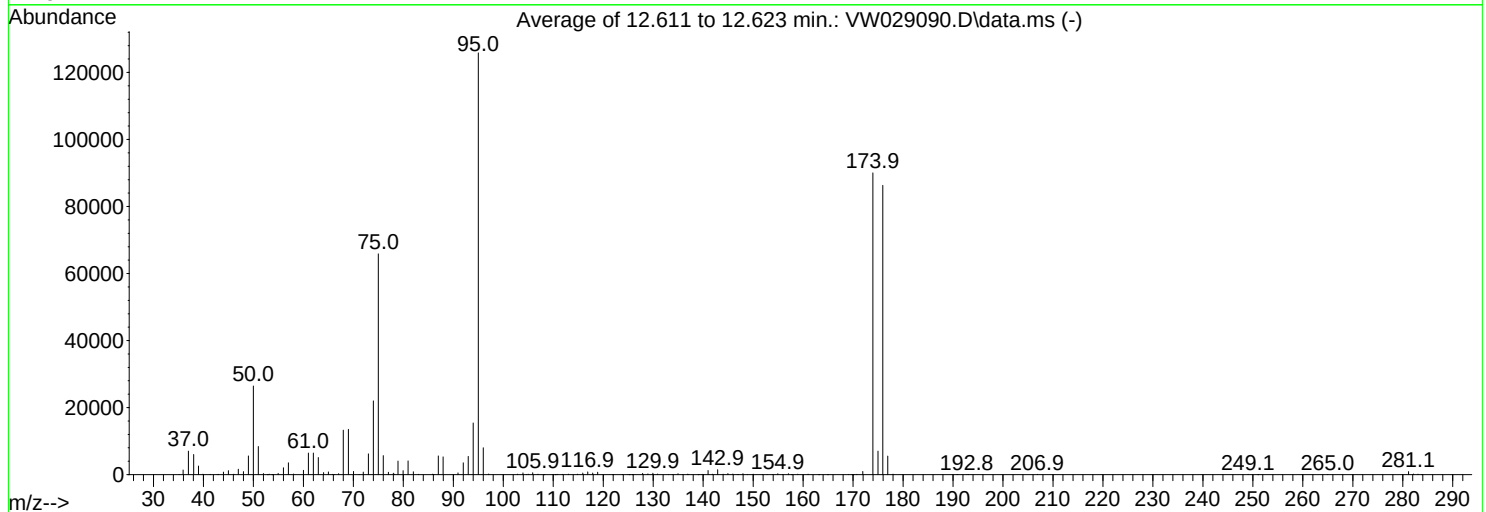


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061124\
Data File : VW029090.D
Acq On : 11 Jun 2024 09:21
Operator : SY/MD
Sample : BFB503
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB503

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
Title : SFAM01.0
Last Update : Wed Jun 12 00:20:38 2024

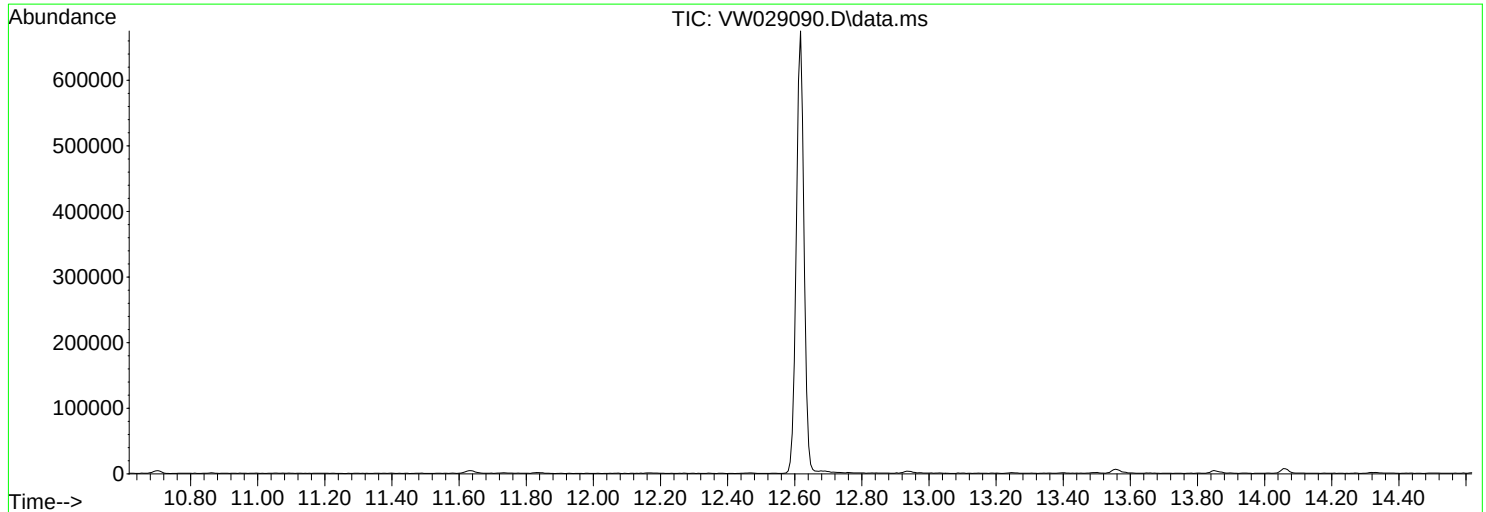

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.0	26427	PASS
75	95	30	80	52.3	65872	PASS
95	95	100	100	100.0	125845	PASS
96	95	5	9	6.4	8042	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	71.5	90024	PASS
175	174	5	9	7.8	7017	PASS
176	174	95	101	95.8	86288	PASS
177	176	5	9	6.4	5540	PASS

m/z	Abundance
35.90	66.0
36.40	64.0
39.90	231.0
43.90	196.0
46.40	50.0
46.70	51.0
50.70	72.0
67.10	53.0

Instrument :
MSVOA_W
ClientSampleId :
BFB503

m/z	Abundance
35.20	59.0
36.00	1527.0
37.00	7384.0
38.00	6404.0
39.00	2731.0
39.90	433.0
41.40	64.0
43.10	153.0
44.00	978.0
45.00	1153.0
46.10	179.0
47.00	1701.0
48.00	958.0
49.00	5873.0
50.00	27640.0
51.00	8584.0
52.00	324.0
53.10	173.0
54.00	71.0
55.00	440.0
56.00	2170.0
57.00	4011.0
58.10	211.0
60.00	1575.0
61.00	6523.0
62.00	6625.0
63.00	5806.0
64.10	848.0
65.00	993.0
65.80	125.0
67.00	279.0
68.00	14131.0
69.00	13830.0
70.10	978.0
71.10	83.0
72.00	733.0
73.00	6551.0
74.00	22560.0
75.00	66928.0
76.00	5971.0
77.00	851.0
78.00	610.0
79.00	4183.0
80.00	1145.0
80.90	4298.0
82.00	864.0
83.10	124.0
85.90	269.0
87.00	5747.0
88.00	5424.0
90.90	561.0
92.00	3514.0
93.00	5264.0
94.00	14985.0
95.00	121208.0
96.00	7809.0
97.20	192.0
102.80	204.0
103.90	531.0
104.70	207.0
106.00	496.0
107.00	123.0
109.90	125.0
110.40	61.0
111.00	91.0
111.90	85.0
113.00	196.0
114.80	153.0
115.90	493.0
116.90	740.0
117.90	419.0
118.90	728.0
123.90	56.0
125.00	90.0
125.80	54.0
128.00	350.0
129.00	253.0
129.90	323.0
130.80	151.0
133.00	144.0
134.00	51.0
134.90	259.0
136.00	60.0
136.80	247.0
139.90	132.0
141.00	1247.0
141.90	207.0
142.90	1535.0
144.00	117.0
145.00	456.0
146.00	134.0
147.10	106.0

Instrument :
MSVOA_W
ClientSampleId :
BFB503

148.00	251.0
148.80	73.0
150.10	120.0
151.90	68.0
152.80	60.0
154.00	54.0
155.00	293.0
157.00	295.0
158.90	126.0
161.00	145.0
163.10	61.0
164.90	76.0
169.10	63.0
169.80	90.0
170.70	142.0
172.00	1043.0
174.00	82336.0
175.00	6531.0
176.00	82856.0
176.90	5356.0
177.90	154.0
190.80	114.0
192.80	152.0
206.90	108.0
249.10	108.0
251.00	82.0
265.00	158.0
281.10	1451.0
282.10	303.0
283.10	317.0
283.80	53.0

Instrument :
MSVOA_W
ClientSampleId :
BFB503

m/z	Abundance
35.10	51.0
36.00	1654.0
37.00	7980.0
38.00	6931.0
39.00	2937.0
40.00	400.0
41.30	123.0
42.80	143.0
44.10	941.0
45.00	1398.0
46.10	217.0
47.00	1938.0
48.00	812.0
49.00	6082.0
50.00	29592.0
51.00	9573.0
52.00	383.0
53.20	144.0
53.90	86.0
54.90	363.0
56.00	2299.0
57.00	3737.0
58.10	167.0
60.00	1299.0
61.00	6978.0
62.00	7506.0
63.00	5404.0
64.00	624.0
65.00	824.0
65.90	149.0
67.10	412.0
68.00	14832.0
69.00	15570.0
70.00	1212.0
71.20	96.0
72.00	916.0
73.00	6820.0
74.00	24984.0
75.00	74264.0
76.00	6481.0
77.00	672.0
78.00	652.0
79.00	4526.0
80.00	1346.0
81.00	4515.0
82.00	906.0
82.90	80.0
86.10	262.0
87.00	6143.0
88.00	5722.0
91.00	529.0
92.00	3983.0
93.00	6406.0
94.00	18120.0
95.00	147200.0
96.00	9627.0
97.00	238.0
102.90	90.0
104.00	580.0
105.00	214.0
105.90	728.0
106.90	178.0
110.00	126.0
110.90	158.0
111.80	104.0
113.00	121.0
114.90	194.0
115.90	557.0
116.90	855.0
117.90	484.0
118.90	836.0
123.80	83.0
124.90	113.0
126.00	62.0
127.90	545.0
128.90	228.0
129.90	484.0
130.90	194.0
133.10	53.0
133.90	67.0
135.00	315.0
136.00	92.0
137.10	282.0
139.00	68.0
139.70	95.0
140.10	121.0
141.00	1367.0
141.80	169.0
142.90	1586.0
143.90	165.0
144.90	371.0
145.90	219.0

Instrument :
MSVOA_W
ClientSampleId :
BFB503

146.80	85.0
148.00	368.0
148.90	91.0
150.00	163.0
152.80	107.0
153.90	62.0
155.00	324.0
155.90	68.0
157.10	344.0
157.70	71.0
159.00	124.0
161.00	184.0
169.00	56.0
170.80	157.0
171.90	1069.0
173.90	96184.0
175.00	8004.0
175.90	90520.0
177.00	6351.0
178.00	172.0
191.00	131.0
193.10	136.0
206.90	59.0
249.10	80.0
265.00	80.0
281.20	789.0
282.20	158.0
283.00	116.0

Instrument :
MSVOA_W
ClientSampleId :
BFB503

m/z	Abundance
35.20	57.0
36.00	1133.0
37.00	5705.0
38.10	4754.0
39.00	2098.0
40.00	274.0
41.30	102.0
43.00	87.0
44.10	936.0
45.00	1033.0
46.00	124.0
47.00	1312.0
48.00	893.0
49.00	4884.0
50.00	22048.0
51.00	7041.0
52.00	353.0
52.80	67.0
53.20	66.0
53.70	81.0
55.00	377.0
56.00	1628.0
57.00	2826.0
57.90	149.0
60.00	1020.0
61.00	5848.0
62.00	5171.0
63.00	4119.0
64.00	469.0
65.00	661.0
66.20	96.0
67.10	310.0
68.00	10941.0
69.00	11189.0
70.00	758.0
72.00	636.0
73.00	5208.0
74.00	18512.0
75.00	56424.0
76.00	4652.0
77.00	605.0
78.20	426.0
78.90	3410.0
79.90	1109.0
81.00	3516.0
82.00	839.0
83.10	125.0
85.80	190.0
87.00	4927.0
87.90	4792.0
90.90	459.0
92.00	3126.0
93.00	4683.0
94.00	13127.0
95.00	109128.0
96.00	6691.0
97.10	166.0
102.80	99.0
104.00	421.0
105.00	176.0
105.80	485.0
107.00	148.0
108.10	52.0
110.10	52.0
110.80	117.0
111.80	54.0
113.10	125.0
114.80	100.0
115.90	400.0
116.90	825.0
117.90	512.0
118.90	564.0
121.90	58.0
123.80	92.0
125.20	53.0
126.00	65.0
127.80	324.0
128.90	258.0
130.00	417.0
131.00	206.0
134.90	245.0
135.90	54.0
136.90	222.0
139.70	70.0
141.00	1185.0
141.80	136.0
142.90	1409.0
144.10	147.0
145.00	227.0
145.90	197.0
146.80	86.0
147.90	245.0

Instrument :
MSVOA_W
ClientSampleId :
BFB503

148.90	66.0
149.90	119.0
151.90	112.0
152.80	55.0
154.00	60.0
154.90	267.0
155.90	84.0
157.10	184.0
158.80	73.0
159.10	70.0
161.00	148.0
170.00	88.0
171.90	758.0
174.00	91552.0
175.00	6515.0
175.90	85488.0
177.00	4914.0
178.10	197.0
206.90	98.0
249.00	80.0
281.10	515.0
282.10	200.0

Instrument :
MSVOA_W
ClientSampleId :
BFB503