




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061224\
Data File : VW029105.D
Acq On : 12 Jun 2024 14:26
Operator : SY/MD
Sample : P2776-22
Misc : 5.36g/10mL/MSVOA_W/SOIL/A
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4C76

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/13/2024
Supervised By :Mahesh Dadoda 06/13/2024

Quant Time: Jun 13 00:50:15 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jun 13 00:47:39 2024
Response via : Initial Calibration

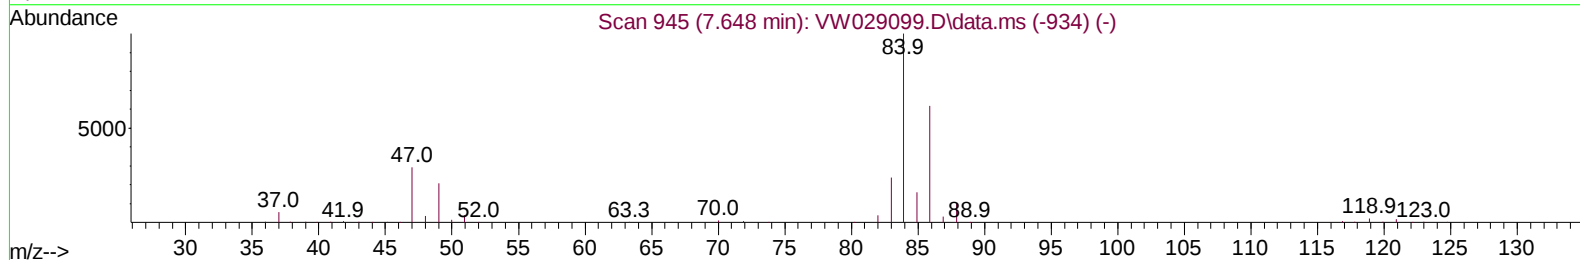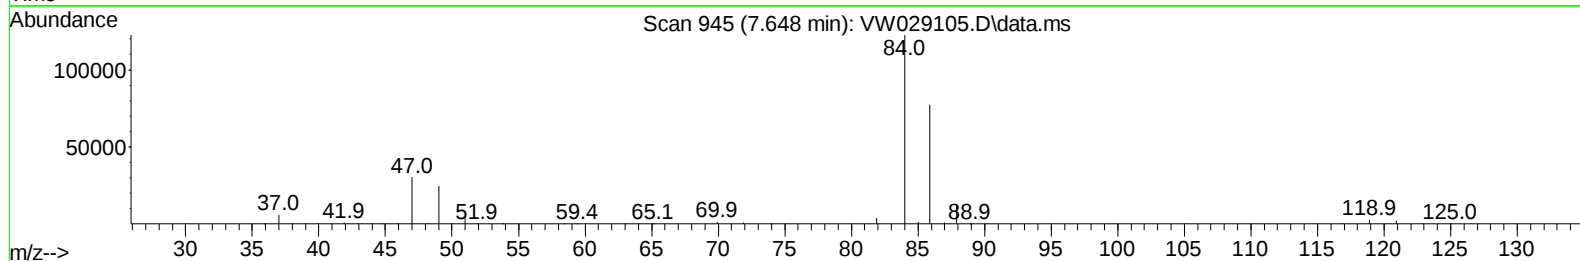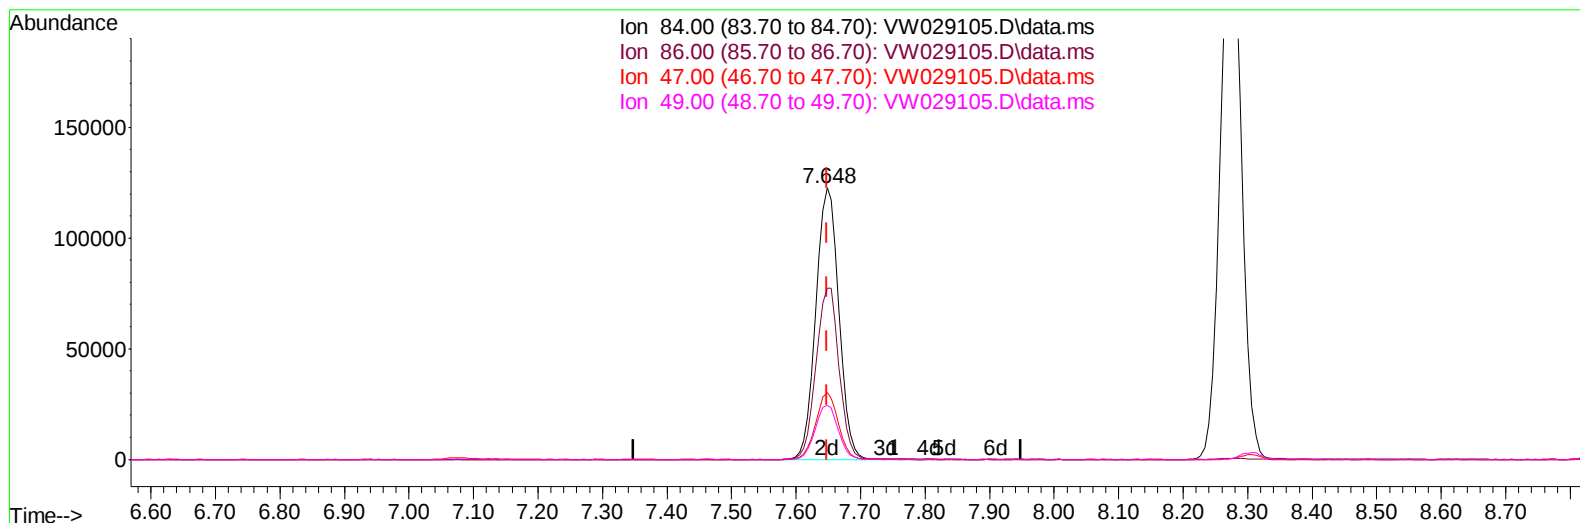

TIC: VW029105.D\data.ms

(24) Chloroform-d (S)

7.648min (-0.000) 23.41 ug/L m

response 303556

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	63.10	0.04#
47.00	46.00	0.02#
49.00	27.00	0.02#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061224\
 Data File : VW029105.D
 Acq On : 12 Jun 2024 14:26
 Operator : SY/MD
 Sample : P2776-22
 Misc : 5.36g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4C76

Manual IntegrationsAPPROVED

Quant Time: Jun 13 00:50:15 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 13 00:47:39 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/13/2024
 Supervised By :Mahesh Dadoda 06/13/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.837	114		454430	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		289313	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.555	152		59425	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.362	65		149777	20.747	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	83.000%		
7) Chloroethane-d5	2.899	69		125708	22.676	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	90.720%		
11) 1,1-Dichloroethene-d2	4.021	65		66709	21.024	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	84.080%		
21) 2-Butanone-d5	7.075	46		82825	56.153	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	112.300%		
24) Chloroform-d	7.648	84		303556m	23.414	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	93.640%		
26) 1,2-Dichloroethane-d4	8.306	65		174356	25.545	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	102.200%		
32) Benzene-d6	8.276	84		580956	32.717	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	130.880%		
36) 1,2-Dichloropropane-d6	9.270	67		187160	34.762	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	139.040%#		
41) Toluene-d8	10.318	98		421626	26.607	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	106.440%		
43) trans-1,3-Dichloroprop...	10.574	79		47303	22.865	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	91.440%		
47) 2-Hexanone-d5	10.922	63		34832	49.025	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	98.060%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		99827	26.690	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	106.760%		
66) 1,2-Dichlorobenzene-d4	13.848	152		49303	23.380	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	93.520%		
Target Compounds							
						Qvalue	
13) Acetone	4.124	43		6099	3.946	ug/L	99
16) Methylene chloride	4.923	84		15238	2.234	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061224\
Data File : VW029105.D
Acq On : 12 Jun 2024 14:26
Operator : SY/MD
Sample : P2776-22
Misc : 5.36g/10mL/MSVOA_W/SoIL/A
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4C76

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/13/2024
Supervised By :Mahesh Dadoda 06/13/2024

Quant Time: Jun 13 00:50:15 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jun 13 00:47:39 2024
Response via : Initial Calibration

