

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061322\
 Data File : VW023466.D
 Acq On : 13 Jun 2022 09:34
 Operator : SY/VA
 Sample : VW0613SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Jun 14 01:32:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jun 14 01:31:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	395811	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	365546	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	162030	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	147158	23.402	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.600%
7) Chloroethane-d5	2.885	69	103627	22.418	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.680%
11) 1,1-Dichloroethene-d2	4.019	63	163776	18.659	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	74.640%
21) 2-Butanone-d5	7.080	46	55625	43.325	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	86.660%
24) Chloroform-d	7.653	84	252675	23.190	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.760%
26) 1,2-Dichloroethane-d4	8.311	65	133314	22.718	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	90.880%
32) Benzene-d6	8.281	84	482483	24.893	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	99.560%
36) 1,2-Dichloropropane-d6	9.274	67	142985	25.040	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	100.160%
41) Toluene-d8	10.323	98	461025	24.352	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	97.400%
43) trans-1,3-Dichloroprop...	10.579	79	59395	22.789	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	91.160%
47) 2-Hexanone-d5	10.926	63	41046	44.984	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.960%
56) 1,1,2,2-Tetrachloroeth...	12.694	84	114497	21.468	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	85.880%
66) 1,2-Dichlorobenzene-d4	13.853	152	153277	26.205	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	104.800%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.036	75	5604	0.709	ug/L	# 72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061322\
Data File : VW023466.D
Acq On : 13 Jun 2022 09:34
Operator : SY/VA
Sample : VW0613SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Jun 14 01:32:35 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jun 14 01:31:49 2022
Response via : Initial Calibration

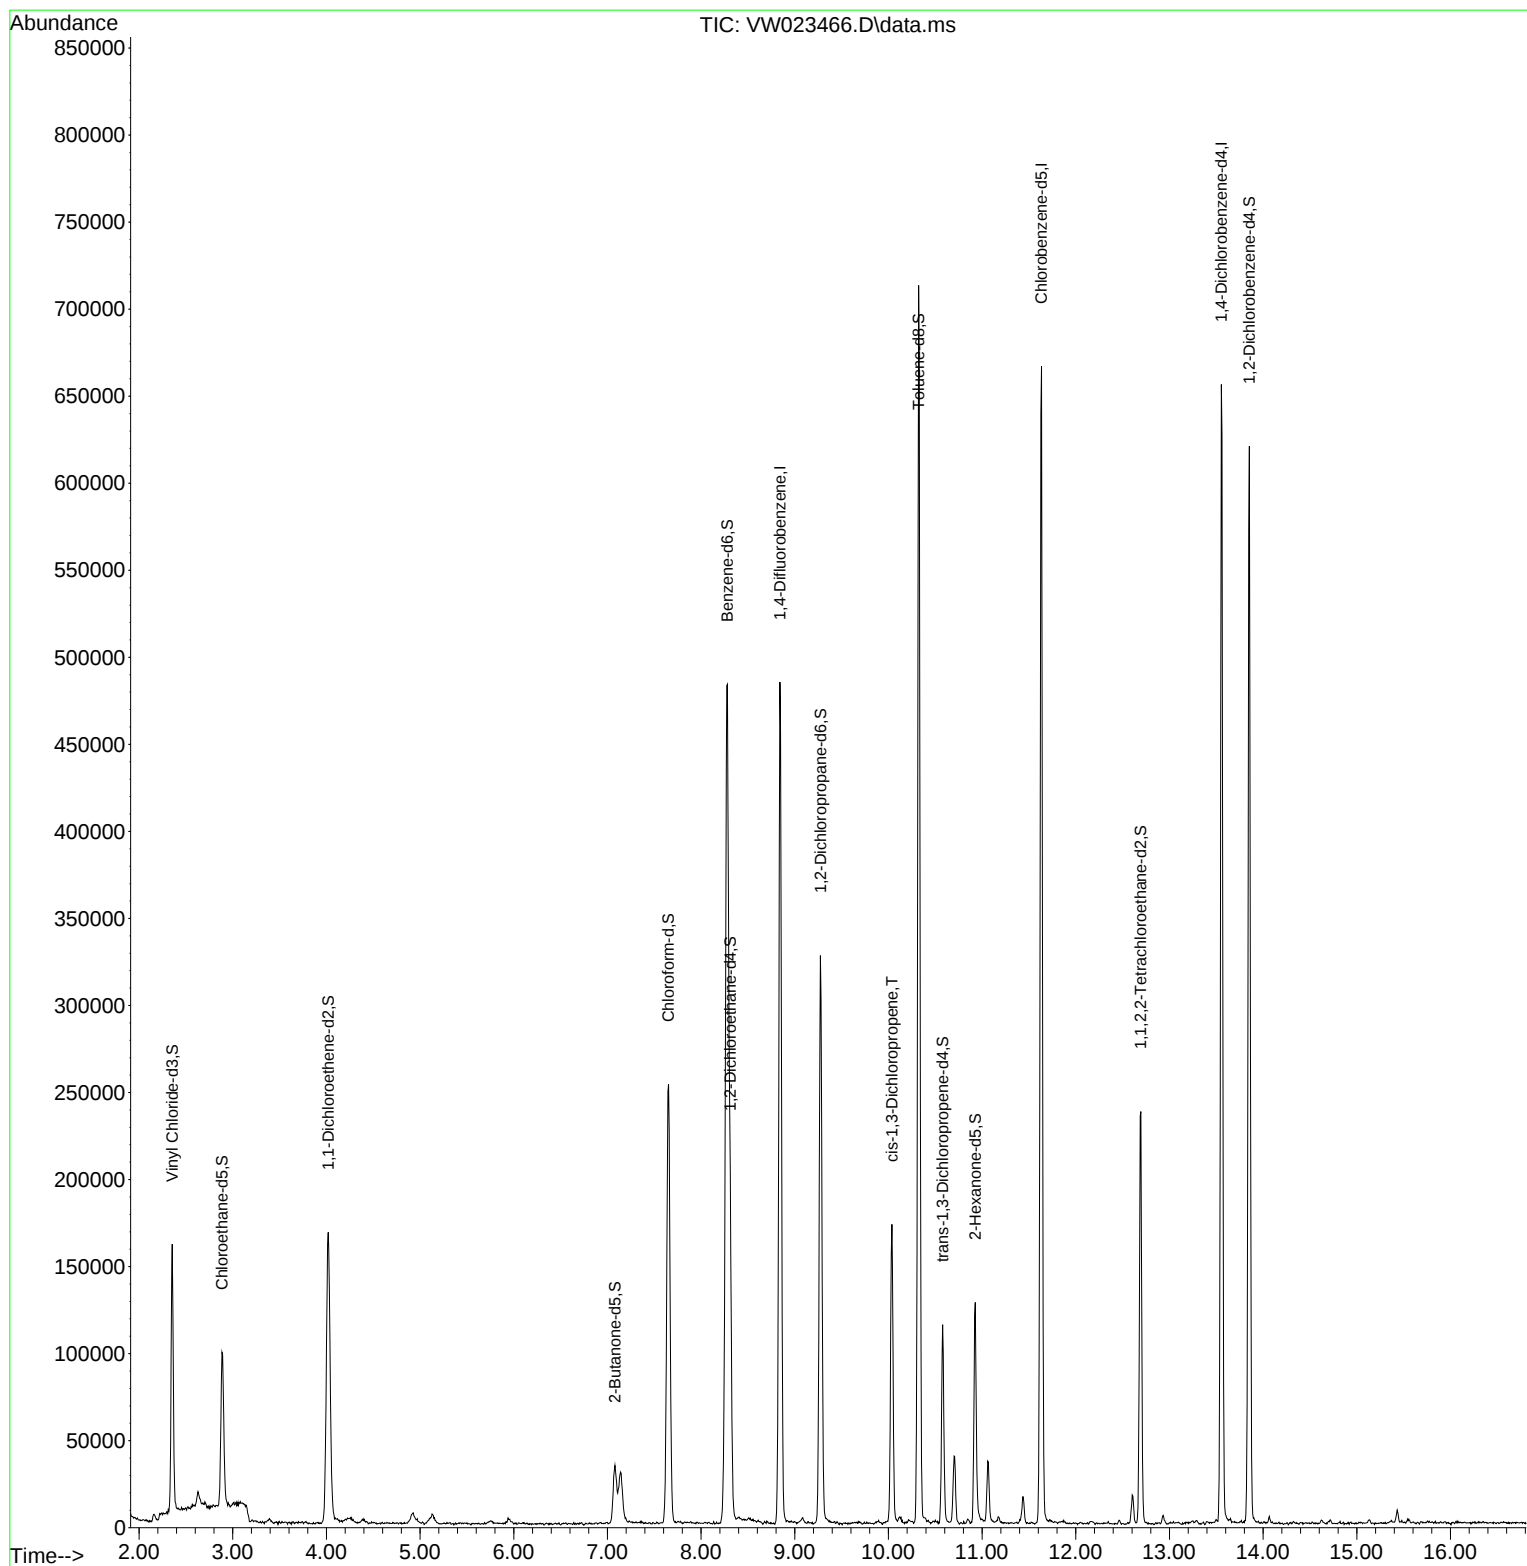

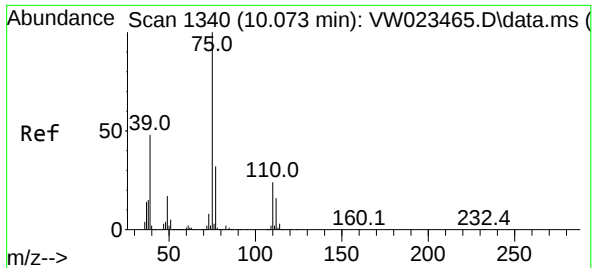

#39
 cis-1,3-Dichloropropene
 Concen: 0.709 ug/L
 RT: 10.036 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW023466.D
 Acq: 13 Jun 2022 09:34

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 5604
 Ion Ratio Lower Upper
 75 100
 77 47.2 22.1 41.1#

