

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061322\
 Data File : VW023470.D
 Acq On : 13 Jun 2022 11:11
 Operator : SY/VA
 Sample : N3226-18RE
 Misc : 6.48g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Jun 14 01:33:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jun 14 01:31:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	357125	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	222504	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	39454	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	155795	27.460	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	109.840%
7) Chloroethane-d5	2.885	69	107757	25.837	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	103.360%
11) 1,1-Dichloroethene-d2	4.013	63	148753	18.784	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	75.120%
21) 2-Butanone-d5	7.080	46	65380	56.439	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	112.880%
24) Chloroform-d	7.647	84	239487	24.361	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	97.440%
26) 1,2-Dichloroethane-d4	8.305	65	130873	24.718	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.880%
32) Benzene-d6	8.275	84	444143	37.646	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	150.600%#
36) 1,2-Dichloropropane-d6	9.275	67	139082	40.014	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	160.040%#
41) Toluene-d8	10.323	98	335166	29.086	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	116.360%
43) trans-1,3-Dichloroprop...	10.579	79	36420	22.957	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	91.840%
47) 2-Hexanone-d5	10.921	63	38359	69.065	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	138.120%#
56) 1,1,2,2-Tetrachloroeth...	12.689	84	110544	34.052	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	136.200%#
66) 1,2-Dichlorobenzene-d4	13.853	152	53902	37.845	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	151.400%#
Target Compounds						Qvalue
14) Carbon disulfide	4.379	76	14215	1.188	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061322\
Data File : VW023470.D
Acq On : 13 Jun 2022 11:11
Operator : SY/VA
Sample : N3226-18RE
Misc : 6.48g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Jun 14 01:33:28 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jun 14 01:31:49 2022
Response via : Initial Calibration

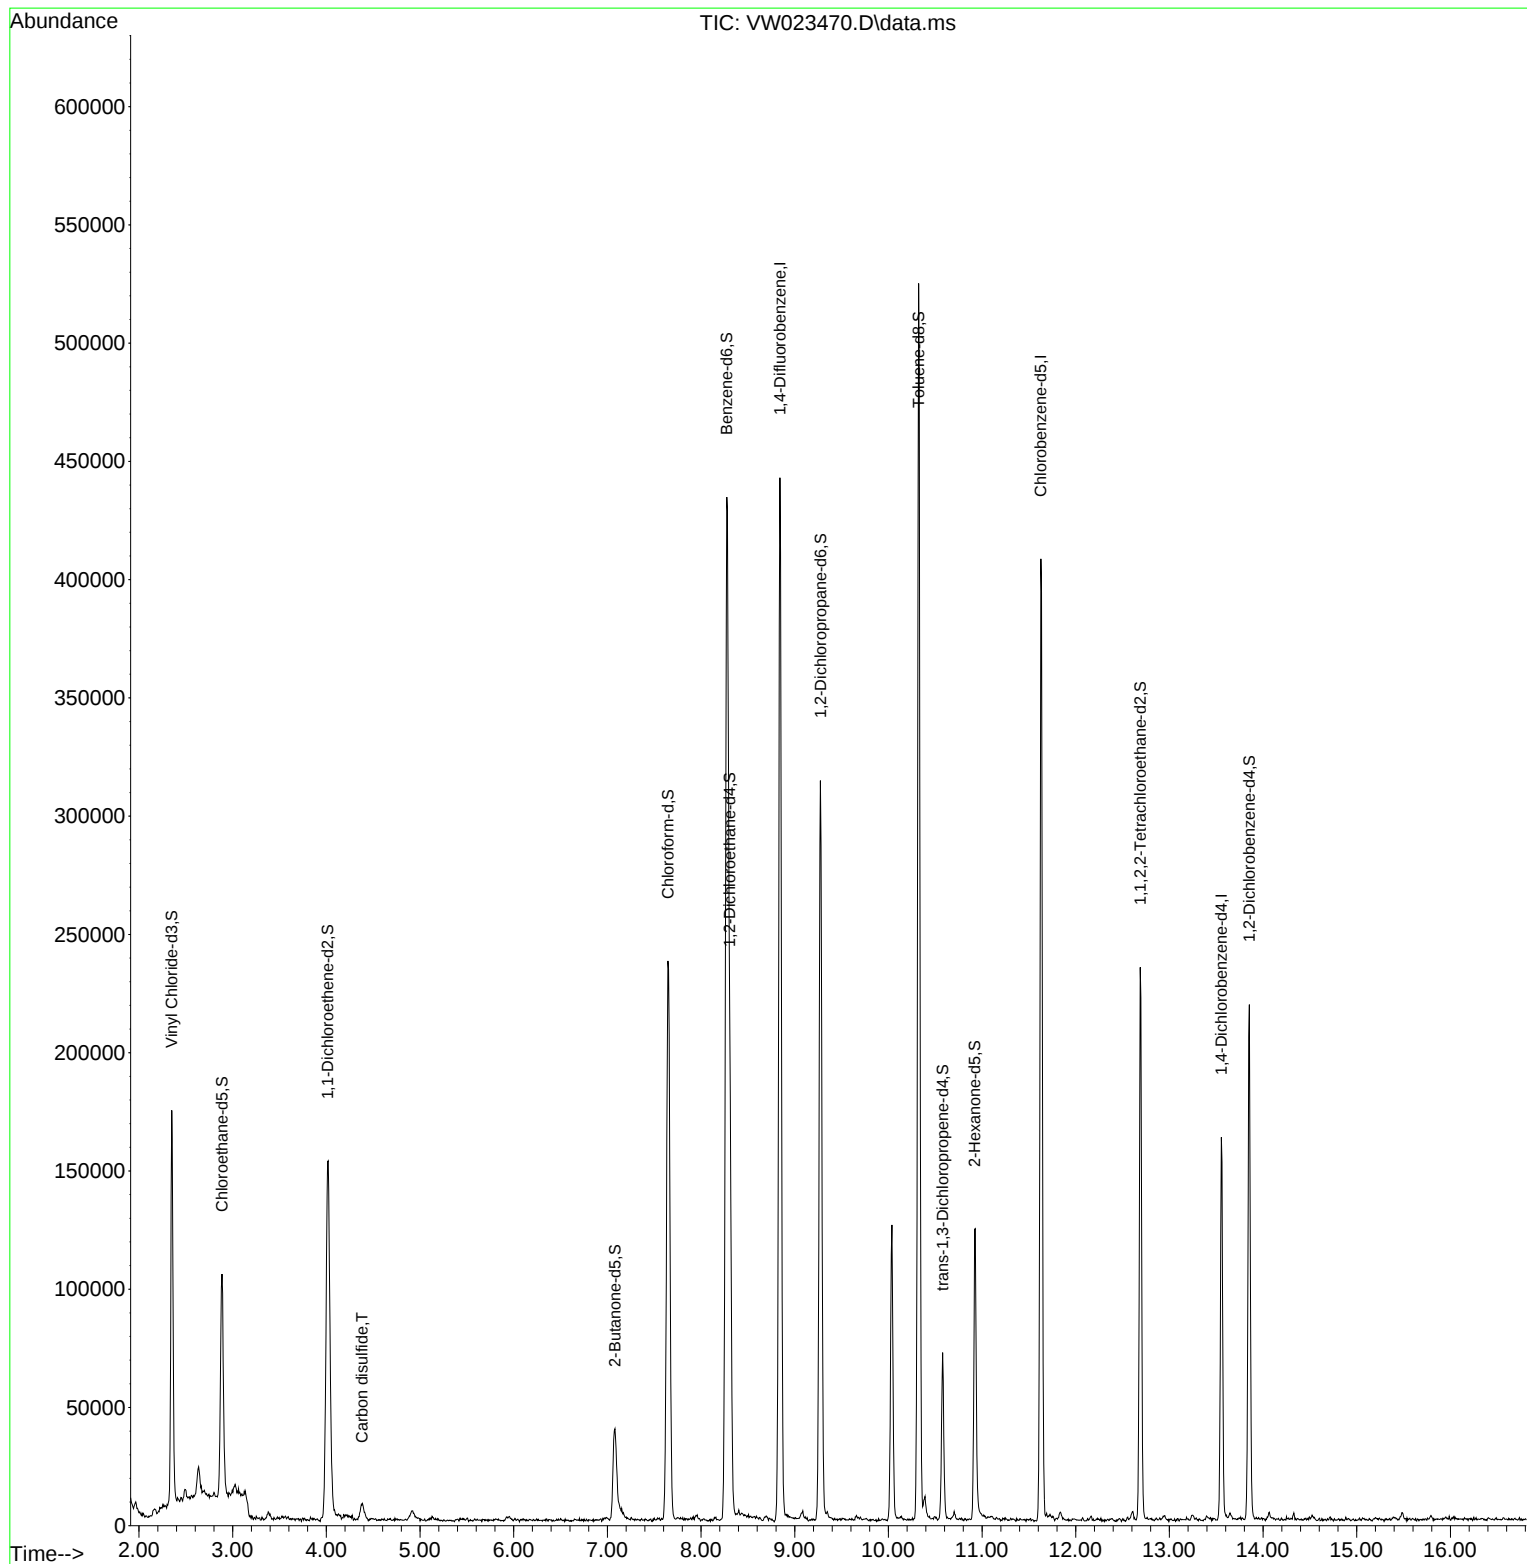

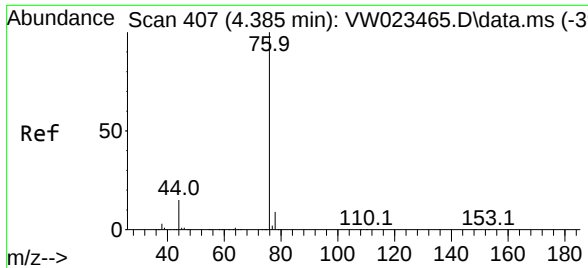

#14
 Carbon disulfide
 Concen: 1.188 ug/L
 RT: 4.379 min Scan# 406
 Delta R.T. -0.006 min
 Lab File: VW023470.D
 Acq: 13 Jun 2022 11:11

Instrument :
 MSVOA_W
 ClientSampleId :

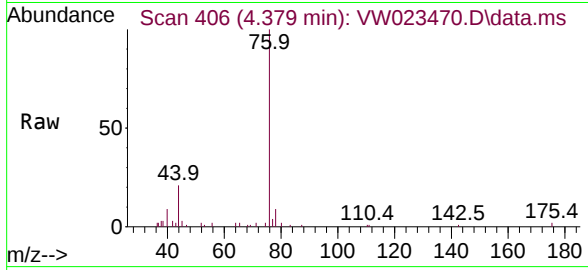

Tgt Ion: 76 Resp: 14215
 Ion Ratio Lower Upper
 76 100
 78 9.3 7.7 11.5

