




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061322\
 Data File : VW023475.D
 Acq On : 13 Jun 2022 13:12
 Operator : SY/VA
 Sample : N3226-19
 Misc : 6.12g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4N9

Manual IntegrationsAPPROVED

Quant Time: Jun 14 01:34:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jun 14 01:31:49 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/14/2022
 Supervised By :Mahesh Dadoda 06/15/2022

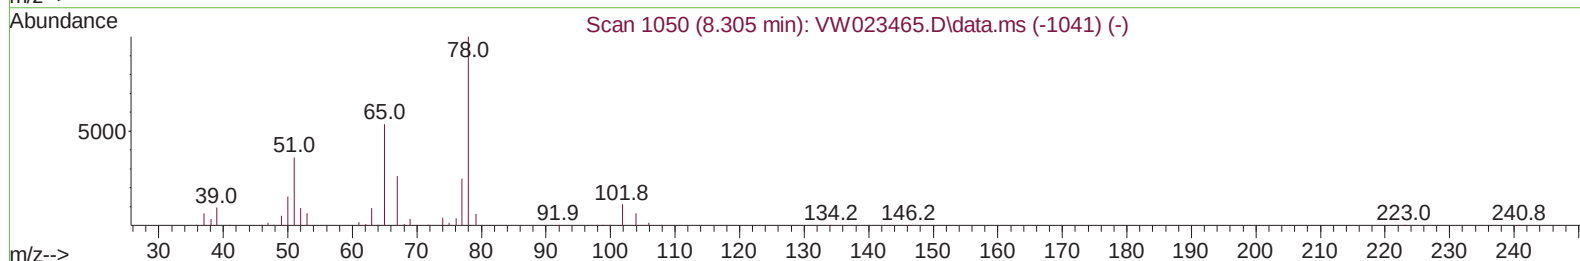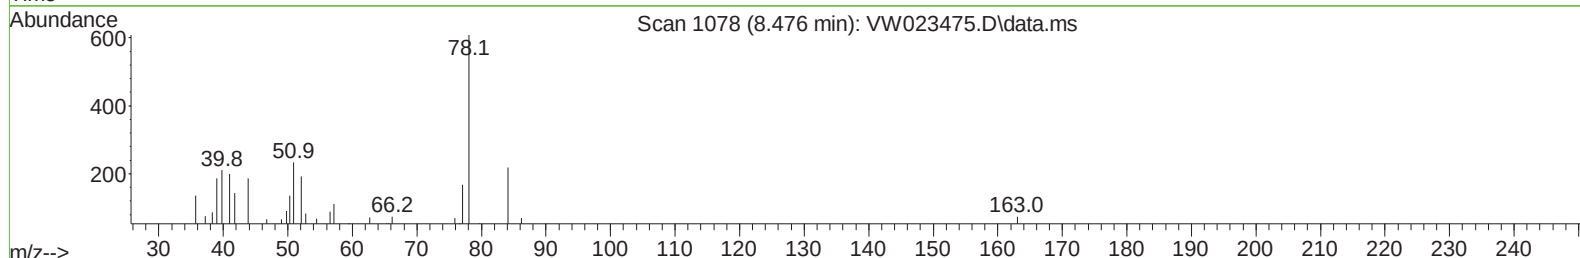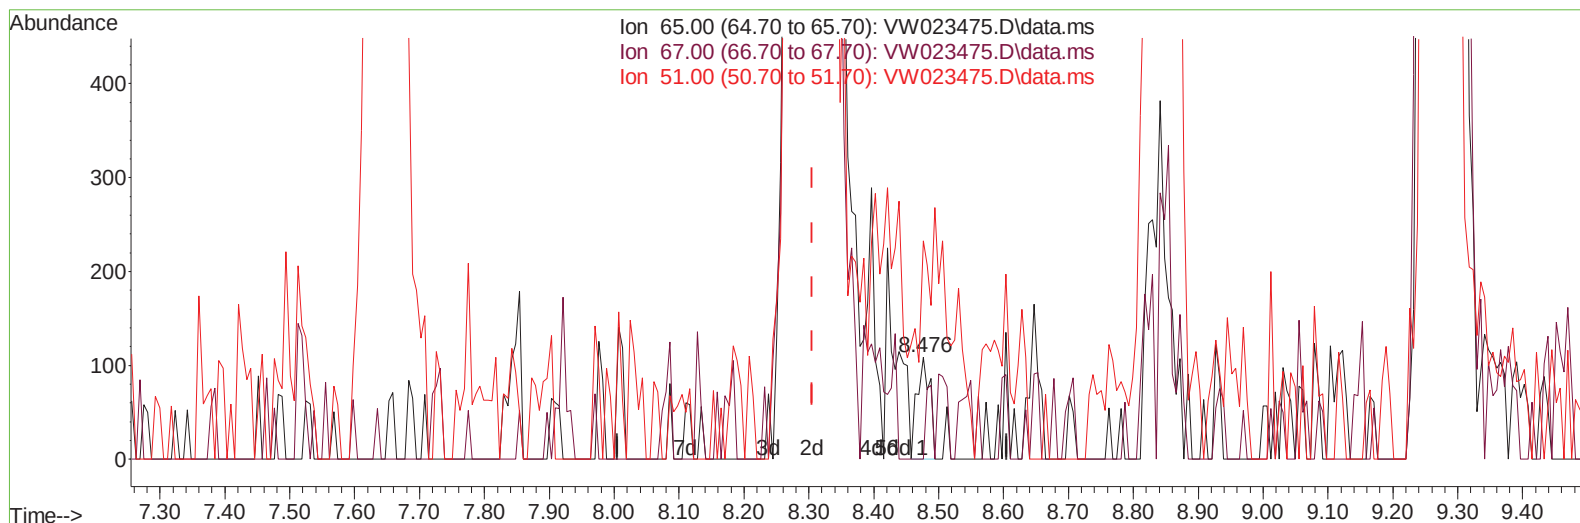

TIC: VW023475.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.476min (+ 0.171) 0.03 ug/L

response 149

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.10	38.26
51.00	92.30	78.52
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061322\
Data File : VW023475.D
Acq On : 13 Jun 2022 13:12
Operator : SY/VA
Sample : N3226-19
Misc : 6.12g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW4N9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/14/2022
Supervised By :Mahesh Dadoda 06/15/2022

Quant Time: Jun 14 01:34:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jun 14 01:31:49 2022
Response via : Initial Calibration

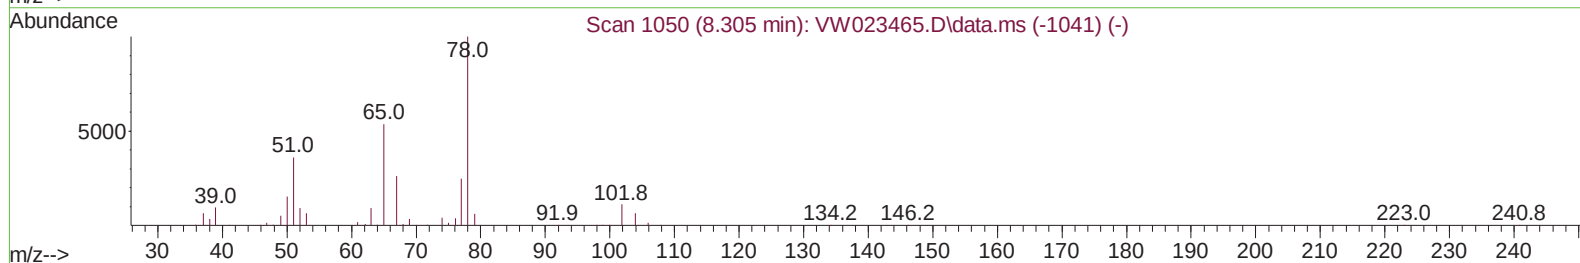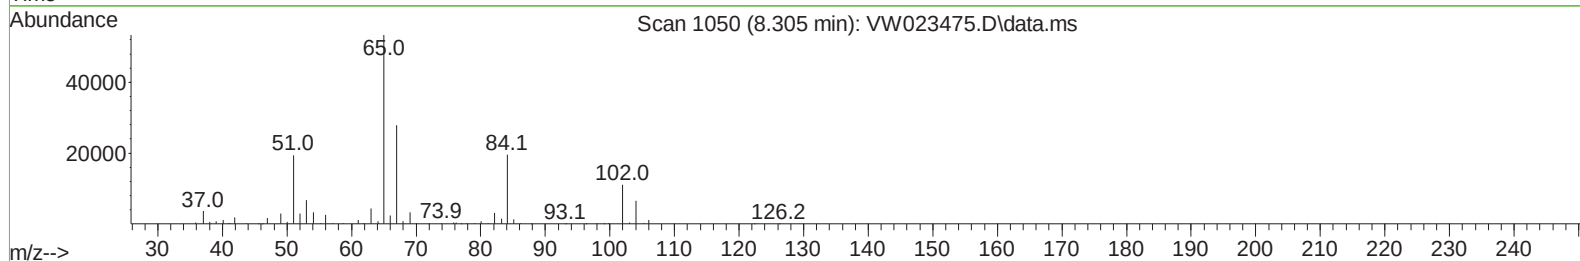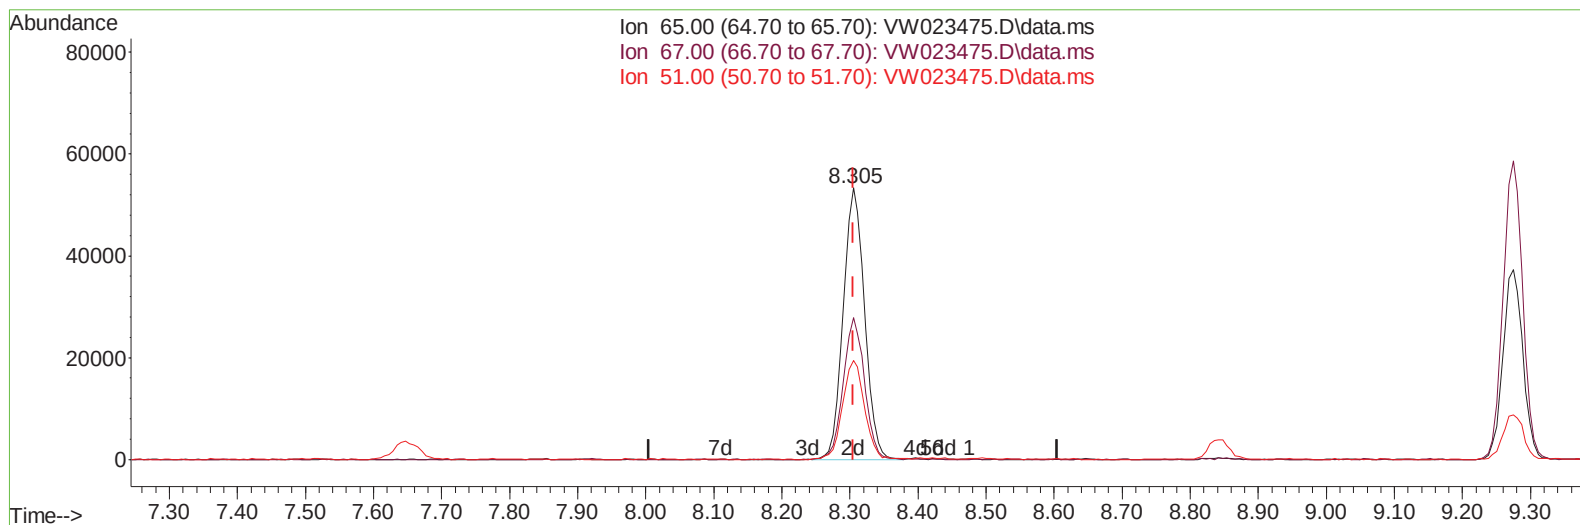

TIC: VW023475.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (-0.000) 20.34 ug/L m

response 116296

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.10	0.05#
51.00	92.30	0.10#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061322\
 Data File : VW023475.D
 Acq On : 13 Jun 2022 13:12
 Operator : SY/VA
 Sample : N3226-19
 Misc : 6.12g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4N9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/14/2022
 Supervised By :Mahesh Dadoda 06/15/2022

Quant Time: Jun 14 01:34:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jun 14 01:31:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	385696	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	326996	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	104291	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	113751	18.564	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	74.240%	
7) Chloroethane-d5	2.879	69	81457	18.084	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	72.320%	
11) 1,1-Dichloroethene-d2	4.013	63	113131	13.227	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110	Recovery	=	52.920%	
21) 2-Butanone-d5	7.080	46	50864	40.656	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	81.320%	
24) Chloroform-d	7.647	84	201338	18.963	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	75.840%	
26) 1,2-Dichloroethane-d4	8.305	65	116296m	20.338	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	81.360%	
32) Benzene-d6	8.275	84	370740	21.383	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	85.520%	
36) 1,2-Dichloropropane-d6	9.275	67	117014	22.907	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	91.640%	
41) Toluene-d8	10.323	98	320114	18.902	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	75.600%	
43) trans-1,3-Dichloroprop...	10.579	79	41692	17.882	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	71.520%	
47) 2-Hexanone-d5	10.921	63	35279	43.221	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	86.440%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	98741	20.697	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	82.800%	
66) 1,2-Dichlorobenzene-d4	13.853	152	74768	19.859	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	79.440%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061322\
Data File : VW023475.D
Acq On : 13 Jun 2022 13:12
Operator : SY/VA
Sample : N3226-19
Misc : 6.12g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW4N9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/14/2022
Supervised By :Mahesh Dadoda 06/15/2022

Quant Time: Jun 14 01:34:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jun 14 01:31:49 2022
Response via : Initial Calibration

