




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061322\
 Data File : VW023479.D
 Acq On : 13 Jun 2022 14:48
 Operator : SY/VA
 Sample : N3256-11
 Misc : 5.77g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AF5

Manual IntegrationsAPPROVED

Quant Time: Jun 14 01:35:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jun 14 01:31:49 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/14/2022
 Supervised By :Mahesh Dadoda 06/15/2022

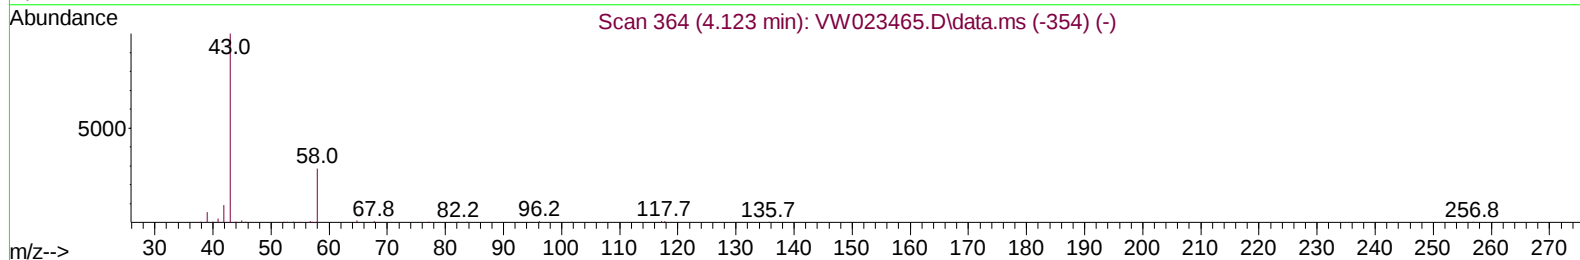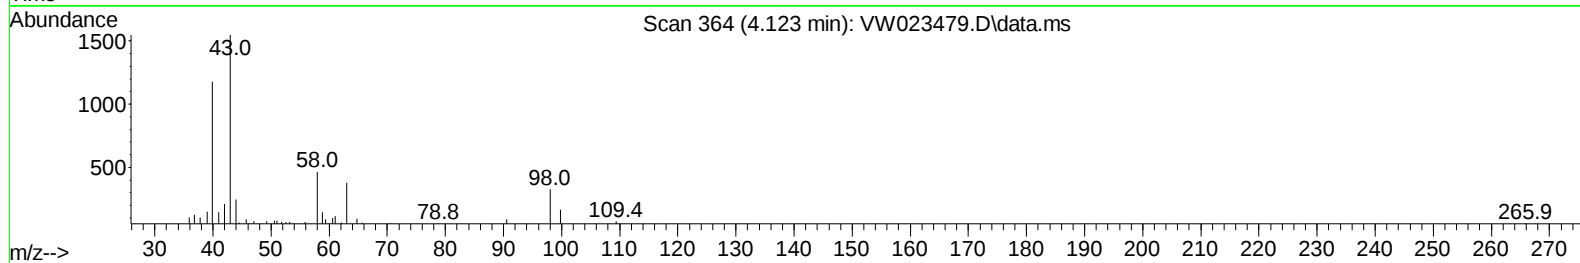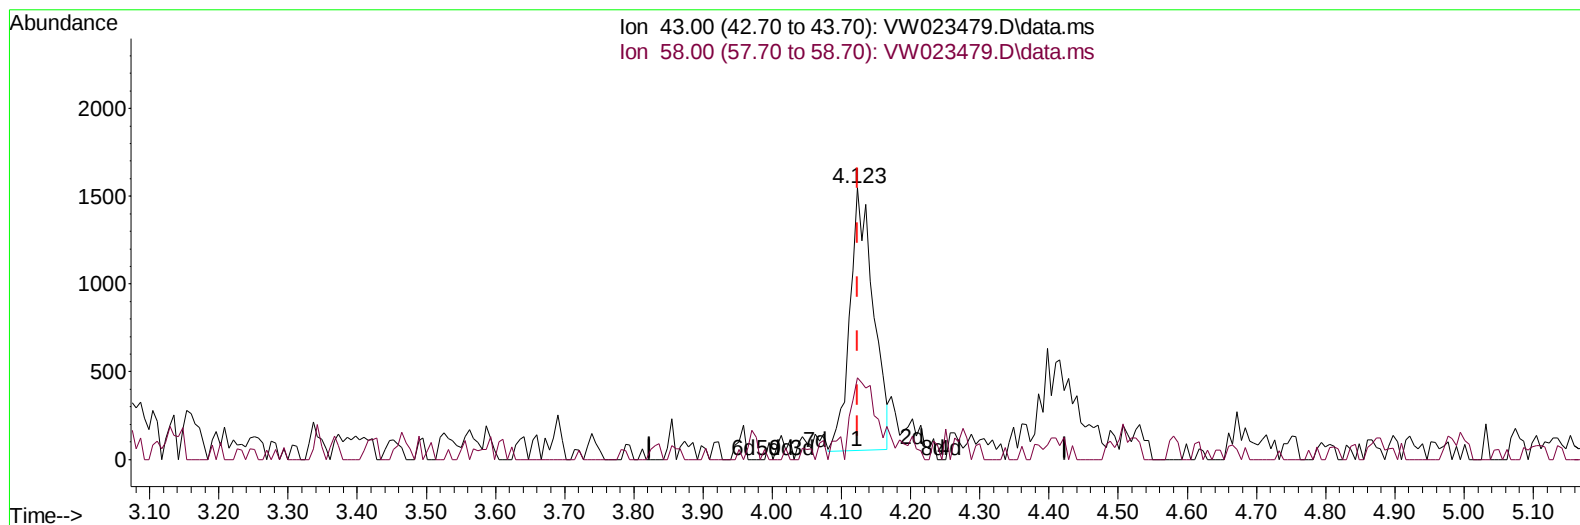

TIC: VW023479.D\data.ms

(13) Acetone (T)

4.123min (-0.000) 4.30 ug/L

response 3509

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	19.69
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061322\
 Data File : VW023479.D
 Acq On : 13 Jun 2022 14:48
 Operator : SY/VA
 Sample : N3256-11
 Misc : 5.77g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AF5

Manual IntegrationsAPPROVED

Quant Time: Jun 14 01:35:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jun 14 01:31:49 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/14/2022
 Supervised By :Mahesh Dadoda 06/15/2022

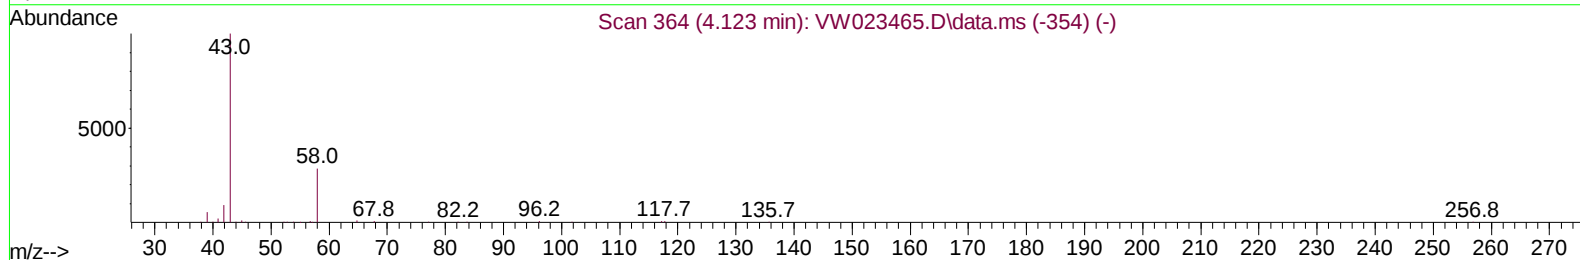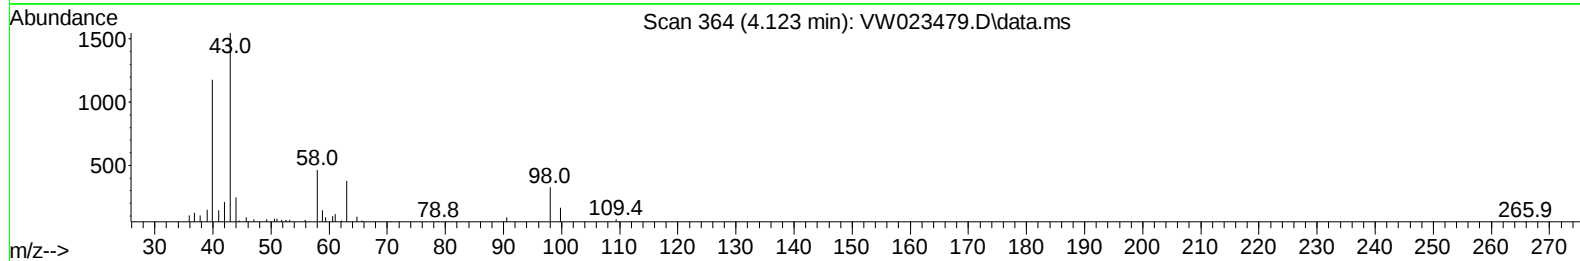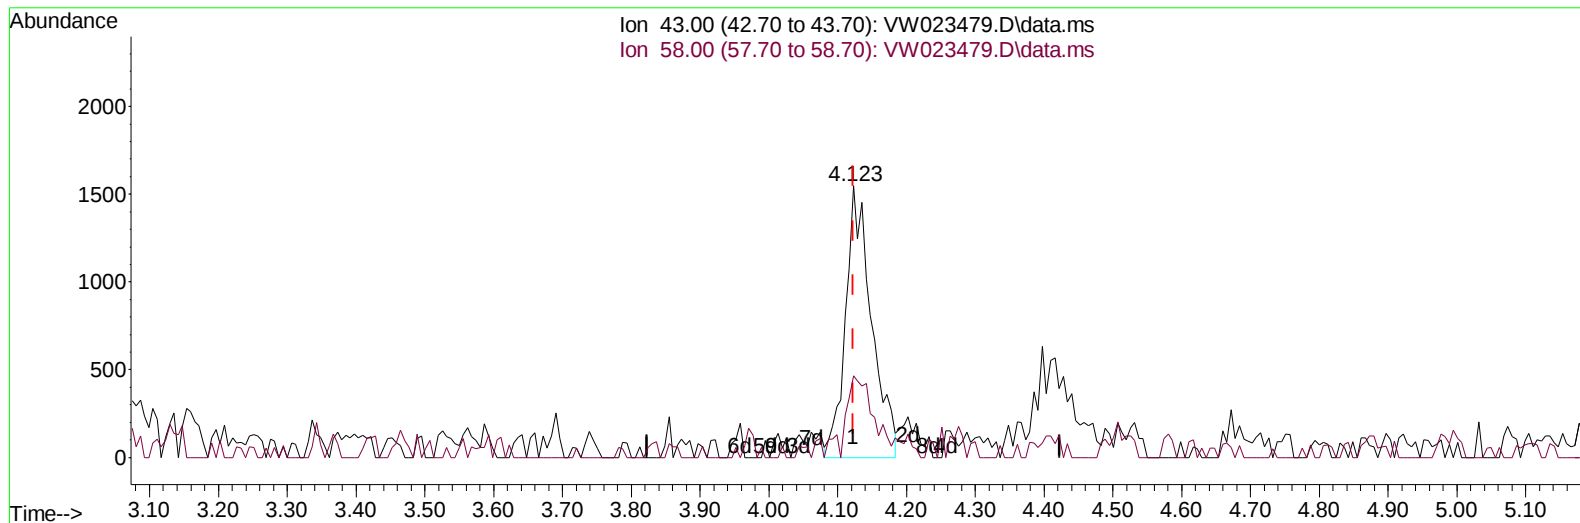

TIC: VW023479.D\data.ms

(13) Acetone (T)

4.123min (-0.000) 4.97 ug/L m

response 4053

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	17.05
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061322\
Data File : VW023479.D
Acq On : 13 Jun 2022 14:48
Operator : SY/VA
Sample : N3256-11
Misc : 5.77g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AF5

Manual IntegrationsAPPROVED

Quant Time: Jun 14 01:35:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jun 14 01:31:49 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/14/2022
Supervised By :Mahesh Dadoda 06/15/2022

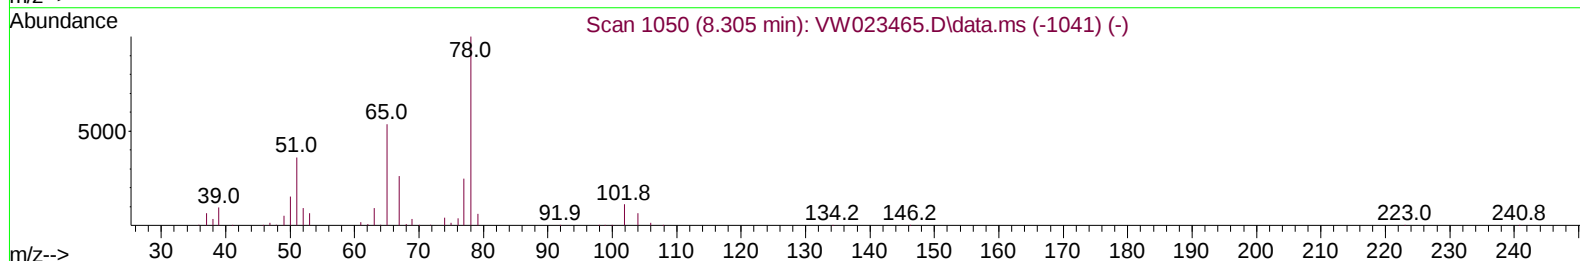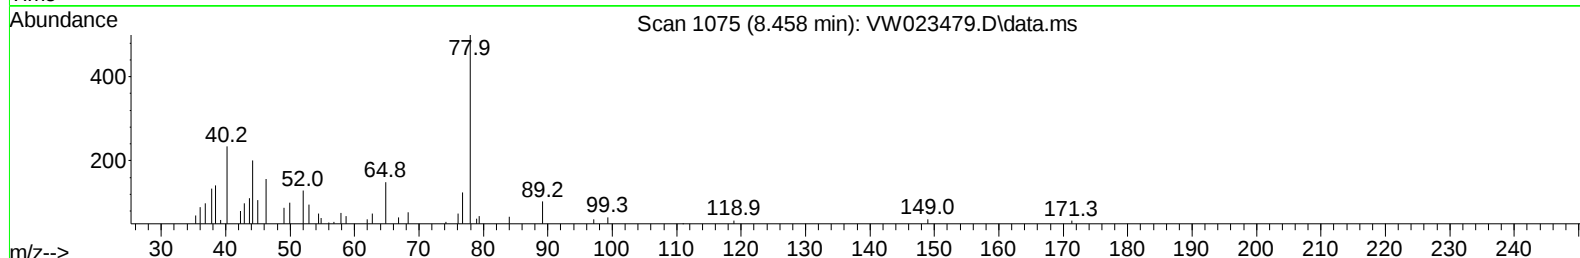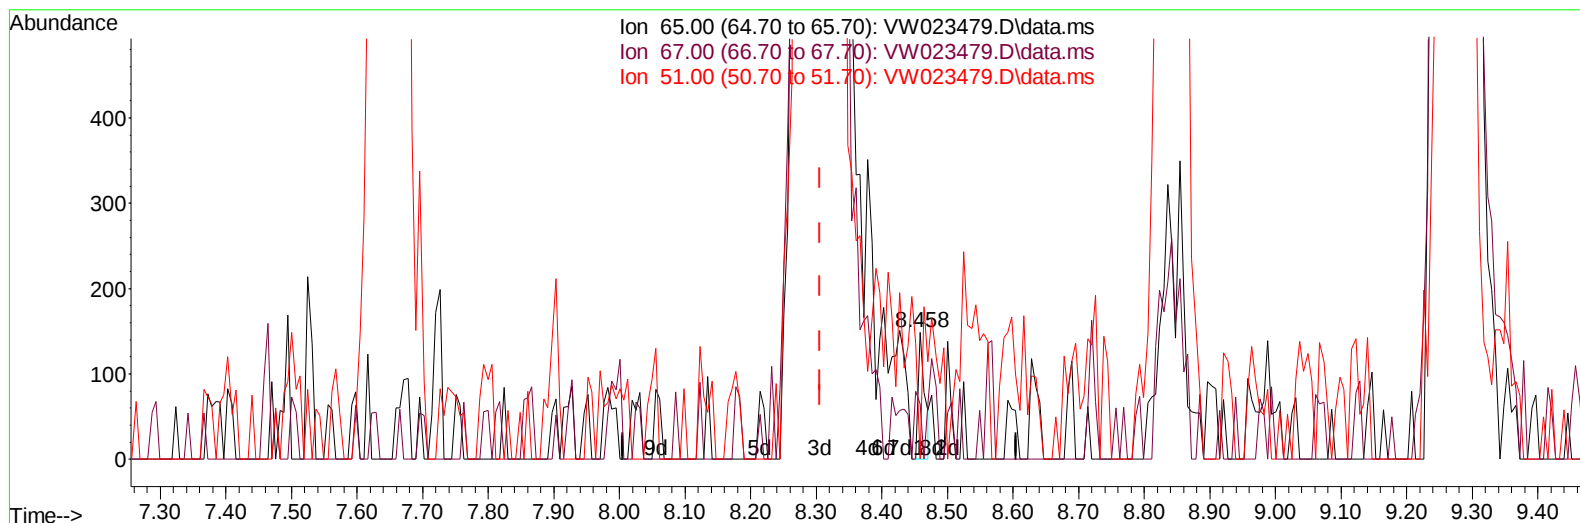

TIC: VW023479.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.458min (+ 0.152) 0.02 ug/L

response 104

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.10	50.96
51.00	92.30	102.88
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061322\
 Data File : VW023479.D
 Acq On : 13 Jun 2022 14:48
 Operator : SY/VA
 Sample : N3256-11
 Misc : 5.77g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AF5

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/14/2022
 Supervised By :Mahesh Dadoda 06/15/2022

Quant Time: Jun 14 01:35:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jun 14 01:31:49 2022
 Response via : Initial Calibration

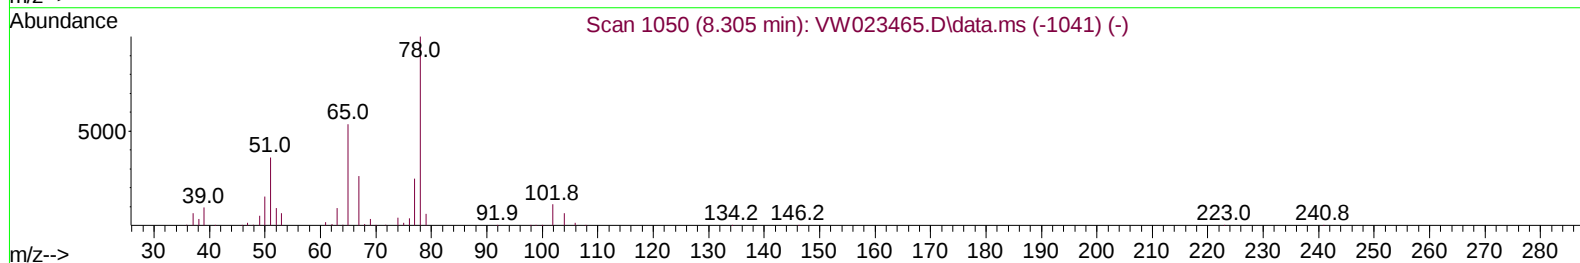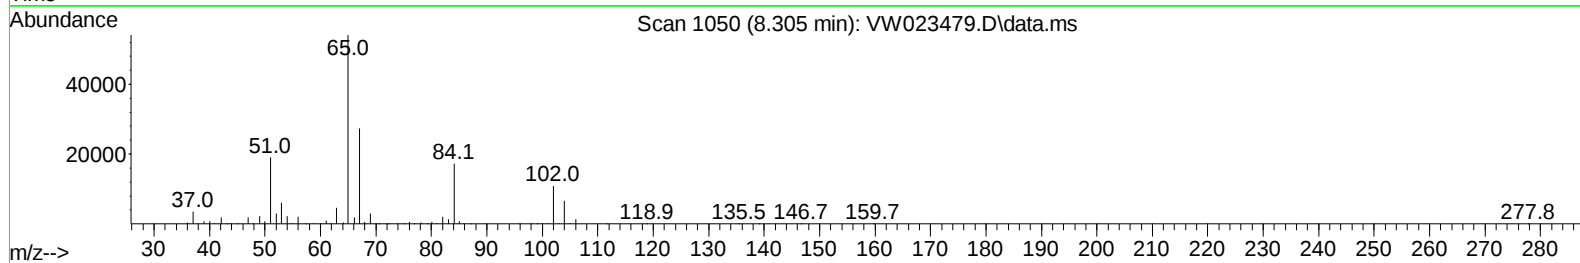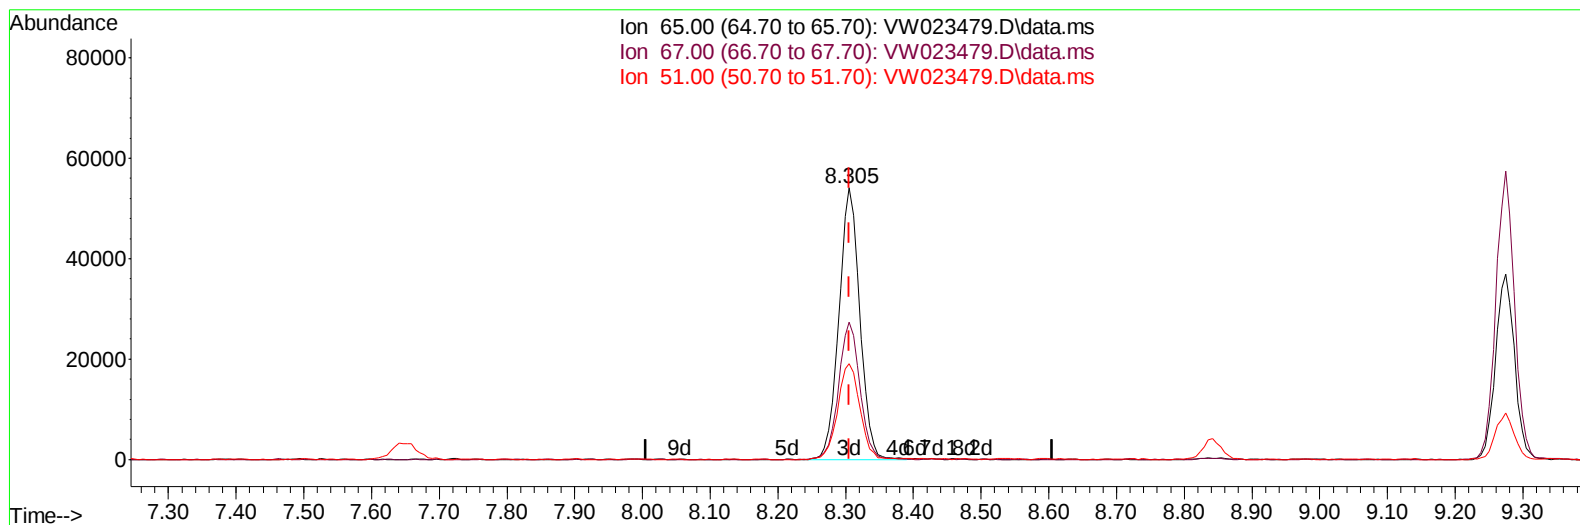

TIC: VW023479.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (0.000) 22.37 ug/L m

response 115817

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.10	0.05#
51.00	92.30	0.09#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061322\
 Data File : VW023479.D
 Acq On : 13 Jun 2022 14:48
 Operator : SY/VA
 Sample : N3256-11
 Misc : 5.77g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AF5

Manual IntegrationsAPPROVED

Quant Time: Jun 14 01:35:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jun 14 01:31:49 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/14/2022
 Supervised By :Mahesh Dadoda 06/15/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		349252	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		327364	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		148537	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.349	65		112406	20.259	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	81.040%		
7) Chloroethane-d5	2.879	69		81161	19.899	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	79.600%		
11) 1,1-Dichloroethene-d2	4.013	63		108695	14.035	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110		Recovery =	56.120%		
21) 2-Butanone-d5	7.074	46		67405	59.499	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	119.000%		
24) Chloroform-d	7.647	84		195856	20.372	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	81.480%		
26) 1,2-Dichloroethane-d4	8.305	65		115817m	22.368	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	89.480%		
32) Benzene-d6	8.275	84		358803	20.671	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	82.680%		
36) 1,2-Dichloropropane-d6	9.275	67		110646	21.636	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	86.560%		
41) Toluene-d8	10.323	98		328540	19.378	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	77.520%		
43) trans-1,3-Dichloroprop...	10.579	79		45302	19.409	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	77.640%		
47) 2-Hexanone-d5	10.927	63		50348	61.614	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	123.220%		
56) 1,1,2,2-Tetrachloroeth...	12.689	84		119176	24.952	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	99.800%		
66) 1,2-Dichlorobenzene-d4	13.853	152		116873	21.796	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	87.200%		
Target Compounds							
13) Acetone	4.123	43		4053m	4.966	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061322\
Data File : VW023479.D
Acq On : 13 Jun 2022 14:48
Operator : SY/VA
Sample : N3256-11
Misc : 5.77g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AF5

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/14/2022
Supervised By :Mahesh Dadoda 06/15/2022

Quant Time: Jun 14 01:35:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jun 14 01:31:49 2022
Response via : Initial Calibration

