

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061322\
 Data File : VW023470.D
 Acq On : 13 Jun 2022 11:11
 Operator : SY/VA
 Sample : N3226-18RE
 Misc : 6.48g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4N8RE

Quant Time: Jun 14 01:33:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jun 14 01:31:49 2022
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		8.842	114	357125	25.000	ug/L	0.00
28) Chlorobenzene-d5		11.628	117	222504	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		13.554	152	39454	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		2.349	65	155795	27.460	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	= 109.840%		
7) Chloroethane-d5		2.885	69	107757	25.837	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	= 103.360%		
11) 1,1-Dichloroethene-d2		4.013	63	148753	18.784	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	= 75.120%		
21) 2-Butanone-d5		7.080	46	65380	56.439	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	= 112.880%		
24) Chloroform-d		7.647	84	239487	24.361	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	= 97.440%		
26) 1,2-Dichloroethane-d4		8.305	65	130873	24.718	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	= 98.880%		
32) Benzene-d6		8.275	84	444143	37.646	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	= 150.600%#		
36) 1,2-Dichloropropane-d6		9.275	67	139082	40.014	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	= 160.040%#		
41) Toluene-d8		10.323	98	335166	29.086	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	= 116.360%		
43) trans-1,3-Dichloroprop...		10.579	79	36420	22.957	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	= 91.840%		
47) 2-Hexanone-d5		10.921	63	38359	69.065	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	= 138.120%#		
56) 1,1,2,2-Tetrachloroeth...		12.689	84	110544	34.052	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	= 136.200%#		
66) 1,2-Dichlorobenzene-d4		13.853	152	53902	37.845	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	= 151.400%#		
Target Compounds							Qvalue
14) Carbon disulfide		4.379	76	14215	1.188	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061322\
Data File : VW023470.D
Acq On : 13 Jun 2022 11:11
Operator : SY/VA
Sample : N3226-18RE
Misc : 6.48g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW4N8RE


Quant Time: Jun 14 01:33:28 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jun 14 01:31:49 2022
Response via : Initial Calibration

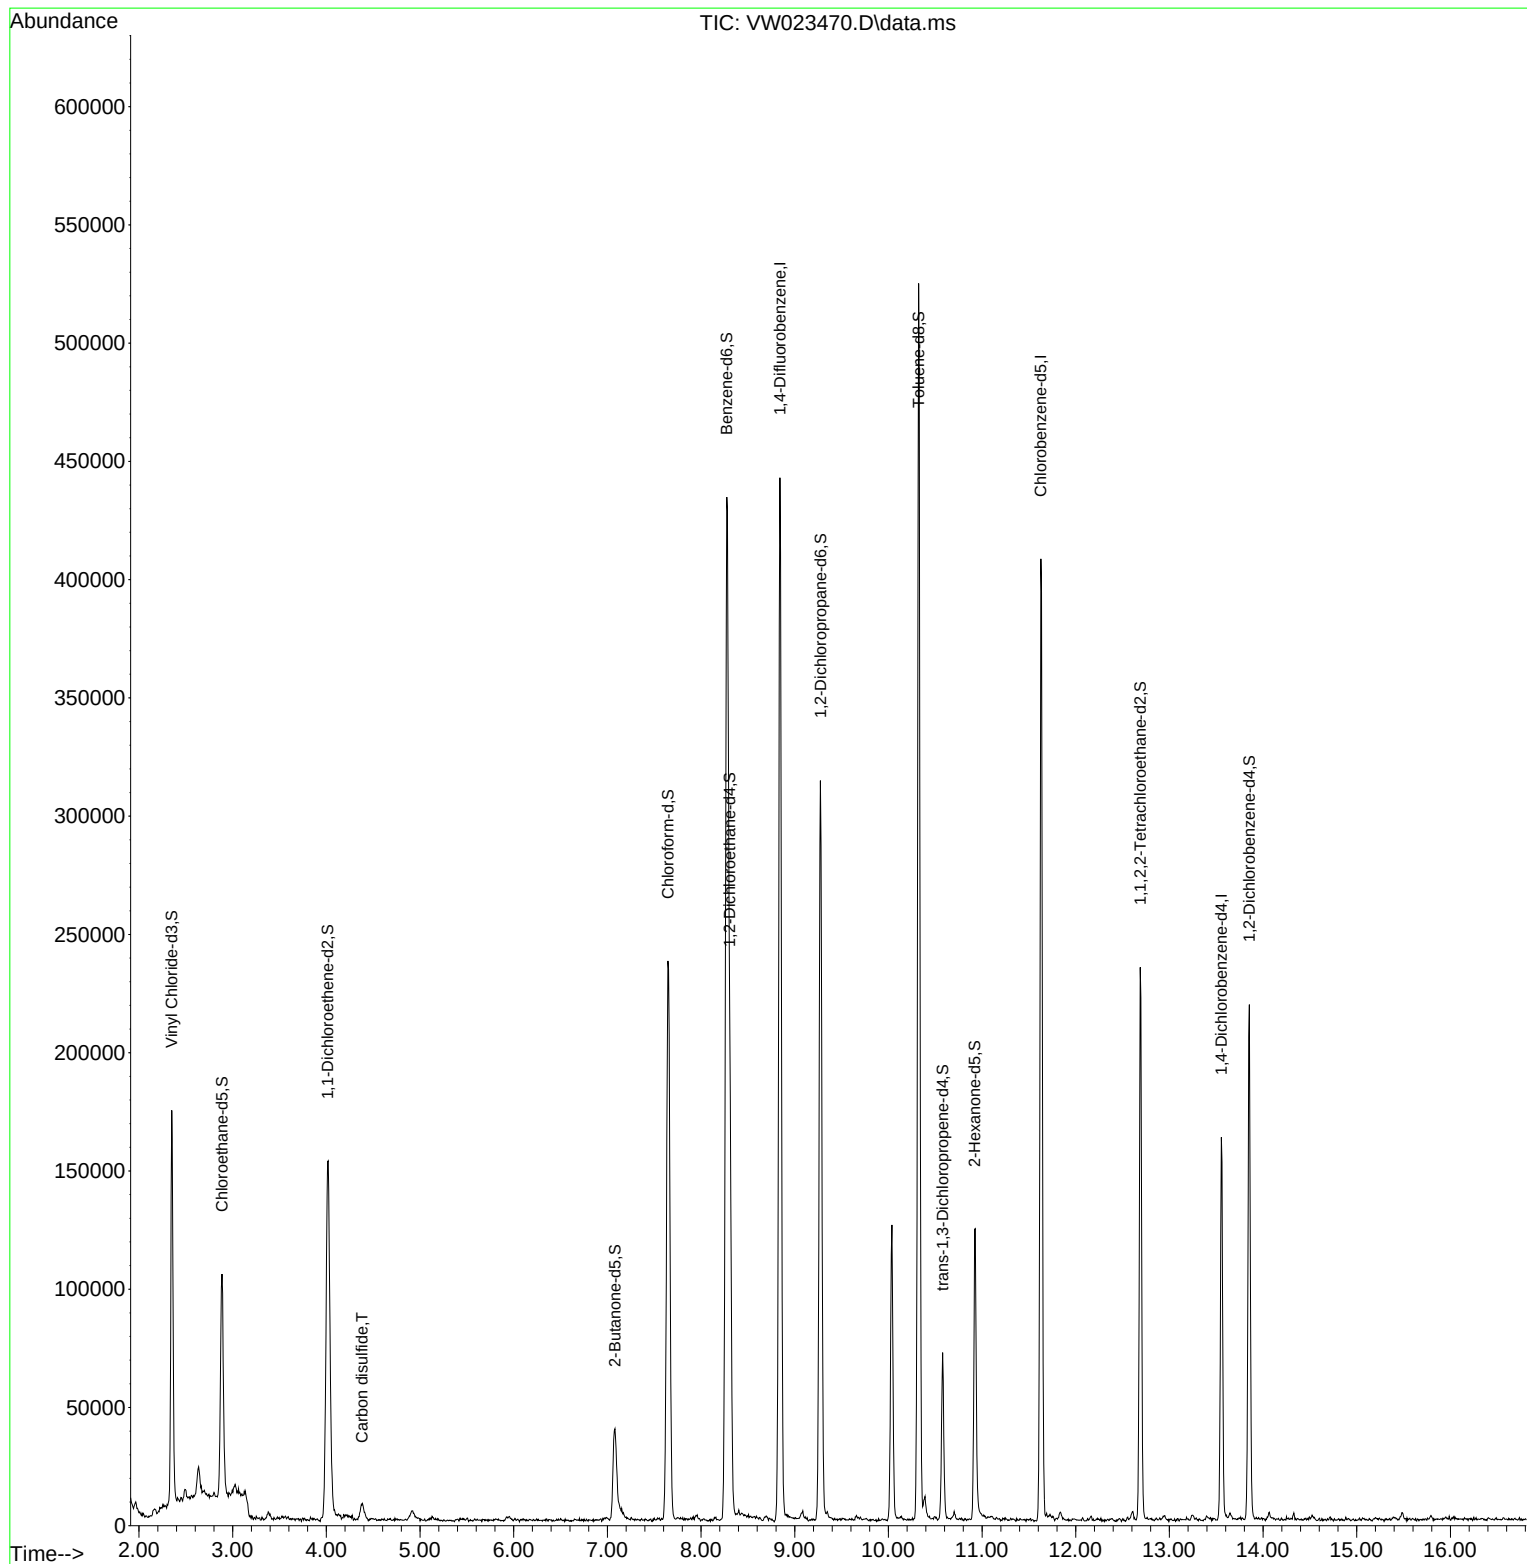

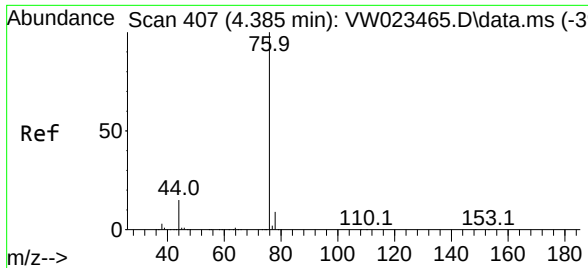

#14
Carbon disulfide
Concen: 1.188 ug/L
RT: 4.379 min Scan# 40
Delta R.T. -0.006 min
Lab File: VW023470.D
Acq: 13 Jun 2022 11:11

Instrument :
MSVOA_W
ClientSampleId :
EW4N8RE

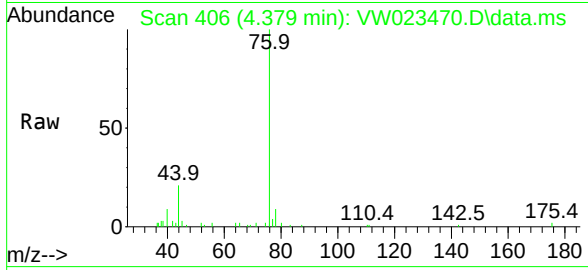

Tgt Ion: 76 Resp: 14215
Ion Ratio Lower Upper
76 100
78 9.3 7.7 11.5

