

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061322\
 Data File : VW023477.D
 Acq On : 13 Jun 2022 14:00
 Operator : SY/VA
 Sample : N3292-02
 Misc : 6.53g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4P3

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 06/14/2022
 Supervised By : Mahesh Dadoda 06/15/2022

Quant Time: Jun 14 01:34:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jun 14 01:31:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	434904	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	382834	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	150412	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	137515	19.903	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.600%
7) Chloroethane-d5	2.885	69	102897	20.259	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.040%
11) 1,1-Dichloroethene-d2	4.019	63	136432	14.147	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	56.600%
21) 2-Butanone-d5	7.080	46	59836	42.416	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	84.840%
24) Chloroform-d	7.647	84	248716	20.775	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	83.080%
26) 1,2-Dichloroethane-d4	8.305	65	139827m	21.686	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	86.760%
32) Benzene-d6	8.275	84	461389	22.730	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	90.920%
36) 1,2-Dichloropropane-d6	9.275	67	143273	23.957	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.840%
41) Toluene-d8	10.323	98	413901	20.876	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	83.520%
43) trans-1,3-Dichloroprop...	10.579	79	55178	20.215	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	80.840%
47) 2-Hexanone-d5	10.921	63	46502	48.662	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.320%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	123081	22.035	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	88.160%
66) 1,2-Dichlorobenzene-d4	13.853	152	122823	22.620	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.480%
Target Compounds					Qvalue	
13) Acetone	4.135	43	7133	7.018	ug/L	69

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061322\
Data File : VW023477.D
Acq On : 13 Jun 2022 14:00
Operator : SY/VA
Sample : N3292-02
Misc : 6.53g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EW4P3

Quant Time: Jun 14 01:34:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jun 14 01:31:49 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By : Semsettin Yesilyurt 06/14/2022
Supervised By : Mahesh Dadoda 06/15/2022

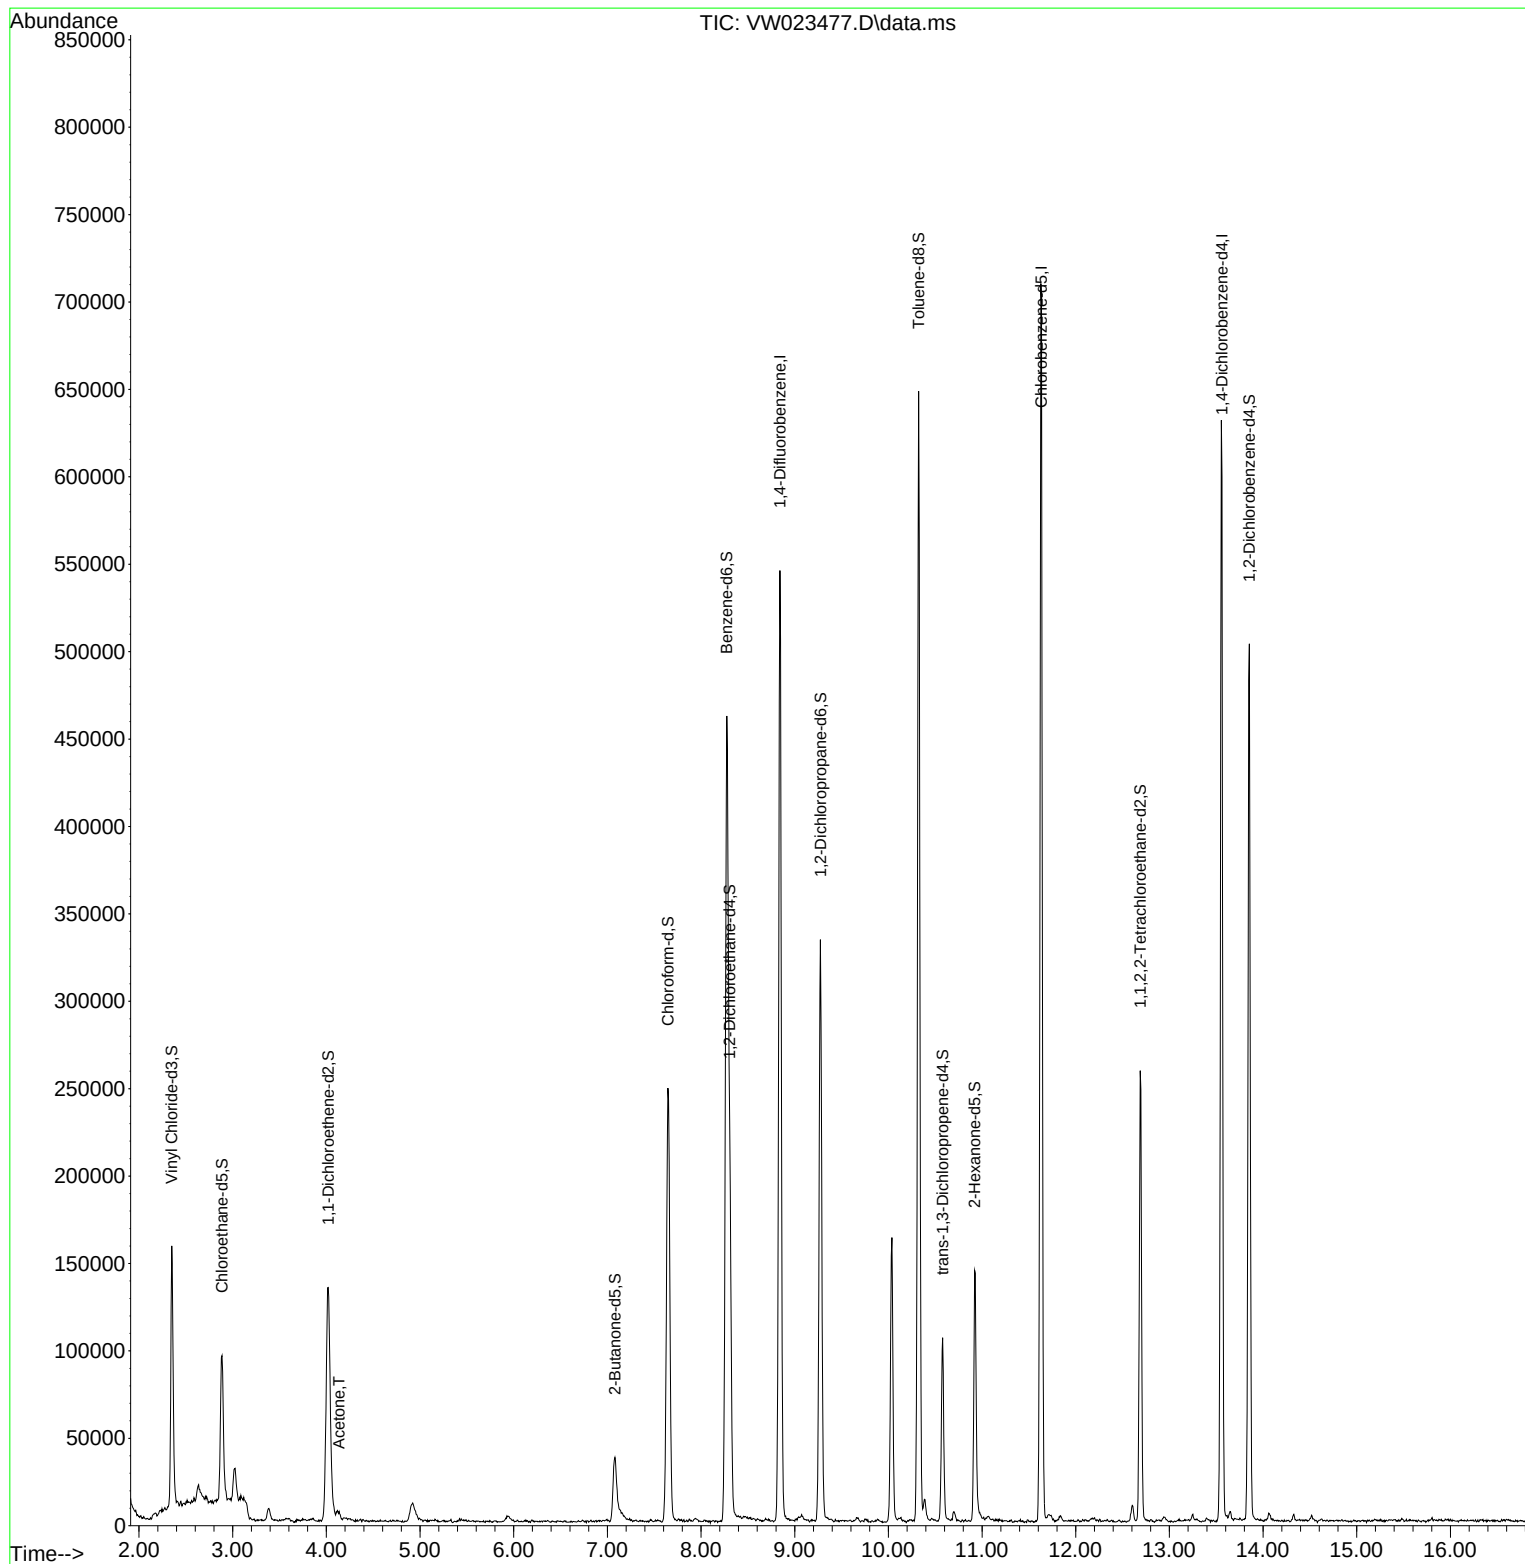

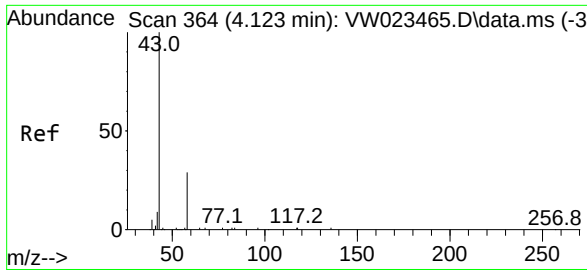

#13
Acetone
Concen: 7.018 ug/L
RT: 4.135 min Scan# 30
Delta R.T. 0.012 min
Lab File: VW023477.D
Acq: 13 Jun 2022 14:00

Instrument :
MSVOA_W
ClientSampleId :
EW4P3

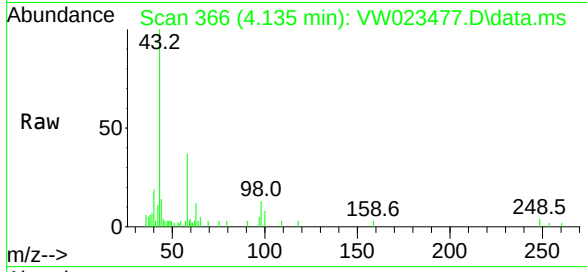

Tgt Ion: 43 Resp: 713
Ion Ratio Lower Upper
43 100
58 15.0 0.0 64.0

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 06/14/2022
Supervised By :Mahesh Dadoda 06/15/2022

