

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061322\
 Data File : VW023479.D
 Acq On : 13 Jun 2022 14:48
 Operator : SY/VA
 Sample : N3256-11
 Misc : 5.77g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AF5

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 06/14/2022
 Supervised By :Mahesh Dadoda 06/15/2022

Quant Time: Jun 14 01:35:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jun 14 01:31:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	349252	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	327364	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	148537	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	112406	20.259	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	81.040%		
7) Chloroethane-d5	2.879	69	81161	19.899	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	79.600%		
11) 1,1-Dichloroethene-d2	4.013	63	108695	14.035	ug/L	-0.01
Spiked Amount 25.000	Range 45 - 110		Recovery =	56.120%		
21) 2-Butanone-d5	7.074	46	67405	59.499	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	119.000%		
24) Chloroform-d	7.647	84	195856	20.372	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	81.480%		
26) 1,2-Dichloroethane-d4	8.305	65	115817m	22.368	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	89.480%		
32) Benzene-d6	8.275	84	358803	20.671	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	82.680%		
36) 1,2-Dichloropropane-d6	9.275	67	110646	21.636	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	86.560%		
41) Toluene-d8	10.323	98	328540	19.378	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	77.520%		
43) trans-1,3-Dichloroprop...	10.579	79	45302	19.409	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	77.640%		
47) 2-Hexanone-d5	10.927	63	50348	61.614	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	123.220%		
56) 1,1,2,2-Tetrachloroeth...	12.689	84	119176	24.952	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	99.800%		
66) 1,2-Dichlorobenzene-d4	13.853	152	116873	21.796	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	87.200%		
Target Compounds					Qvalue	
13) Acetone	4.123	43	4053m	4.966	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061322\
Data File : VW023479.D
Acq On : 13 Jun 2022 14:48
Operator : SY/VA
Sample : N3256-11
Misc : 5.77g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
C0AF5

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 06/14/2022
Supervised By :Mahesh Dadoda 06/15/2022


Quant Time: Jun 14 01:35:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jun 14 01:31:49 2022
Response via : Initial Calibration

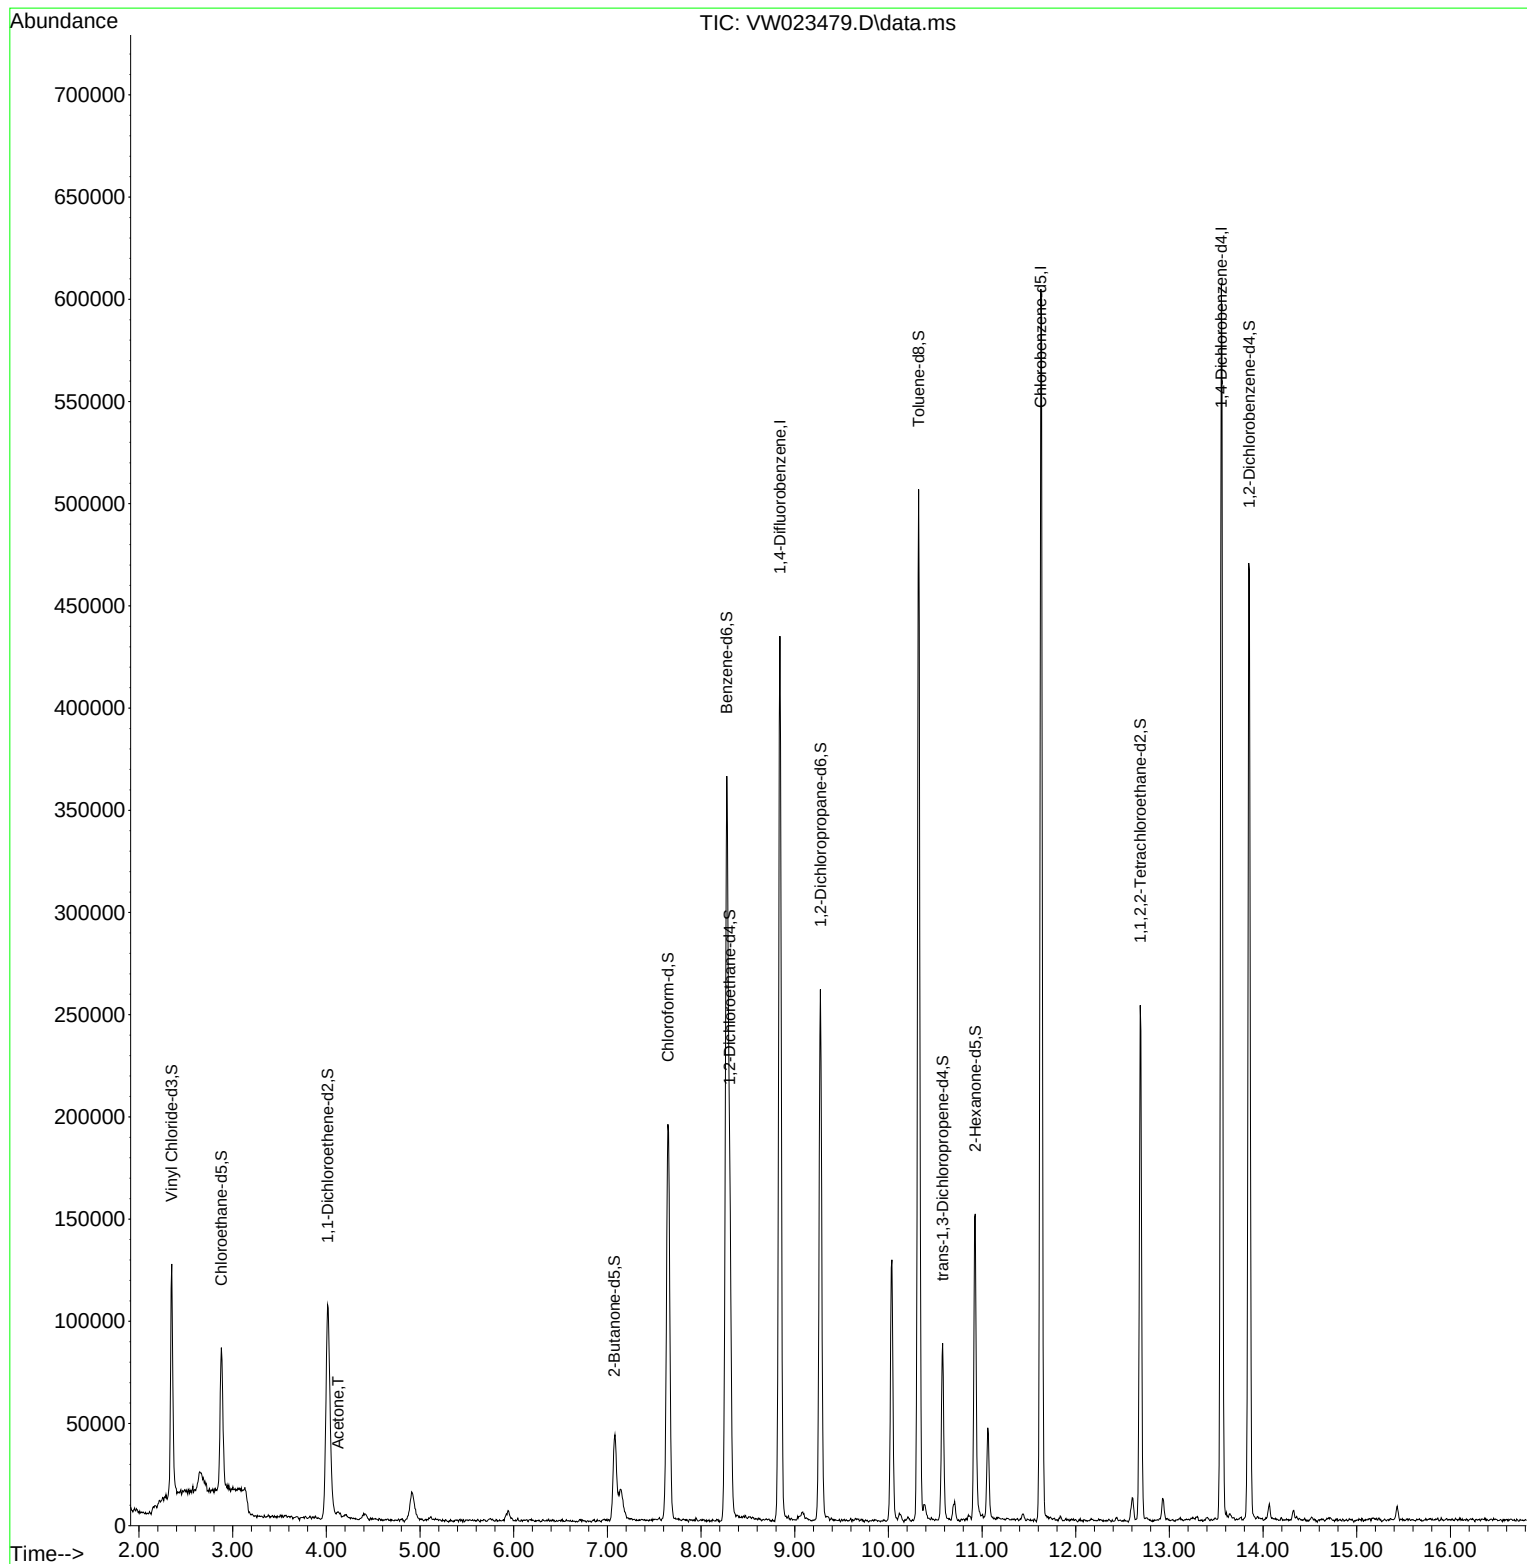

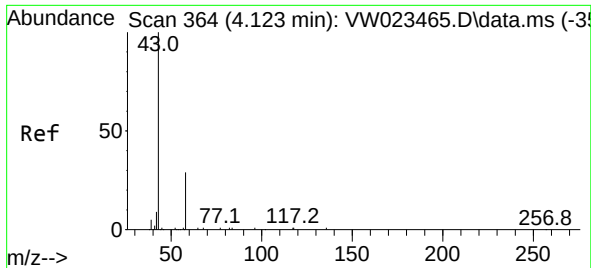

#13
 Acetone
 Concen: 4.966 ug/L m
 RT: 4.123 min Scan# 30
 Delta R.T. -0.000 min
 Lab File: VW023479.D
 Acq: 13 Jun 2022 14:48

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AF5

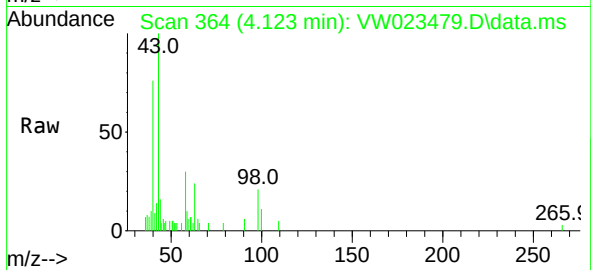

Tgt Ion: 43 Resp: 405
 Ion Ratio Lower Upper
 43 100
 58 17.0 0.0 64.0

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 06/14/2022
 Supervised By :Mahesh Dadoda 06/15/2022

