

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061324\
 Data File : VW029128.D
 Acq On : 13 Jun 2024 16:29
 Operator : SY/MD
 Sample : P2844-16
 Misc : 5.28g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Jun 14 05:23:20 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 14 05:21:04 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	406329	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	309008	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	95594	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	135235	20.950	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.800%
7) Chloroethane-d5	2.899	69	119885	24.186	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	96.760%
11) 1,1-Dichloroethene-d2	4.021	65	60548	21.341	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	85.360%
21) 2-Butanone-d5	7.075	46	80928	61.362	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	122.720%
24) Chloroform-d	7.648	84	283643	24.468	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	97.880%
26) 1,2-Dichloroethane-d4	8.398	65	193	0.032	ug/L	0.09
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.120%#
32) Benzene-d6	8.276	84	537317	28.330	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	113.320%
36) 1,2-Dichloropropane-d6	9.270	67	177575	30.880	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	123.520%#
41) Toluene-d8	10.319	98	424557	25.085	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	100.320%
43) trans-1,3-Dichloroprop...	10.575	79	55356	25.052	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	100.200%
47) 2-Hexanone-d5	10.922	63	41011	54.043	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	108.080%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	119340	29.873	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	119.480%
66) 1,2-Dichlorobenzene-d4	13.848	152	83113	24.501	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.000%
Target Compounds						Qvalue
16) Methylene chloride	4.917	84	13374	2.193	ug/L	96
48) 2-Hexanone	10.922	43	6491	3.383	ug/L #	70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061324\
Data File : VW029128.D
Acq On : 13 Jun 2024 16:29
Operator : SY/MD
Sample : P2844-16
Misc : 5.28g/10mL/MSVOA_W/SOIL/A
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Jun 14 05:23:20 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 14 05:21:04 2024
Response via : Initial Calibration

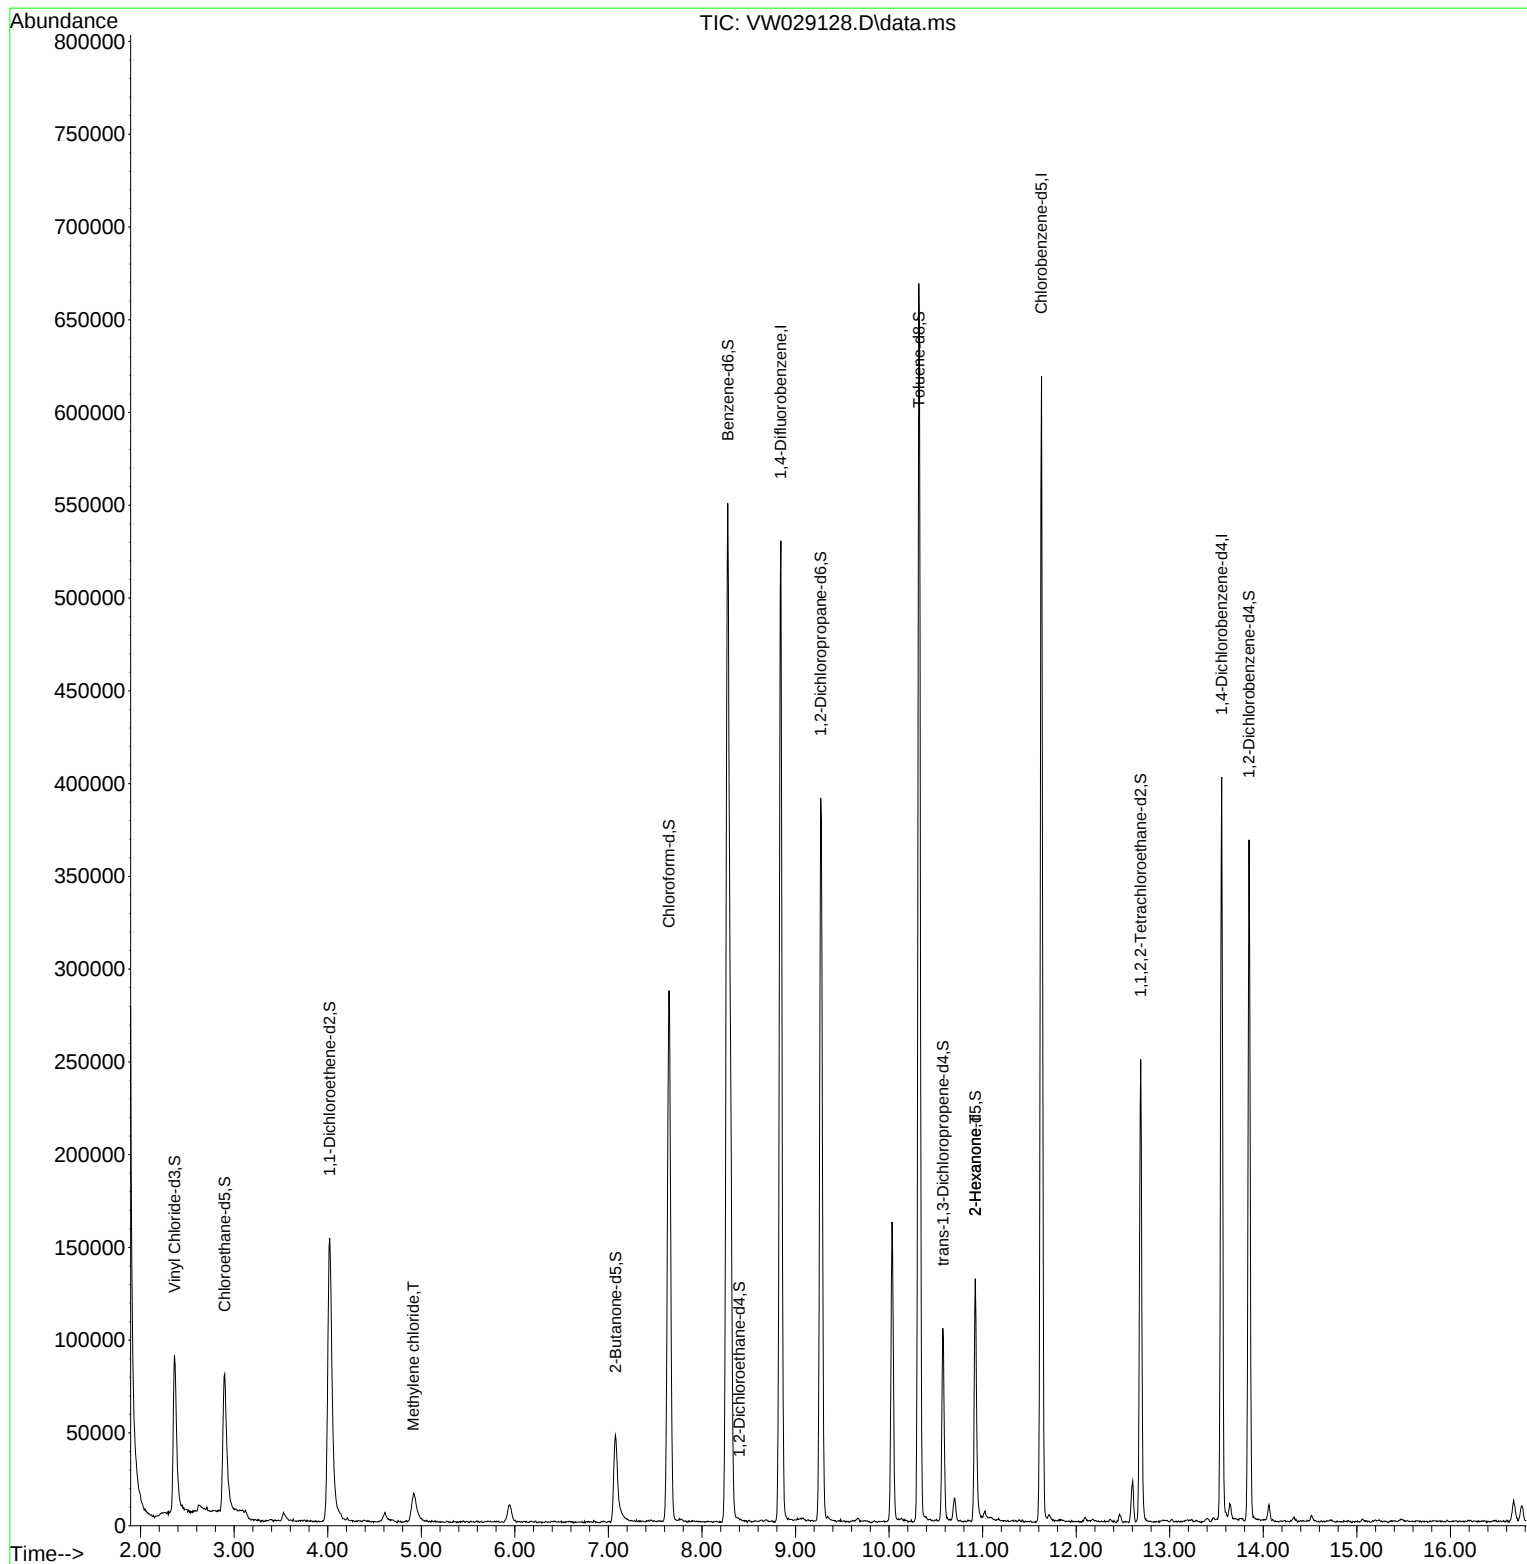

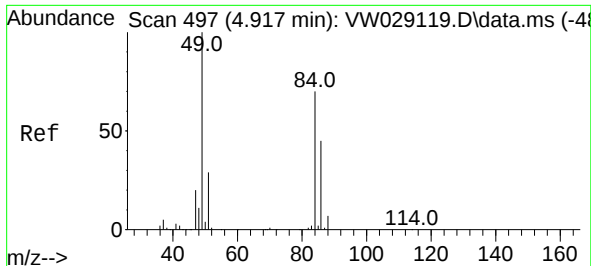

#16

Methylene chloride

Concen: 2.193 ug/L

RT: 4.917 min Scan# 497

Delta R.T. 0.000 min

Lab File: VW029128.D

Acq: 13 Jun 2024 16:29

Instrument :

MSVOA_W

ClientSampleId :





Tgt Ion: 84 Resp: 13374

Ion Ratio Lower Upper

84 100

86 61.3 43.8 81.4

49 136.1 91.3 169.5

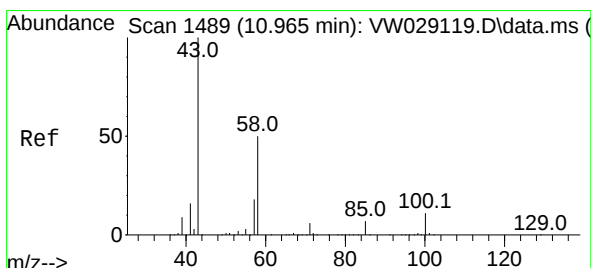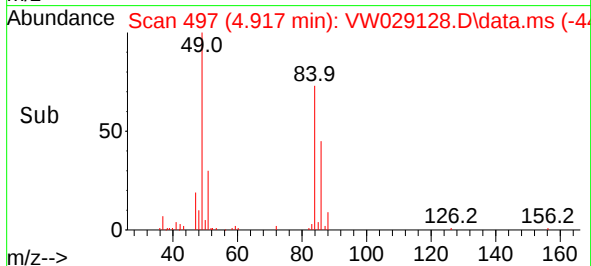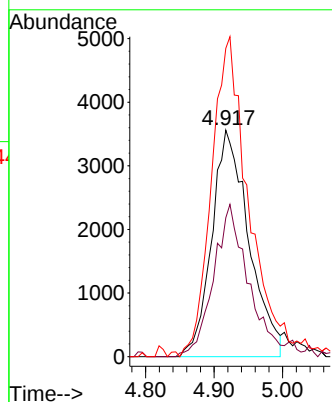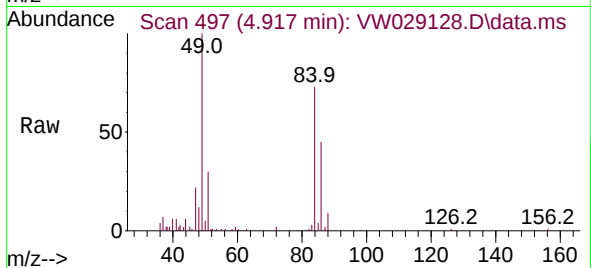

#48

2-Hexanone

Concen: 3.383 ug/L

RT: 10.922 min Scan# 1482

Delta R.T. -0.043 min

Lab File: VW029128.D

Acq: 13 Jun 2024 16:29

Tgt Ion: 43 Resp: 6491

Ion Ratio Lower Upper

43 100

58 29.0 41.4 62.0#

57 31.3 14.2 21.4#

100 4.5 9.1 13.7#

