




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061324\
 Data File : VW029120.D
 Acq On : 13 Jun 2024 13:03
 Operator : SY/MD
 Sample : VW0613SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK503

Manual IntegrationsAPPROVED

Quant Time: Jun 14 05:21:38 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 14 05:21:04 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/14/2024
 Supervised By :Mahesh Dadoda 06/20/2024

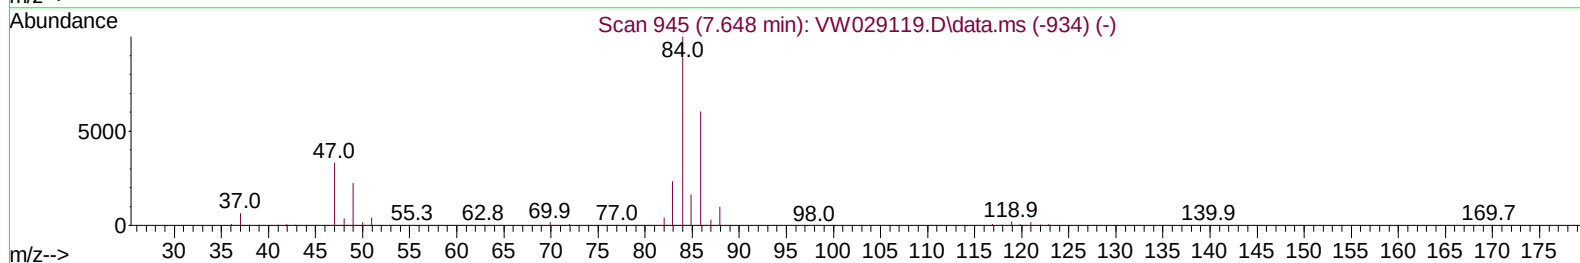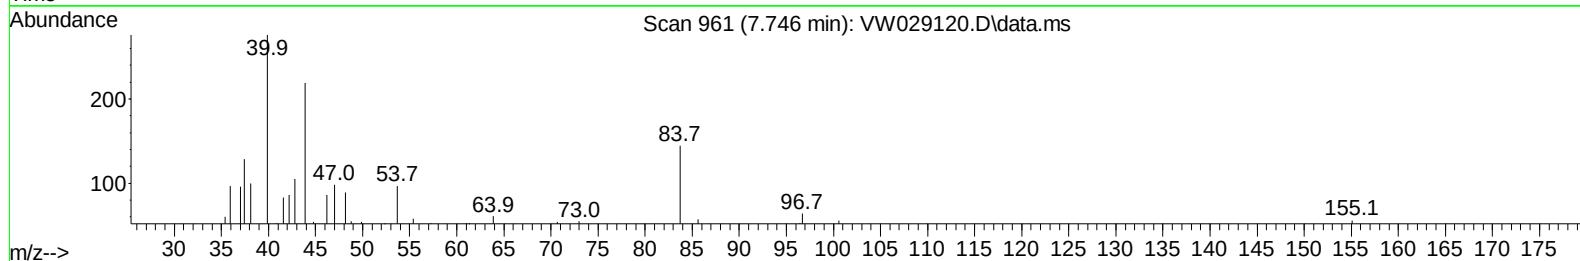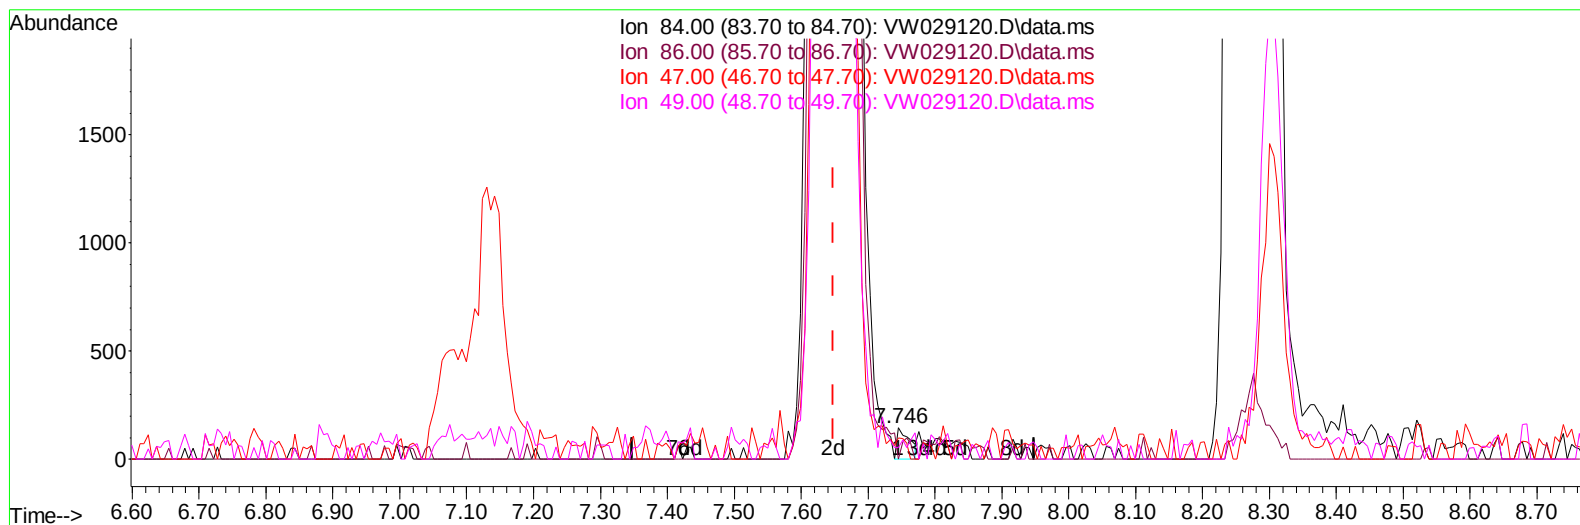

TIC: VW029120.D\data.ms

(24) Chloroform-d (S)

7.746min (+ 0.097) 0.02 ug/L

response 190

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	63.10	48.95
47.00	46.00	52.11
49.00	27.00	27.89




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061324\
 Data File : VW029120.D
 Acq On : 13 Jun 2024 13:03
 Operator : SY/MD
 Sample : VW0613SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK503

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/14/2024
 Supervised By :Mahesh Dadoda 06/20/2024

Quant Time: Jun 14 05:21:38 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 14 05:21:04 2024
 Response via : Initial Calibration

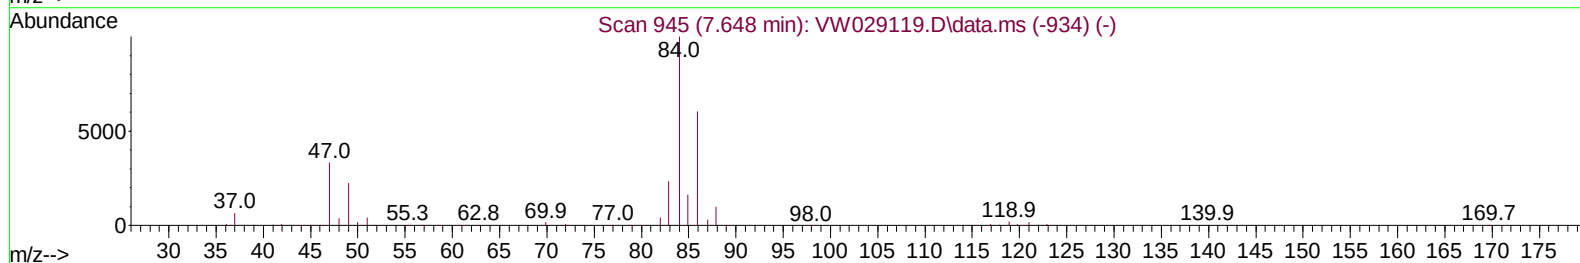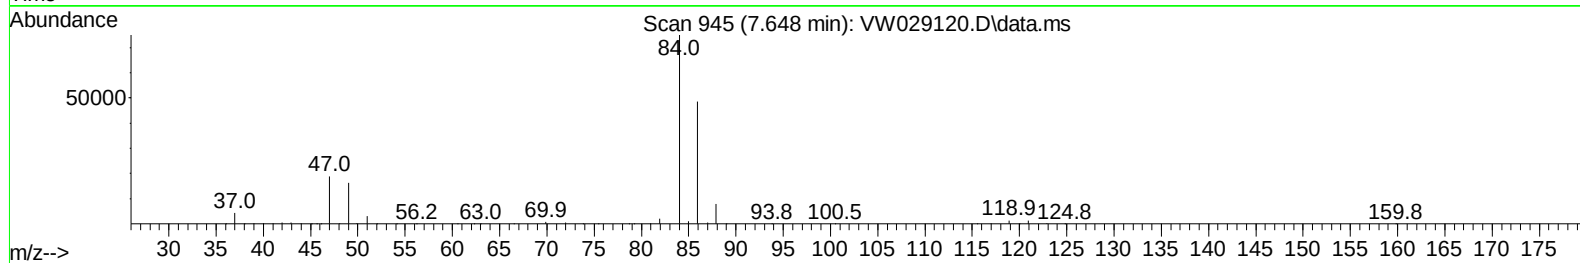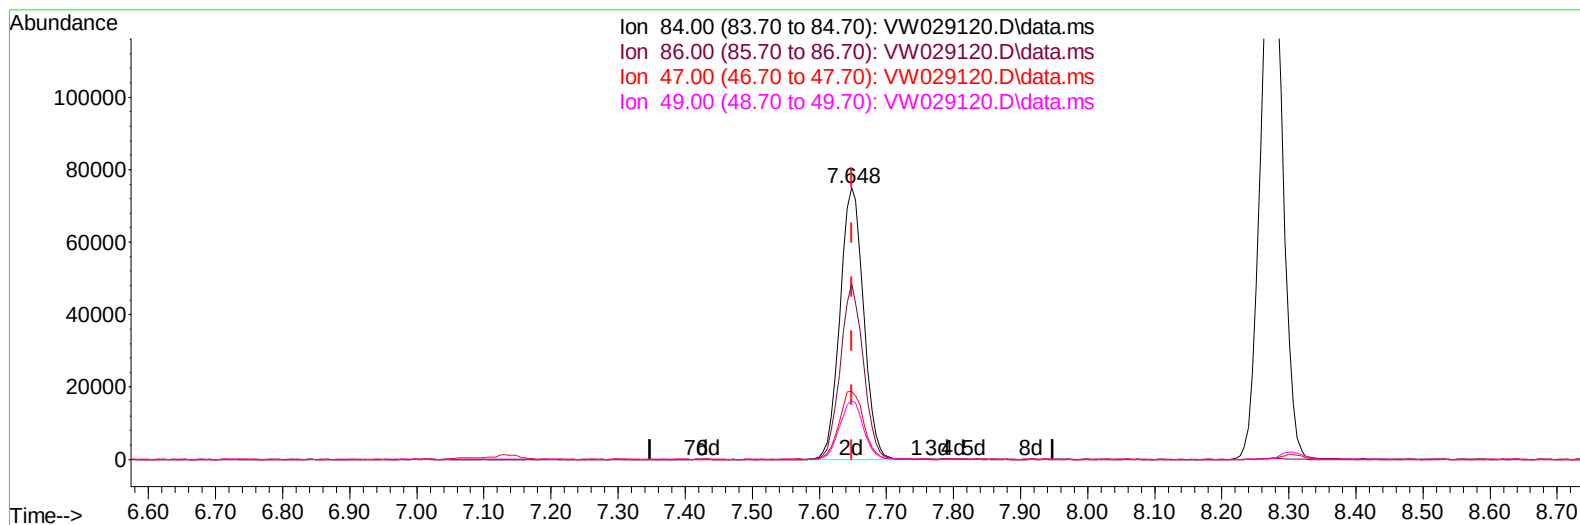

TIC: VW029120.D\data.ms

(24) Chloroform-d (S)

7.648min (-0.000) 24.02 ug/L m

response 183136

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	63.10	0.05#
47.00	46.00	0.05#
49.00	27.00	0.03#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061324\
 Data File : VW029120.D
 Acq On : 13 Jun 2024 13:03
 Operator : SY/MD
 Sample : VW0613SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK503

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/14/2024
 Supervised By :Mahesh Dadoda 06/20/2024

Quant Time: Jun 14 05:21:38 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 14 05:21:04 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		267247	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		261220	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		115201	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.362	65		86061	20.271	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.080%	
7) Chloroethane-d5	2.893	69		72082	22.110	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.440%	
11) 1,1-Dichloroethene-d2	4.021	65		38085	20.410	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	81.640%	
21) 2-Butanone-d5	7.075	46		49904	57.530	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	115.060%	
24) Chloroform-d	7.648	84		183136m	24.020	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	96.080%	
26) 1,2-Dichloroethane-d4	8.306	65		106897	26.631	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	106.520%	
32) Benzene-d6	8.276	84		346496	21.611	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	86.440%	
36) 1,2-Dichloropropane-d6	9.270	67		112449	23.132	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	92.520%	
41) Toluene-d8	10.324	98		292647	20.454	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	81.800%	
43) trans-1,3-Dichloroprop...	10.574	79		40225	21.534	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	86.120%	
47) 2-Hexanone-d5	10.922	63		33148	51.673	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.340%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		87246	25.835	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	103.320%	
66) 1,2-Dichlorobenzene-d4	13.848	152		98346	24.057	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	96.240%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061324\
Data File : VW029120.D
Acq On : 13 Jun 2024 13:03
Operator : SY/MD
Sample : VW0613SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK503

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/14/2024
Supervised By :Mahesh Dadoda 06/20/2024

Quant Time: Jun 14 05:21:38 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 14 05:21:04 2024
Response via : Initial Calibration

