




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061324\
Data File : VW029142.D
Acq On : 13 Jun 2024 22:06
Operator : SY/MD
Sample : P2870-15
Misc : 3.61g/10mL/MSVOA_W/SOIL/A
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AB6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/14/2024
Supervised By :Mahesh Dadoda 06/20/2024

Quant Time: Jun 14 05:26:38 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 14 05:21:04 2024
Response via : Initial Calibration

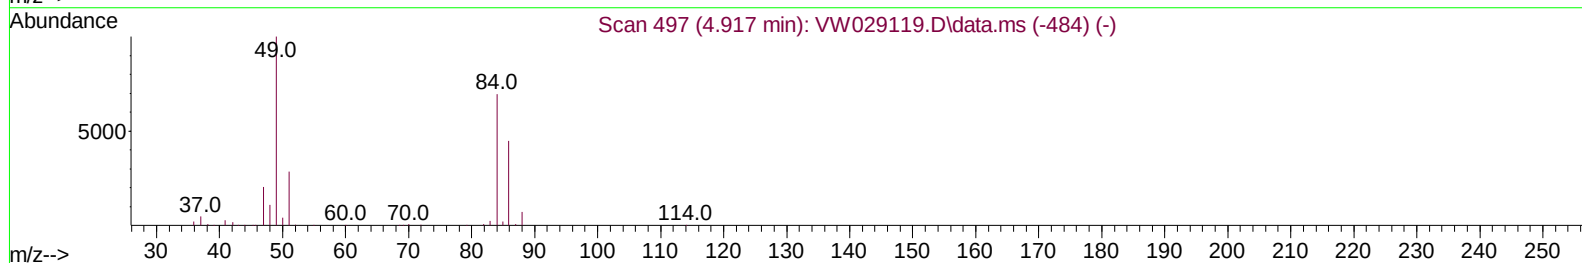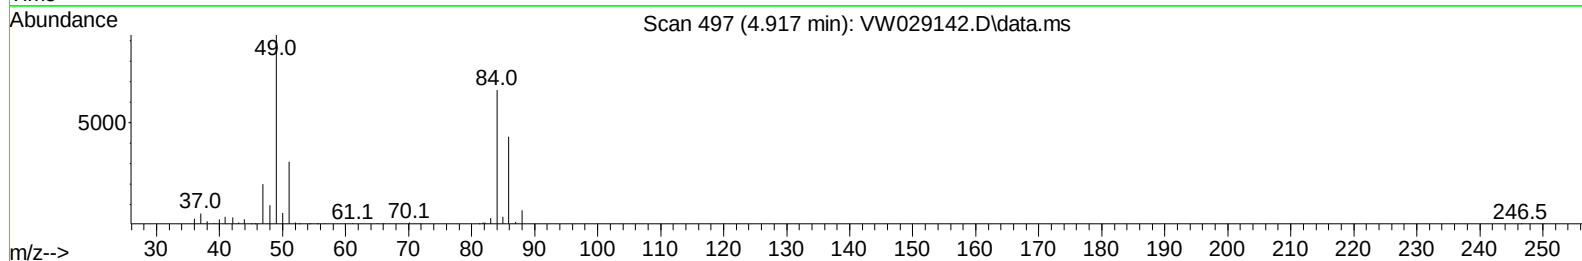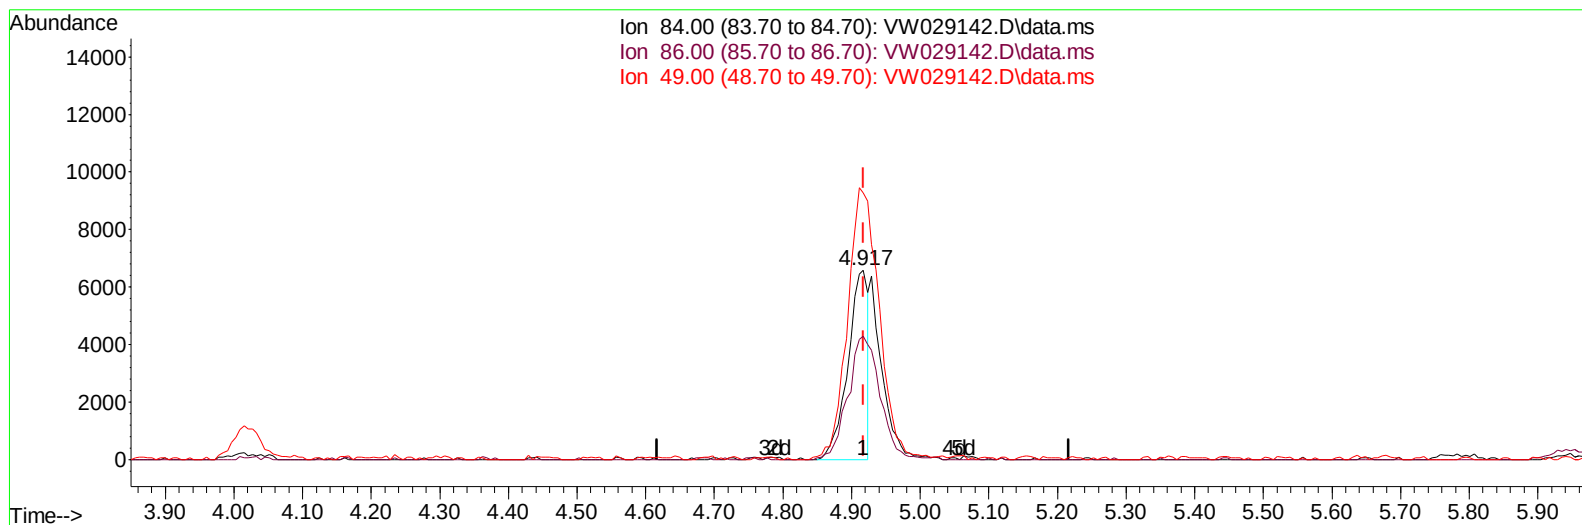

TIC: VW029142.D\data.ms

(16) Methylene chloride (T)

4.917min (+ 0.000) 4.29 ug/L

response 13293

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.60	65.12
49.00	130.40	140.71
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061324\
 Data File : VW029142.D
 Acq On : 13 Jun 2024 22:06
 Operator : SY/MD
 Sample : P2870-15
 Misc : 3.61g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AB6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/14/2024
 Supervised By :Mahesh Dadoda 06/20/2024

Quant Time: Jun 14 05:26:38 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 14 05:21:04 2024
 Response via : Initial Calibration

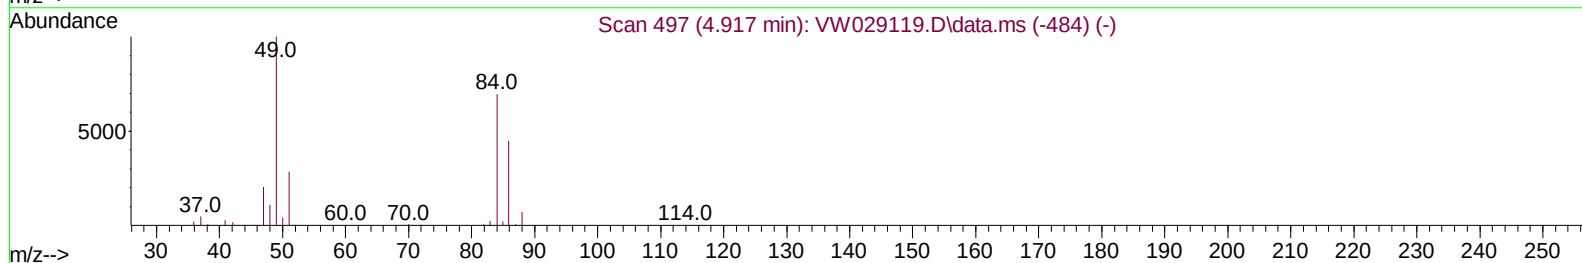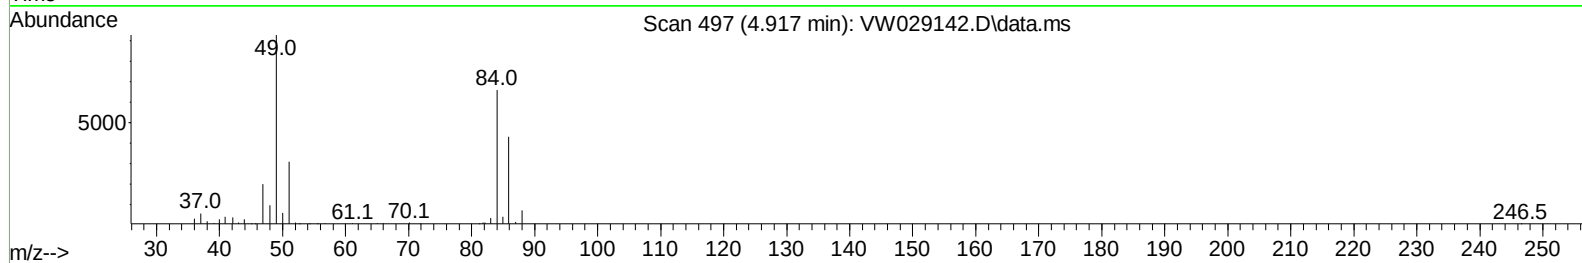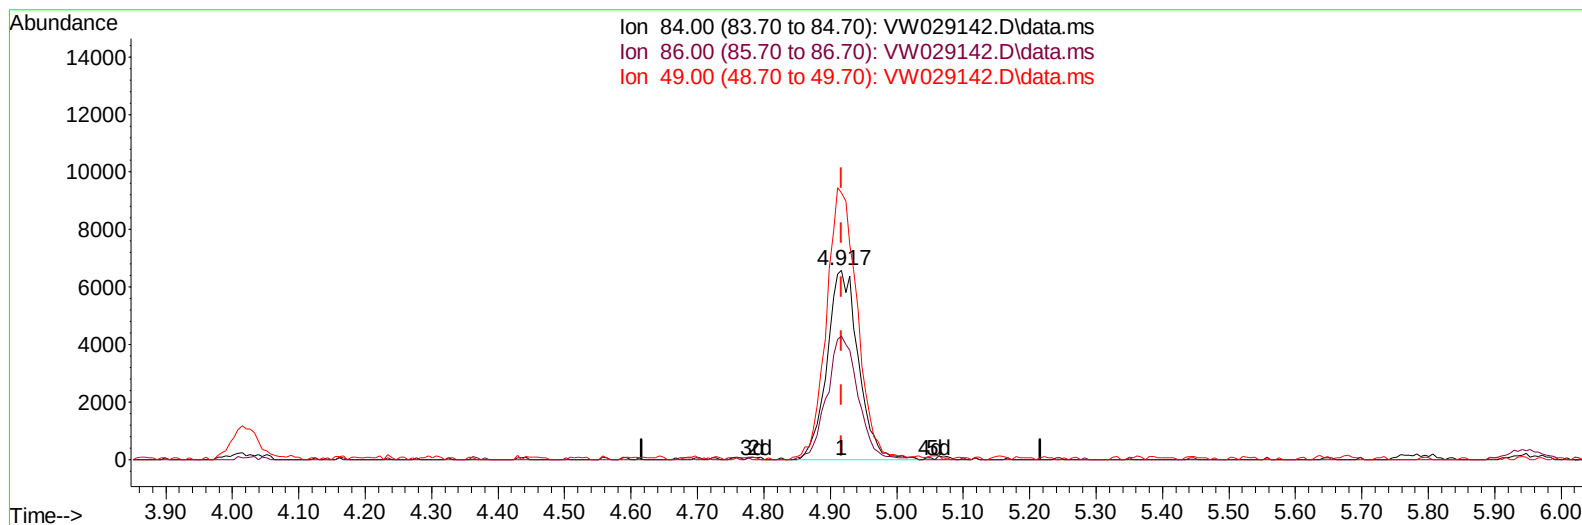

TIC: VW029142.D\data.ms

(16) Methylene chloride (T)

4.917min (+ 0.000) 6.93 ug/L m

response 21475

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.60	65.12
49.00	130.40	140.71
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061324\
 Data File : VW029142.D
 Acq On : 13 Jun 2024 22:06
 Operator : SY/MD
 Sample : P2870-15
 Misc : 3.61g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AB6

Manual IntegrationsAPPROVED

Quant Time: Jun 14 05:26:38 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 14 05:21:04 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/14/2024
 Supervised By :Mahesh Dadoda 06/20/2024

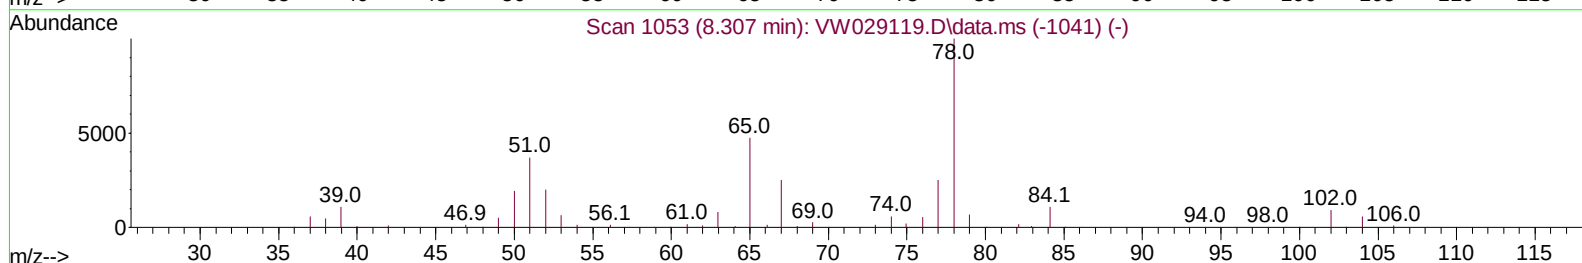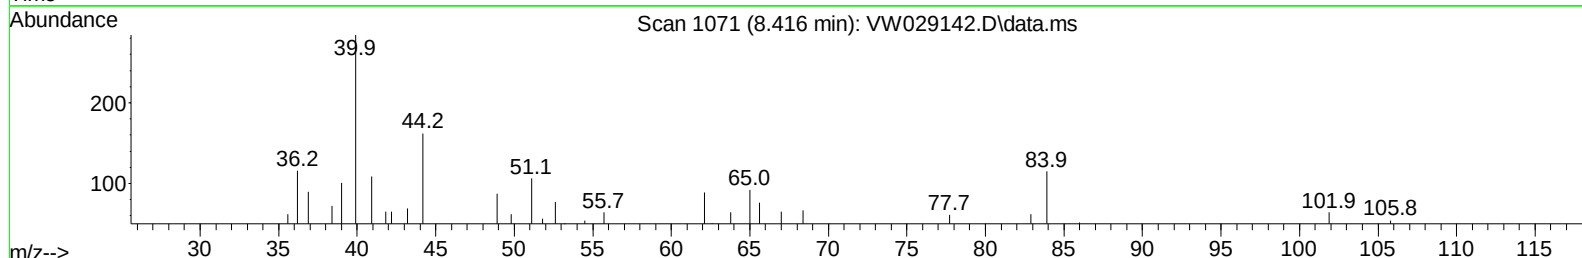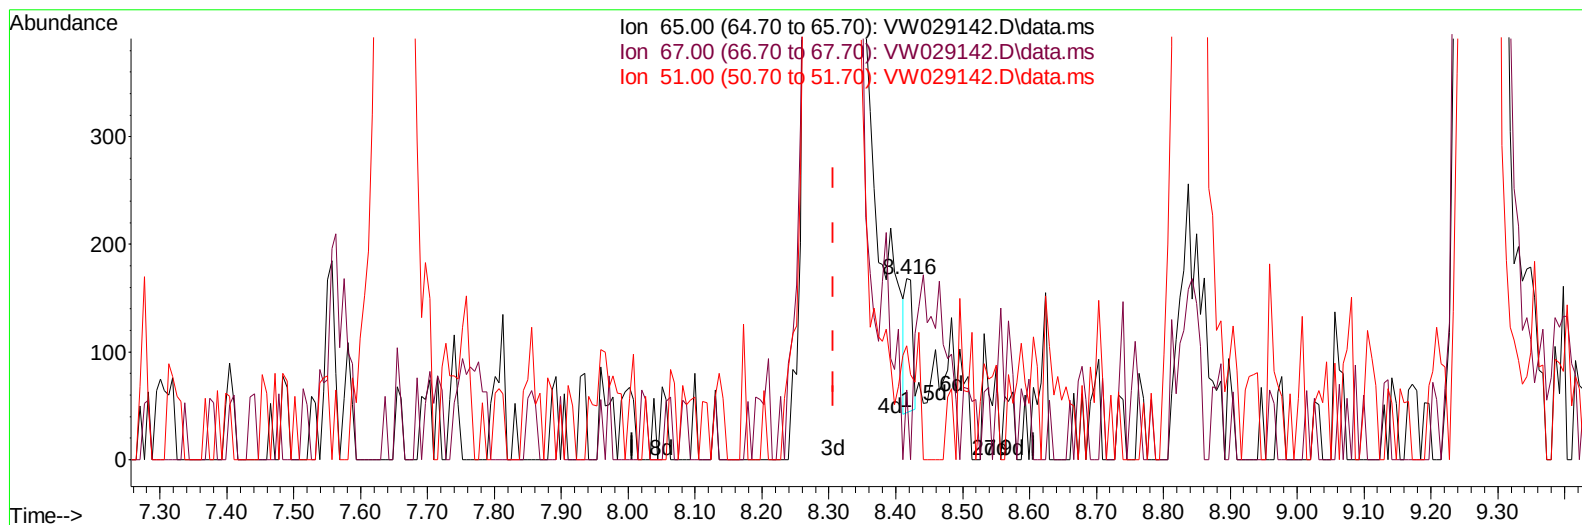

TIC: VW029142.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.416min (+ 0.110) 0.03 ug/L

response 95

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.90	46.32
51.00	105.10	98.95
0.00	0.00	0.00


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061324\
 Data File : VW029142.D
 Acq On : 13 Jun 2024 22:06
 Operator : SY/MD
 Sample : P2870-15
 Misc : 3.61g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AB6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/14/2024
 Supervised By :Mahesh Dadoda 06/20/2024

Quant Time: Jun 14 05:26:38 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 14 05:21:04 2024
 Response via : Initial Calibration

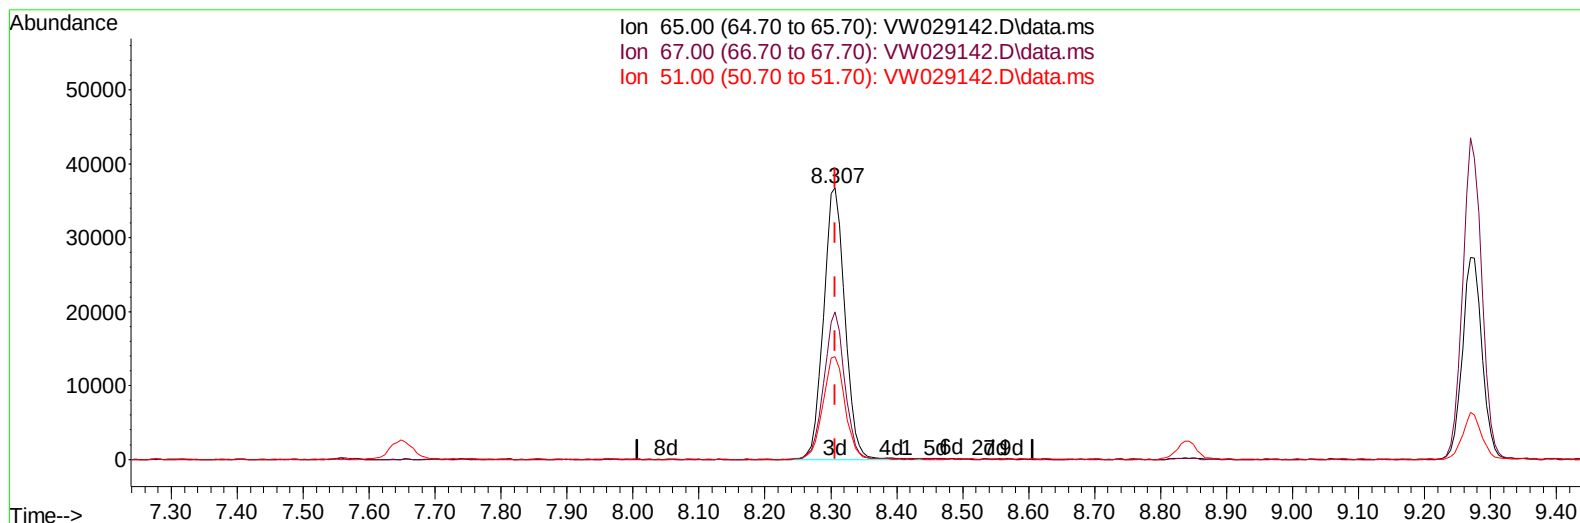

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061324\
 Data File : VW029142.D
 Acq On : 13 Jun 2024 22:06
 Operator : SY/MD
 Sample : P2870-15
 Misc : 3.61g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AB6

Manual IntegrationsAPPROVED

Quant Time: Jun 14 05:26:38 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 14 05:21:04 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/14/2024
 Supervised By :Mahesh Dadoda 06/20/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		206469	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		160174	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		43845	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.357	65		69061	21.055	ug/L	-0.01
Spiked Amount 25.000	Range 30	- 150		Recovery	=	84.200%	
7) Chloroethane-d5	2.899	69		60798	24.138	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	96.560%	
11) 1,1-Dichloroethene-d2	4.021	65		30105	20.882	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	83.520%	
21) 2-Butanone-d5	7.075	46		22033	32.877	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	65.760%	
24) Chloroform-d	7.648	84		140692	23.885	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	95.560%	
26) 1,2-Dichloroethane-d4	8.307	65		82877m	26.725	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	106.920%	
32) Benzene-d6	8.270	84		269003	27.363	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	109.440%	
36) 1,2-Dichloropropane-d6	9.270	67		87875	29.481	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	117.920%	
41) Toluene-d8	10.319	98		207064	23.602	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	94.400%	
43) trans-1,3-Dichloroprop...	10.581	79		18601	16.240	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	64.960%	
47) 2-Hexanone-d5	10.922	63		8278	21.045	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	42.080%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		51209	24.730	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	98.920%	
66) 1,2-Dichlorobenzene-d4	13.848	152		36316	23.341	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	93.360%	
Target Compounds							
13) Acetone	4.131	43		7844	11.169	ug/L	92
16) Methylene chloride	4.917	84		21475m	6.930	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061324\
Data File : VW029142.D
Acq On : 13 Jun 2024 22:06
Operator : SY/MD
Sample : P2870-15
Misc : 3.61g/10mL/MSVOA_W/SOIL/A
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AB6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/14/2024
Supervised By :Mahesh Dadoda 06/20/2024

Quant Time: Jun 14 05:26:38 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 14 05:21:04 2024
Response via : Initial Calibration

