

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061422\
 Data File : VW023483.D
 Acq On : 14 Jun 2022 10:45
 Operator : SY/VA
 Sample : VW0614SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK528

Quant Time: Jun 15 02:15:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 15 02:14:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	373889	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	349136	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	158935	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	134985	22.725	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.880%
7) Chloroethane-d5	2.885	69	97602	22.353	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.400%
11) 1,1-Dichloroethene-d2	4.019	63	142643	17.204	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	68.800%
21) 2-Butanone-d5	7.080	46	61472	50.686	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	101.380%
24) Chloroform-d	7.653	84	240674	23.384	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.520%
26) 1,2-Dichloroethane-d4	8.305	65	130216	23.491	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	93.960%
32) Benzene-d6	8.275	84	450810	24.352	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	97.400%
36) 1,2-Dichloropropane-d6	9.274	67	135654	24.872	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	99.480%
41) Toluene-d8	10.323	98	427377	23.636	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	94.560%
43) trans-1,3-Dichloroprop...	10.579	79	58042	23.316	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	93.280%
47) 2-Hexanone-d5	10.927	63	45511	52.221	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	104.440%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	120481	23.652	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	94.600%
66) 1,2-Dichlorobenzene-d4	13.853	152	152416	26.565	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	106.240%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.030	75	5278	0.699	ug/L	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061422\
Data File : VW023483.D
Acq On : 14 Jun 2022 10:45
Operator : SY/VA
Sample : VW0614SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK528

Quant Time: Jun 15 02:15:02 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 15 02:14:31 2022
Response via : Initial Calibration

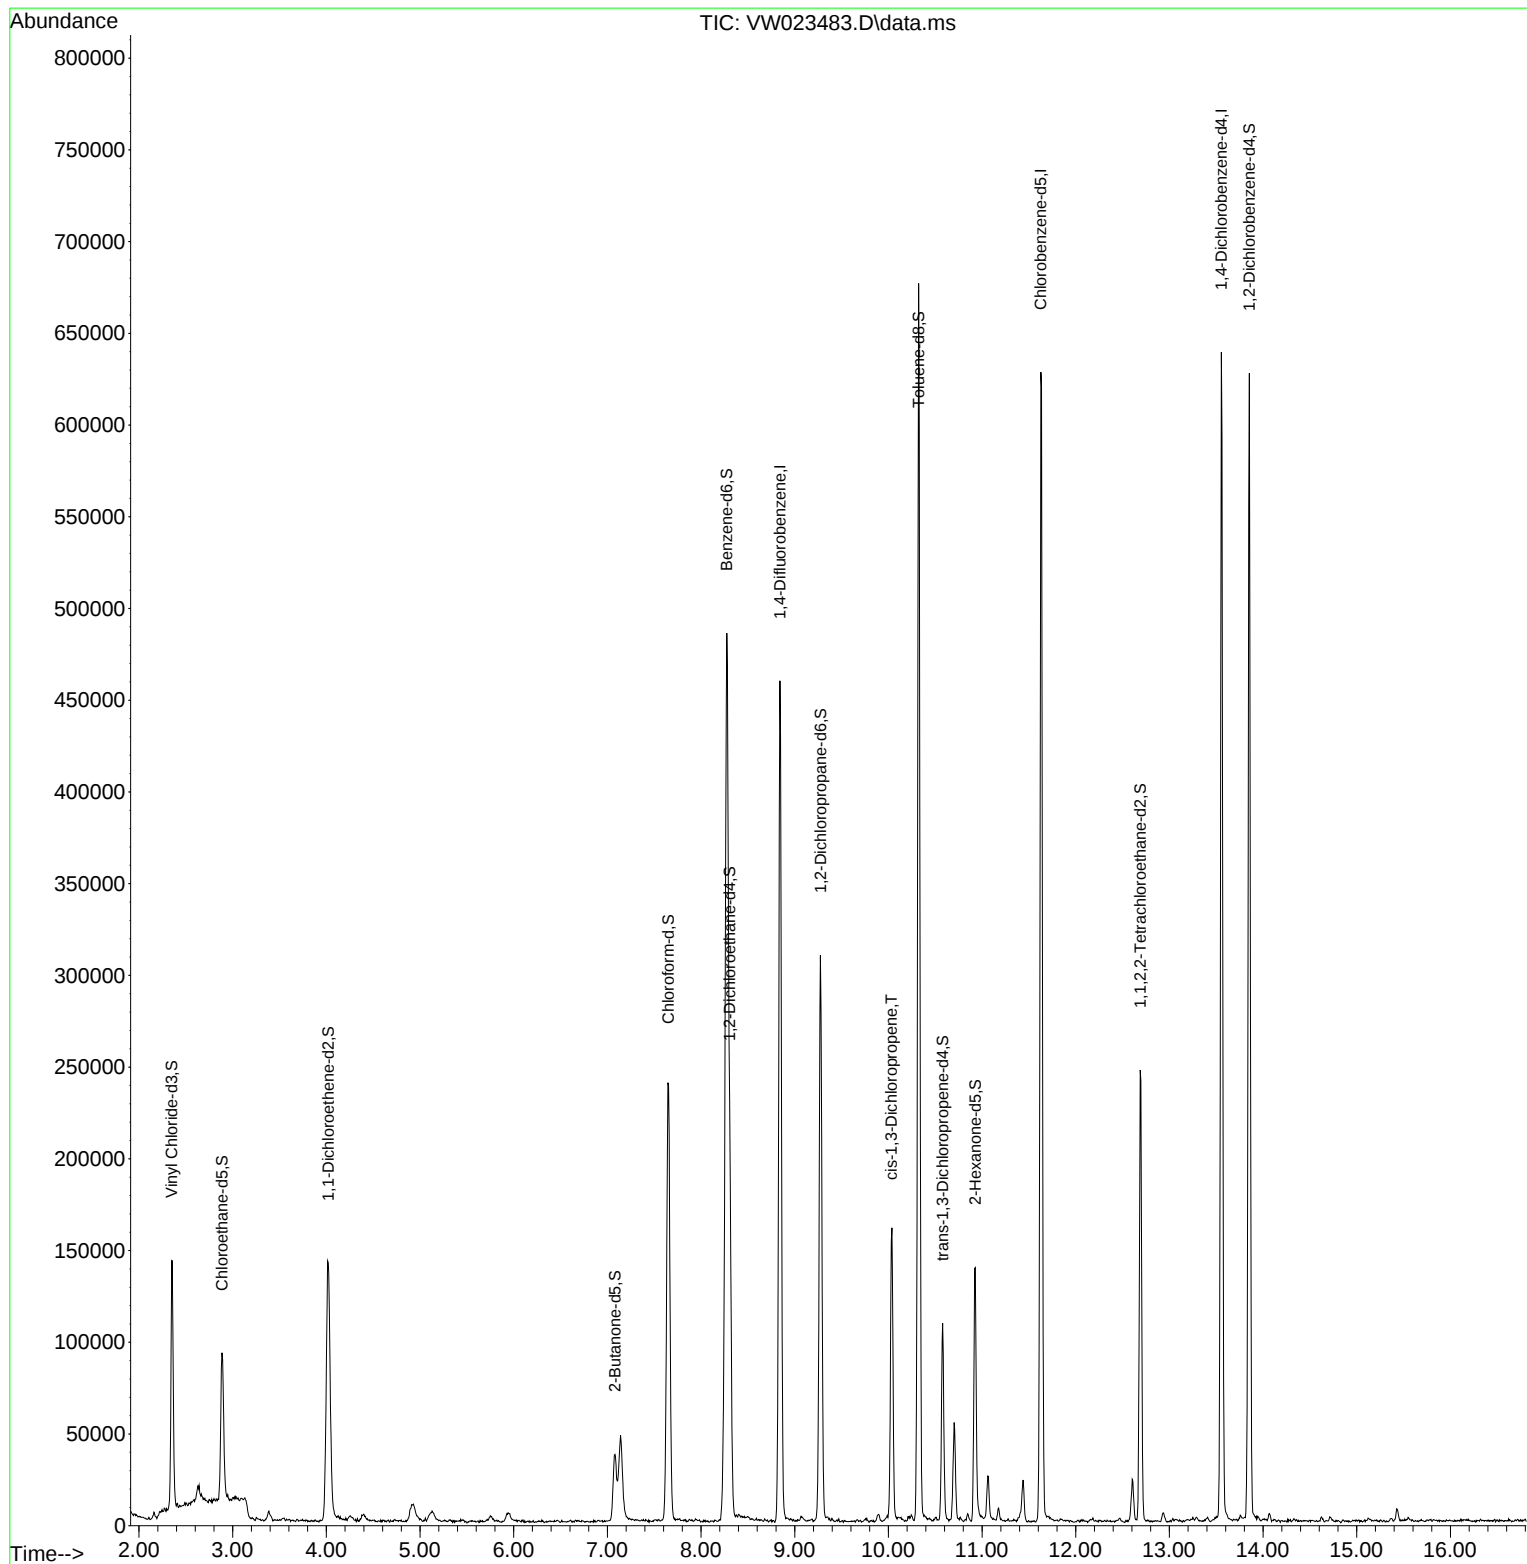

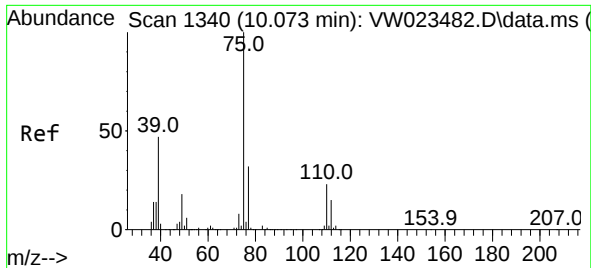

#39

cis-1,3-Dichloropropene

Concen: 0.699 ug/L

RT: 10.030 min Scan# 11

Delta R.T. -0.043 min

Lab File: VW023483.D


Acq: 14 Jun 2022 10:45

Instrument :

MSVOA_W

ClientSampleId :

VBLK528

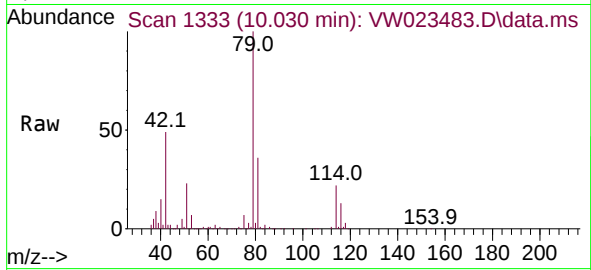

Tgt Ion: 75 Resp: 5278

Ion Ratio Lower Upper

75 100

77 41.0 22.1 41.1

